


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
 Data File : BG040639.D
 Acq On : 26 Apr 2019 22:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

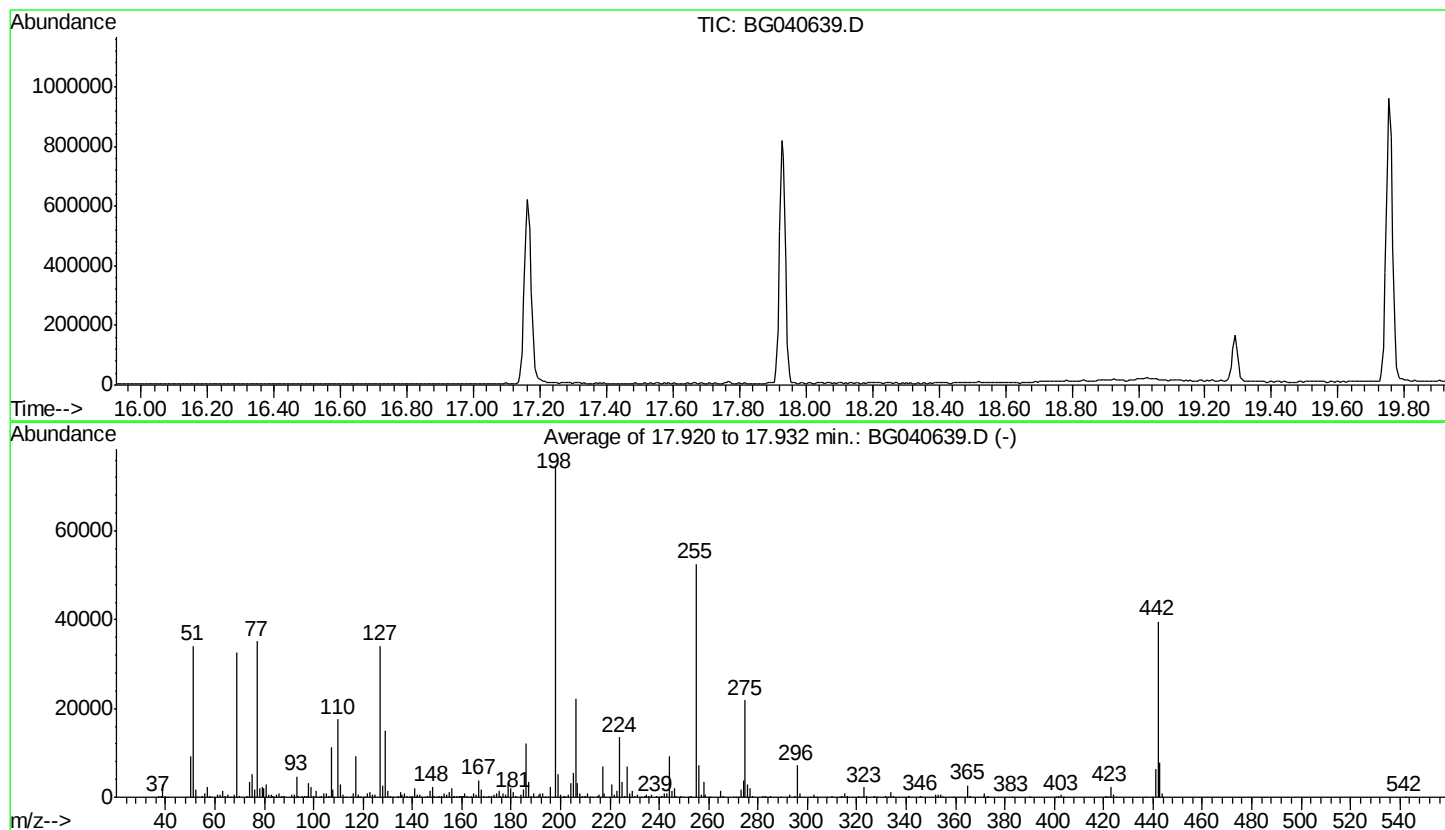

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	34104	PASS
68	69	0.00	2	1.5	486	PASS
69	198	0.00	100	43.7	32658	PASS
70	69	0.00	2	1.0	314	PASS
127	198	10	80	45.6	34082	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74728	PASS
199	198	5	9	6.9	5159	PASS
275	198	10	60	29.3	21858	PASS
365	198	1	100	3.6	2703	PASS
441	198	0.01	100	8.3	6217	PASS
442	198	50	100	52.9	39557	PASS
443	442	15	24	19.9	7854	PASS