
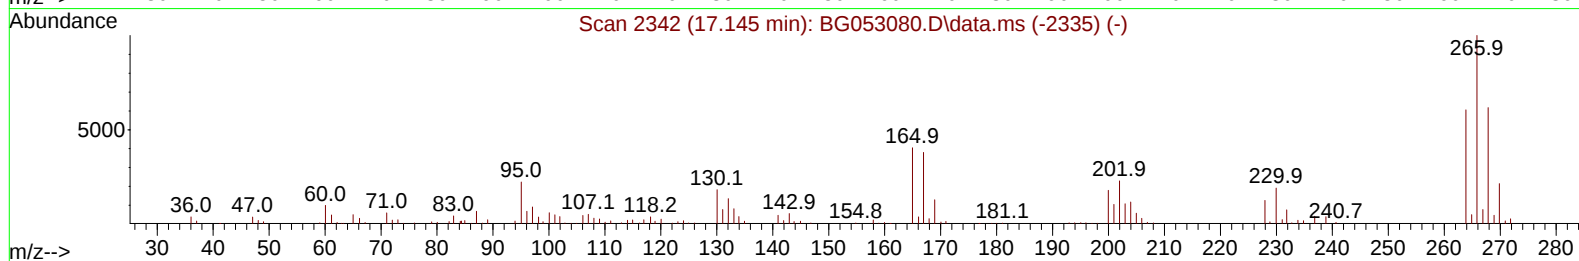
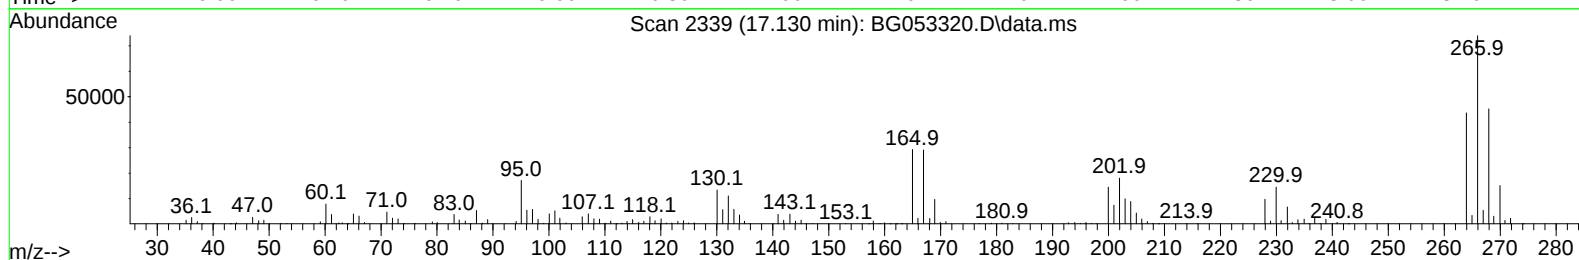


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
Data File : BG053320.D
Acq On : 26 Apr 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 15:21:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

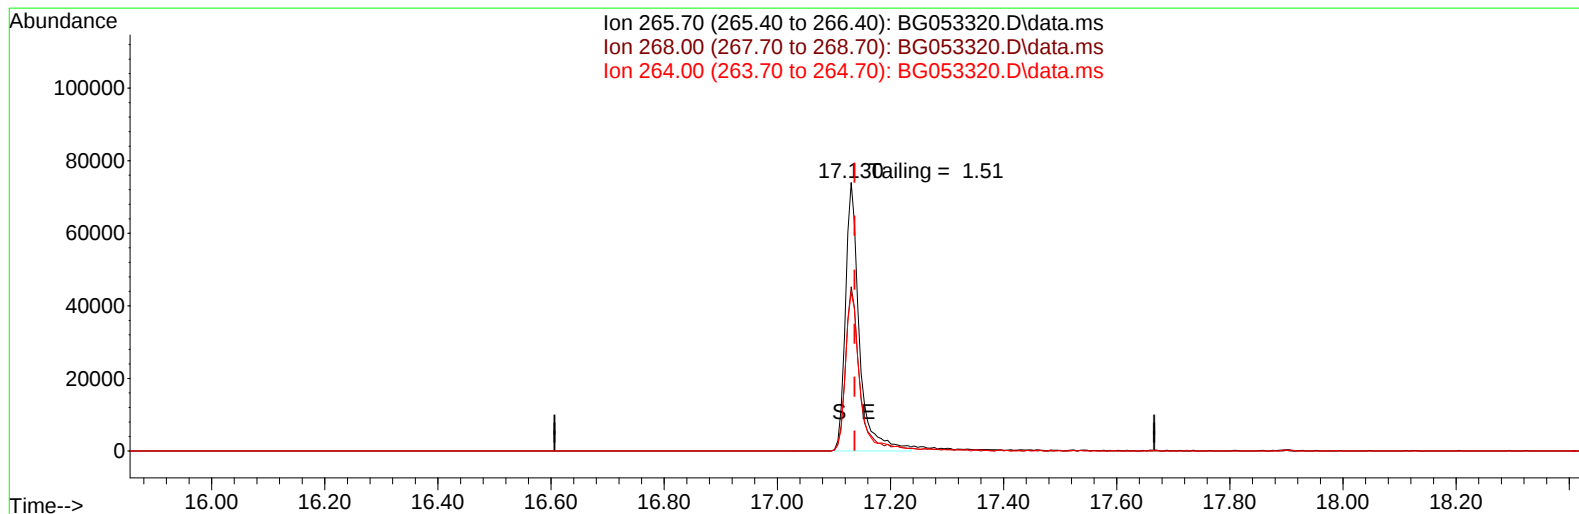

TIC: BG053320.D\data.ms

(70) Pentachlorophenol (C)




17.130min (-0.006) 302564.59 ng

response 130792

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.19
264.00	56.60	59.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
 Data File : BG053320.D
 Acq On : 26 Apr 2022 14:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 15:21:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 01:13:30 2022
 Response via : Initial Calibration

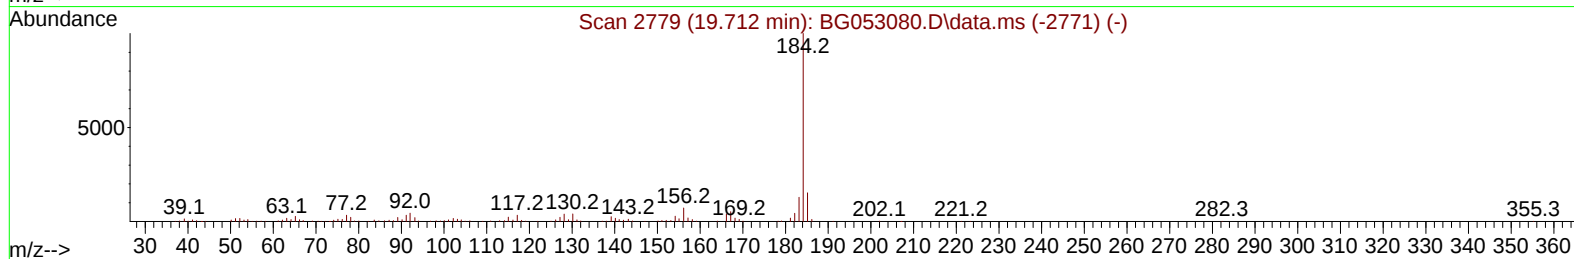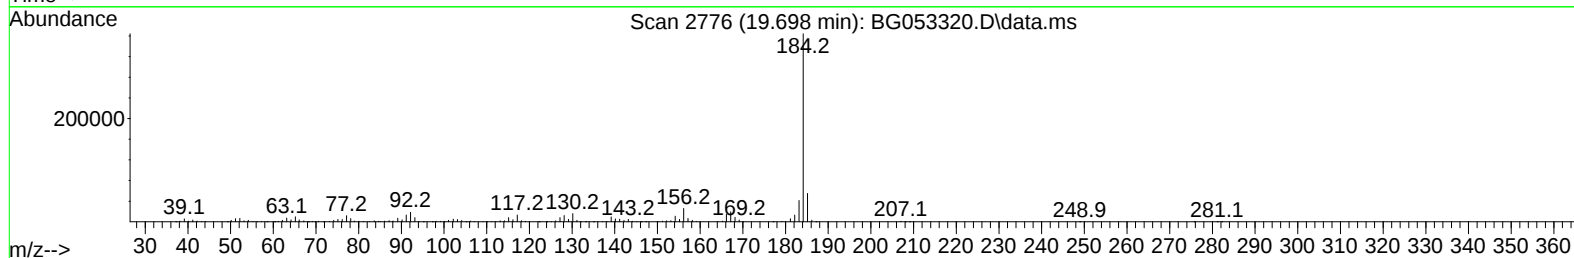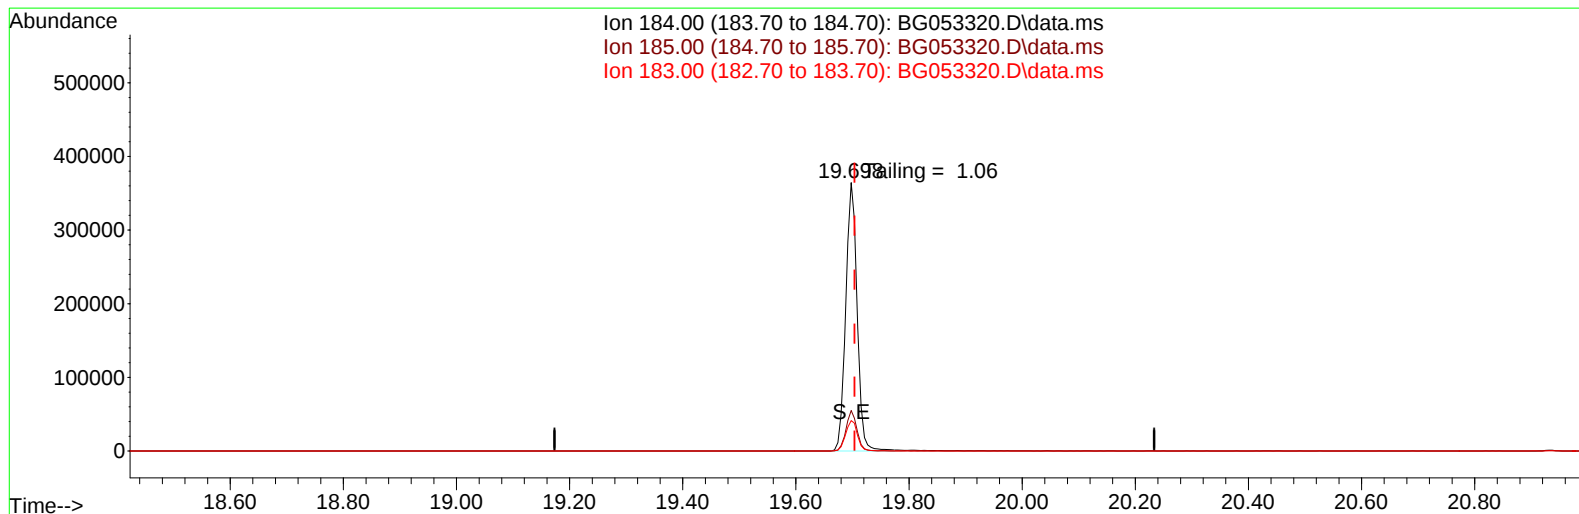

TIC: BG053320.D\data.ms

(77) Benzidine

19.698min (-0.006) 0.00 ng

response 510801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.09
183.00	11.80	11.37
0.00	0.00	0.00