
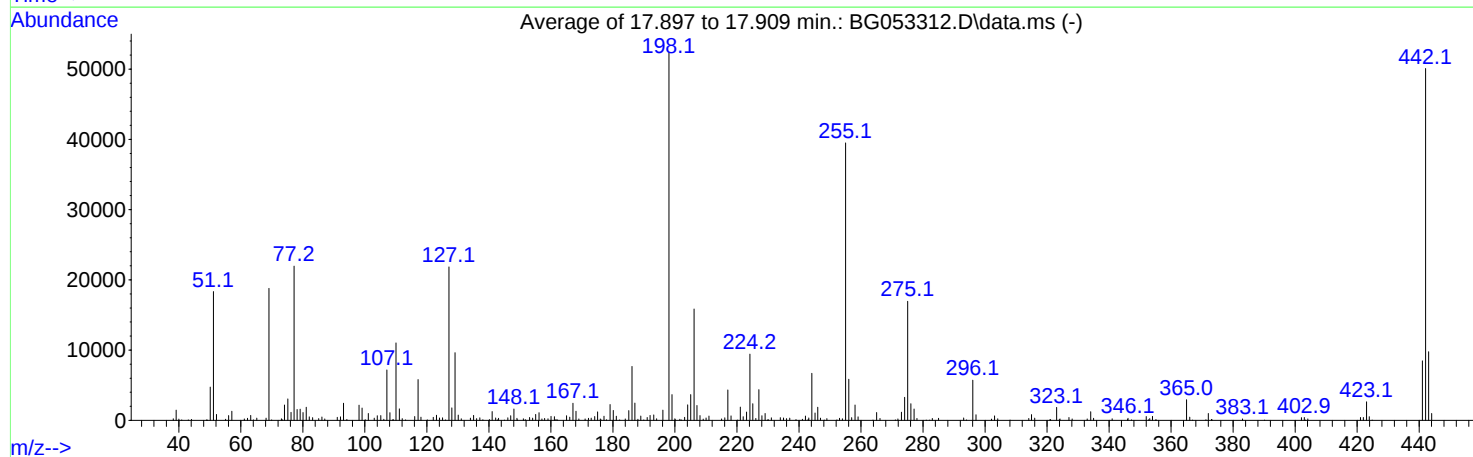


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
 Data File : BG053312.D
 Acq On : 26 Apr 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

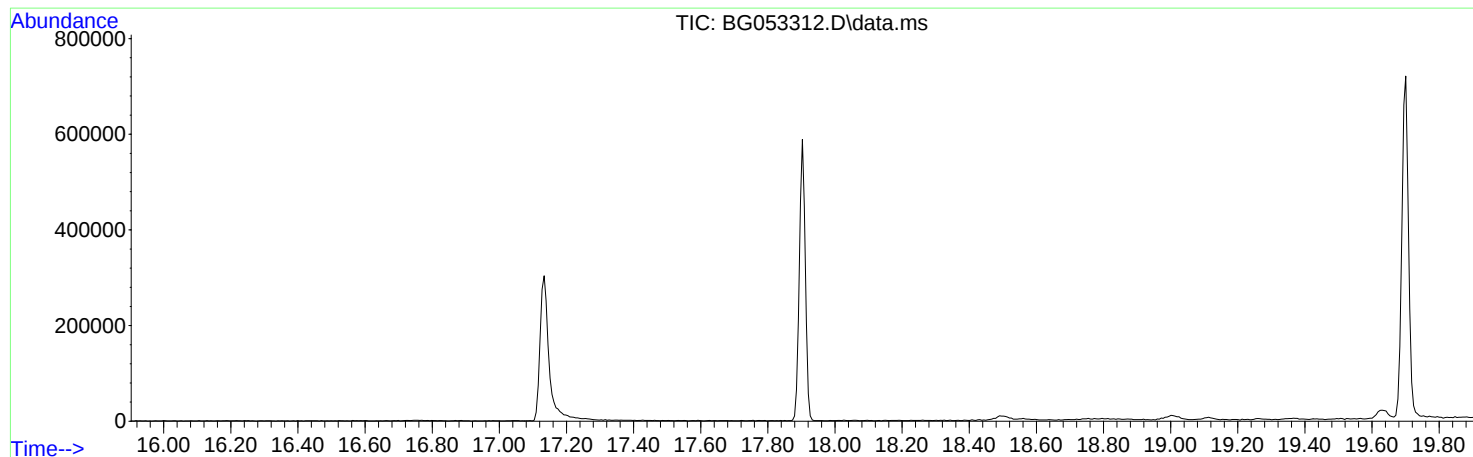




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	18334	PASS
68	69	0.00	2	1.7	317	PASS
69	198	0.00	100	35.9	18793	PASS
70	69	0.00	2	0.4	67	PASS
127	198	10	80	41.7	21851	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52371	PASS
199	198	5	9	7.0	3677	PASS
275	198	10	60	32.4	16950	PASS
365	198	1	100	5.6	2946	PASS
441	198	0.01	100	16.2	8477	PASS
442	442	50	100	100.0	50088	PASS
443	442	15	24	19.5	9763	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
Data File : BG053312.D
Acq On : 26 Apr 2022 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:17:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

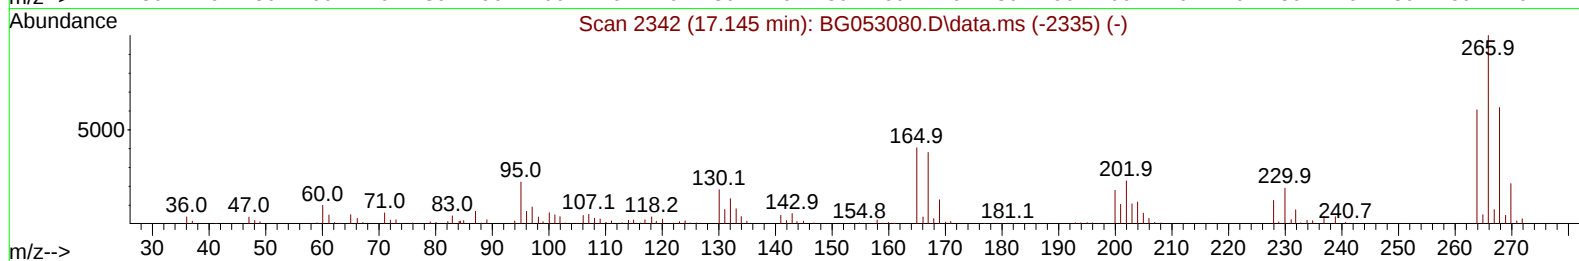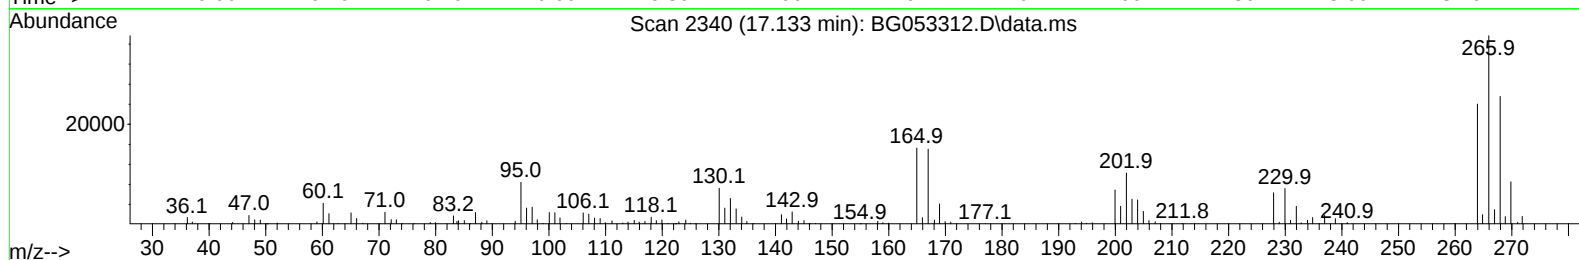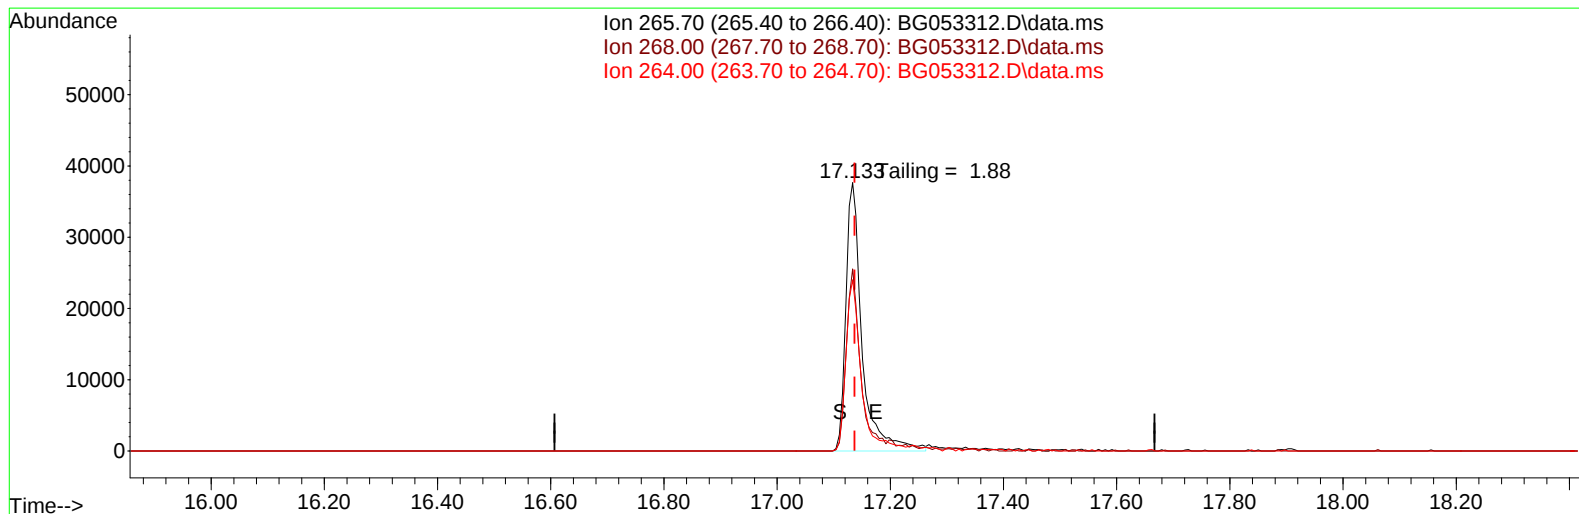

TIC: BG053312.D\data.ms

(70) Pentachlorophenol (C)

17.133min (-0.003) 60253.37 ng




response 74483

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.84
264.00	56.60	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
 Data File : BG053312.D
 Acq On : 26 Apr 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 05:17:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 01:13:30 2022
 Response via : Initial Calibration

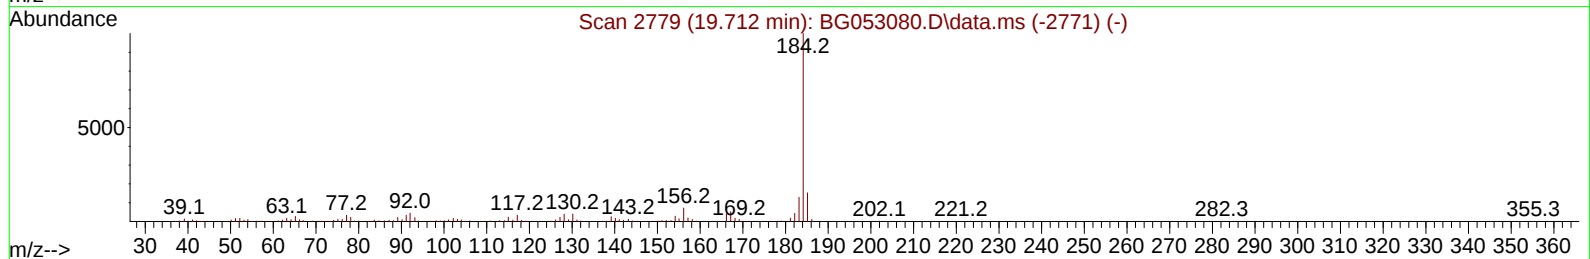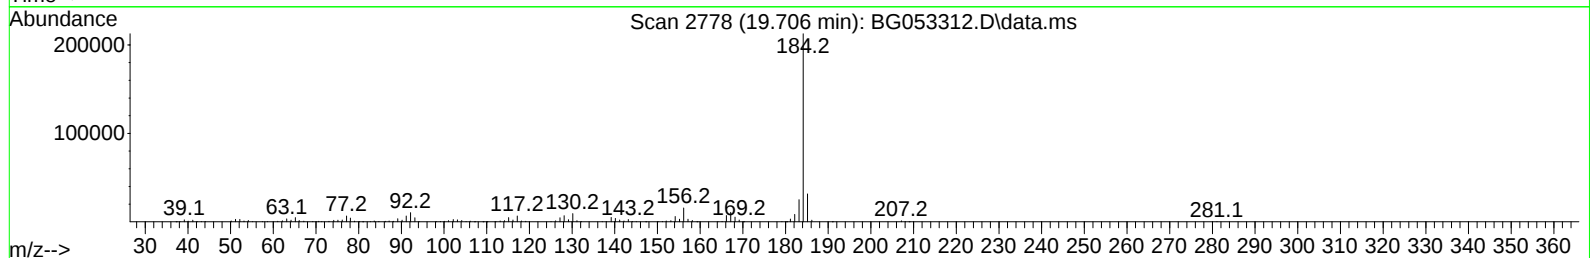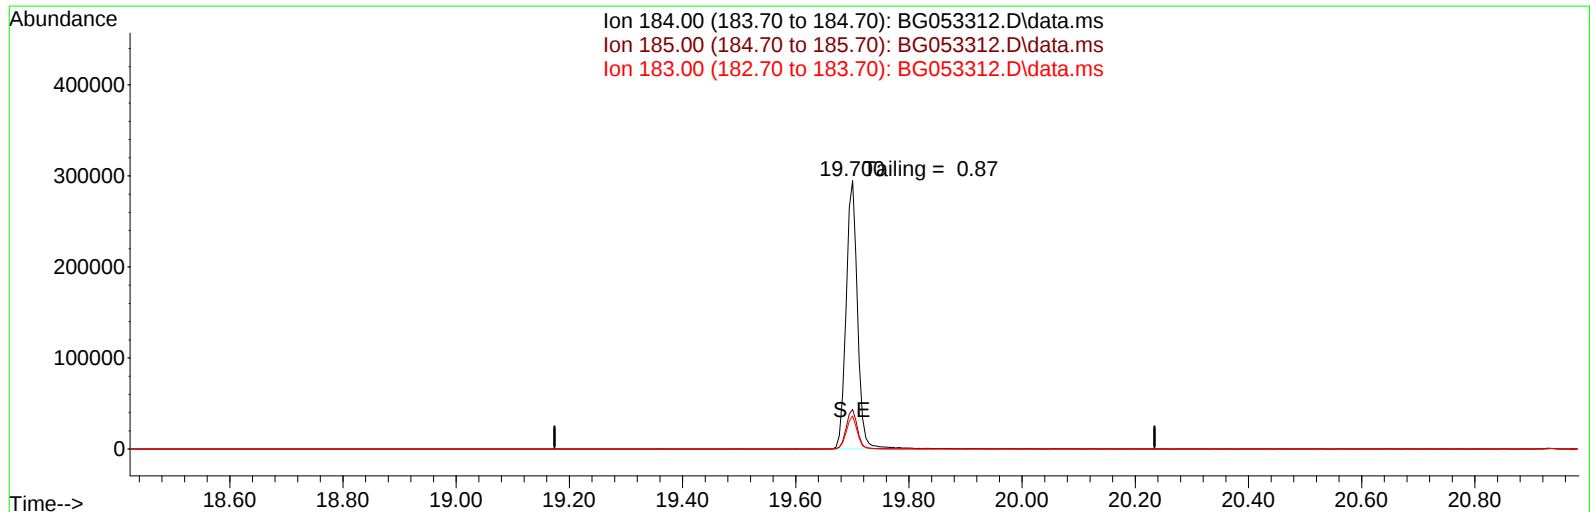

TIC: BG053312.D\data.ms

(77) Benzidine

19.704min (-19.704) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2022	BNA_G	<u>BG053312.D</u>
Compound Name	Response	Retention Time
DDT	196923	20.934
DDD	2073	20.546
DDE	57	19.959
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2130	199053	1.07

Instrument :
BNA_G
ClientSampleId :
DFTPP