
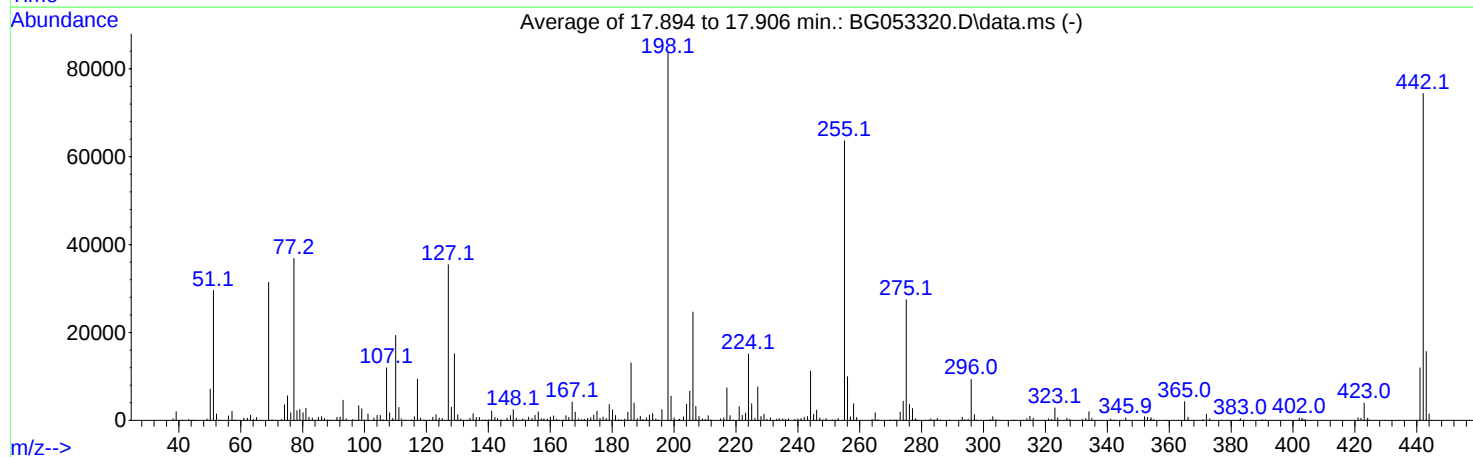


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
 Data File : BG053320.D
 Acq On : 26 Apr 2022 14:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

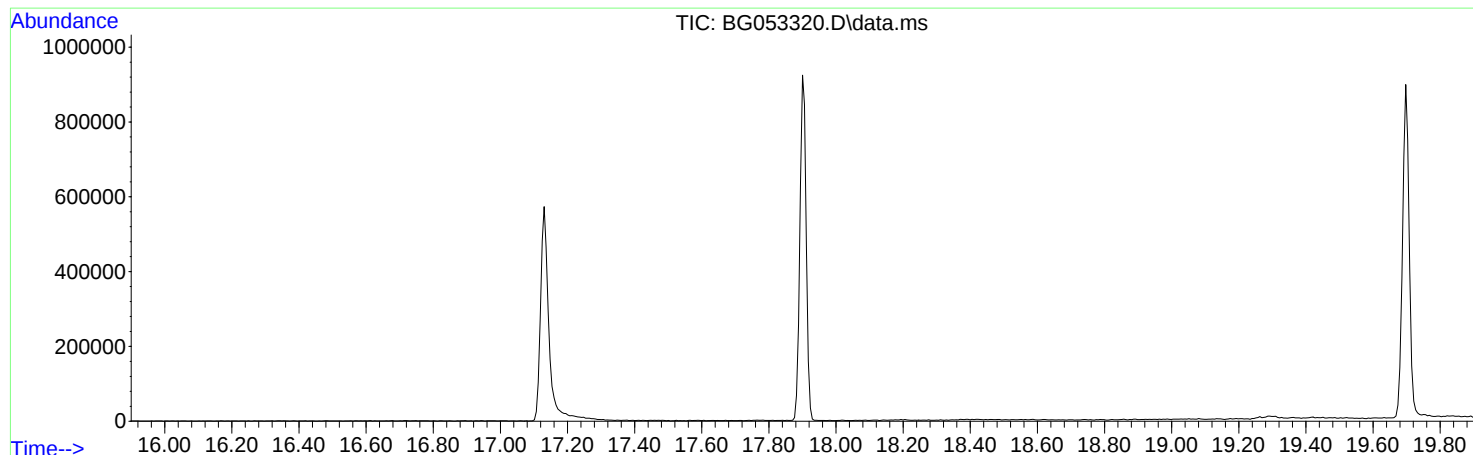




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	29565	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	31390	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	42.3	35448	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83725	PASS
199	198	5	9	6.6	5524	PASS
275	198	10	60	32.8	27477	PASS
365	198	1	100	5.1	4283	PASS
441	198	0.01	100	14.3	11943	PASS
442	442	50	100	100.0	74408	PASS
443	442	15	24	21.0	15645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
 Data File : BG053320.D
 Acq On : 26 Apr 2022 14:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 15:21:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 01:13:30 2022
 Response via : Initial Calibration

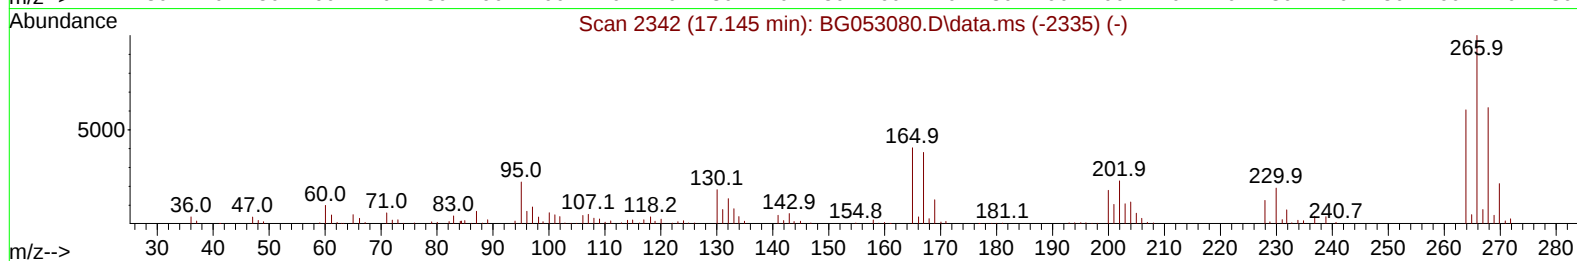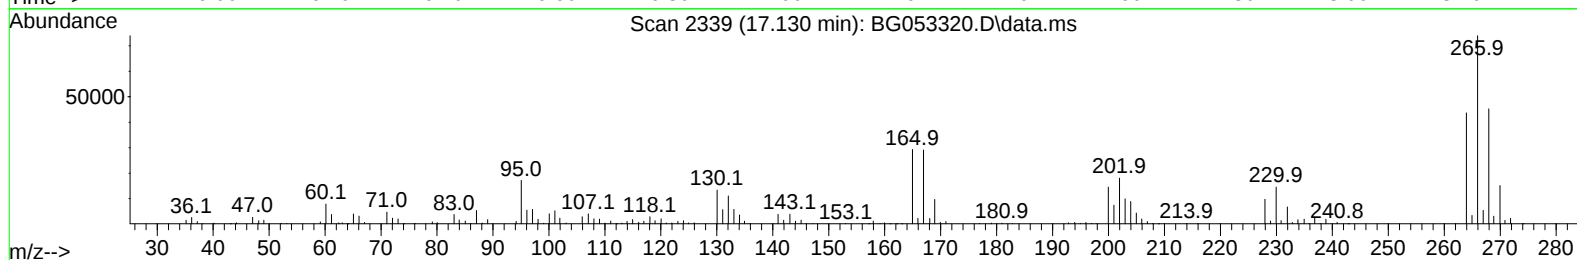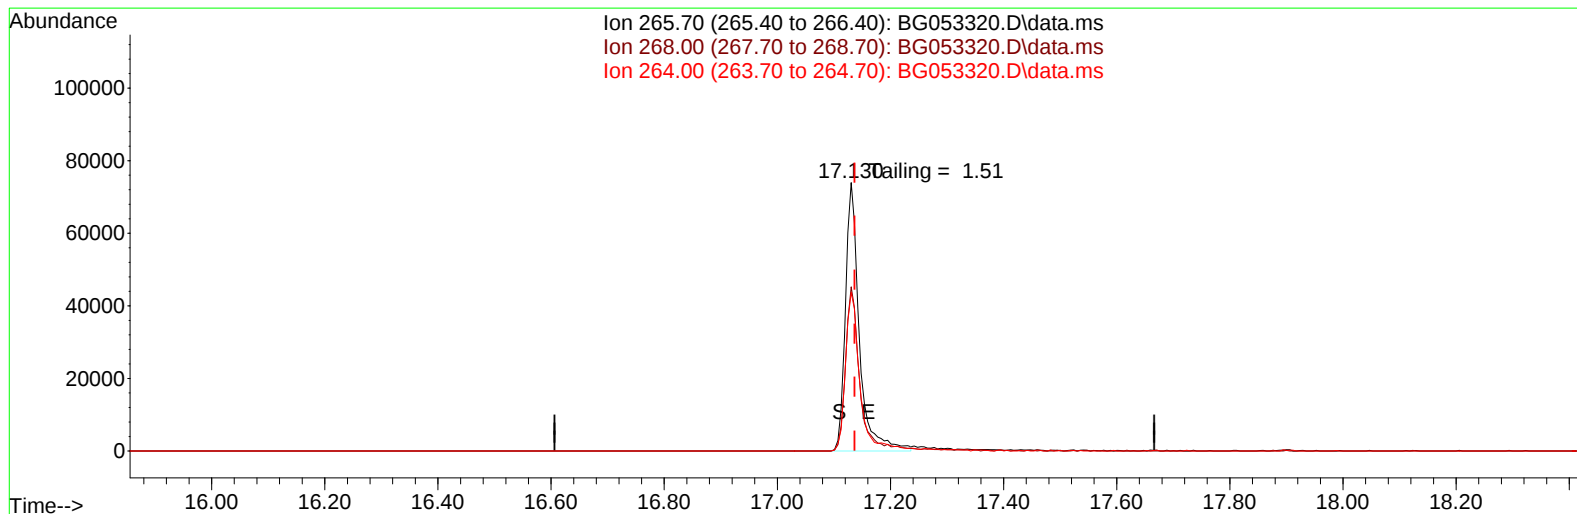

TIC: BG053320.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.006) 302564.59 ng




response 130792

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.19
264.00	56.60	59.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042622\
Data File : BG053320.D
Acq On : 26 Apr 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 26 15:21:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

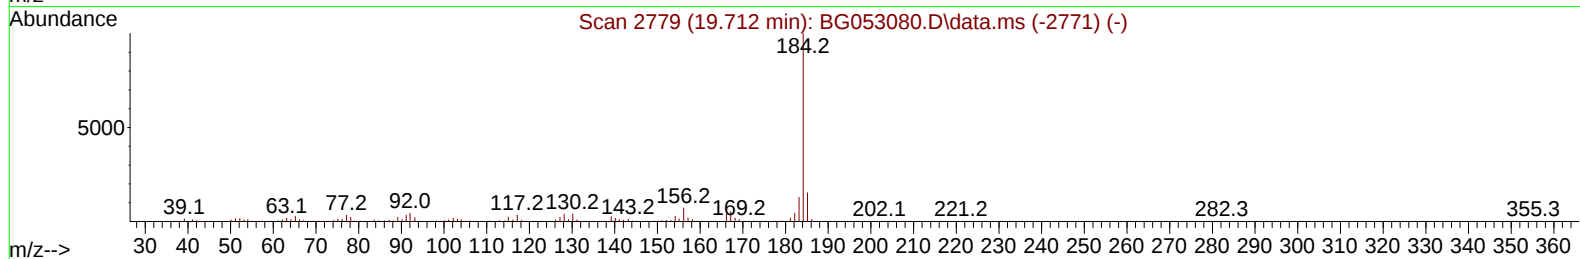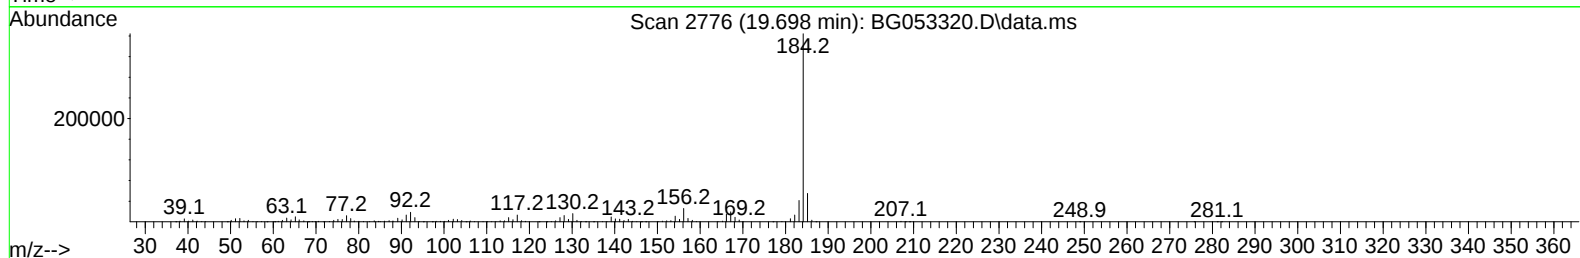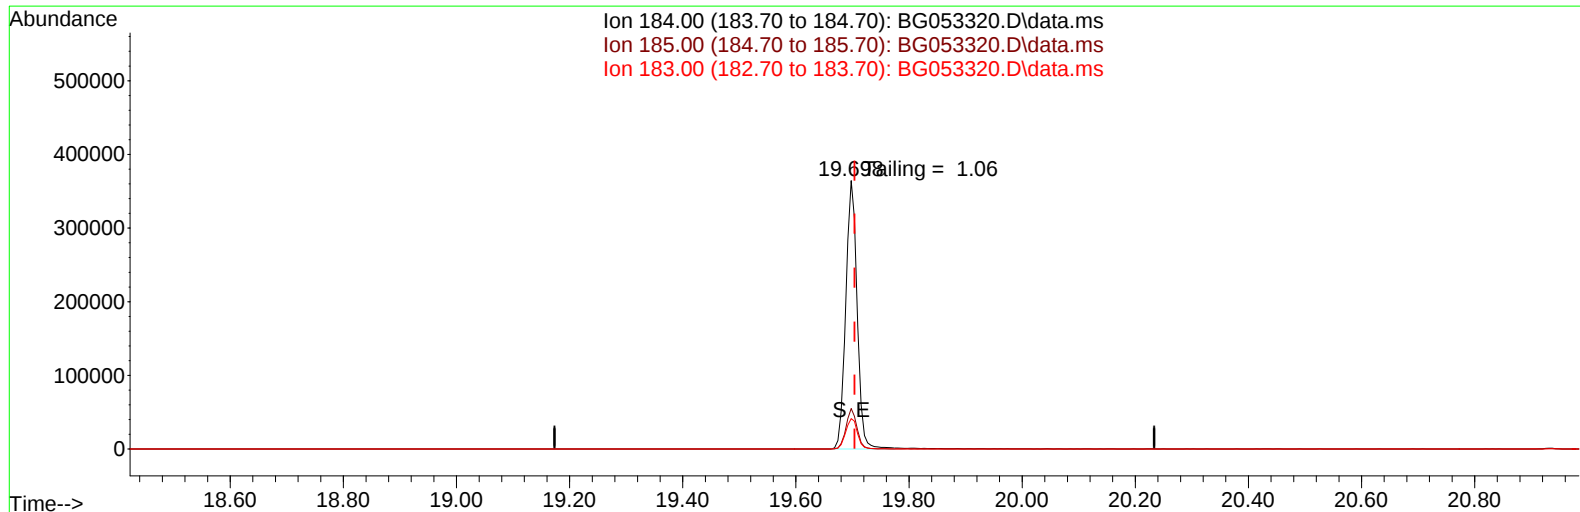

TIC: BG053320.D\data.ms

(77) Benzidine

19.698min (-0.006) 0.00 ng

response 510801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.09
183.00	11.80	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2022	BNA_G	<u>BG053320.D</u>
Compound Name	Response	Retention Time
DDT	269070	20.937
DDD	2520	20.543
DDE	54	19.991
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2574	271644	0.95

Instrument :
BNA_G
ClientSampleId :
DFTPP