

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
 Data File : BG016752.D
 Acq On : 28 Apr 2015 4:35
 Operator : TP/IZ
 Sample : G1992-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEC01

Quant Time: Apr 28 05:44:41 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 01:49:03 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	61625	20.00	ng	0.00
21) Naphthalene-d8	10.36	136	272599	20.00	ng	0.00
38) Acenaphthene-d10	14.22	164	162461	20.00	ng	0.00
63) Phenanthrene-d10	16.97	188	325726	20.00	ng	0.00
75) Chrysene-d12	21.16	240	295263	20.00	ng	0.00
86) Perylene-d12	23.35	264	284218	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	368436	97.02	ng	0.00
7) Phenol-d6	6.77	99	512634	96.22	ng	0.00
23) Nitrobenzene-d5	8.73	82	257730	59.74	ng	0.00
41) 2,4,6-Tribromophenol	15.72	330	126329	104.82	ng	0.00
44) 2-Fluorobiphenyl	12.84	172	651895	64.47	ng	0.00
78) Terphenyl-d14	19.61	244	737023	57.50	ng	0.00
Target Compounds						Qvalue
32) Benzoic acid	9.69	122	2294	9.64	ng	90
49) Dimethylphthalate	13.69	163	59095	4.86	ng	98
70) Phenanthrene	17.01	178	69572	3.72	ng	98
74) Fluoranthene	19.04	202	123211	6.21	ng	95
77) Pyrene	19.40	202	141209	6.81	ng	97
80) Benzo(a)anthracene	21.15	228	60936	3.40	ng	97
82) Chrysene	21.19	228	70568	4.11	ng	97
87) Benzo(b)fluoranthene	22.70	252	112382	6.51	ng	98
88) Benzo(k)fluoranthene	22.70	252	112382	6.67	ng	98
89) Benzo(a)pyrene	23.26	252	58964	3.62	ng	97
91) Benzo(g,h,i)perylene	26.26	276	35073	2.18	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
Data File : BG016752.D
Acq On : 28 Apr 2015 4:35
Operator : TP/IZ
Sample : G1992-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEC01

Quant Time: Apr 28 05:44:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 28 01:49:03 2015
Response via : Initial Calibration

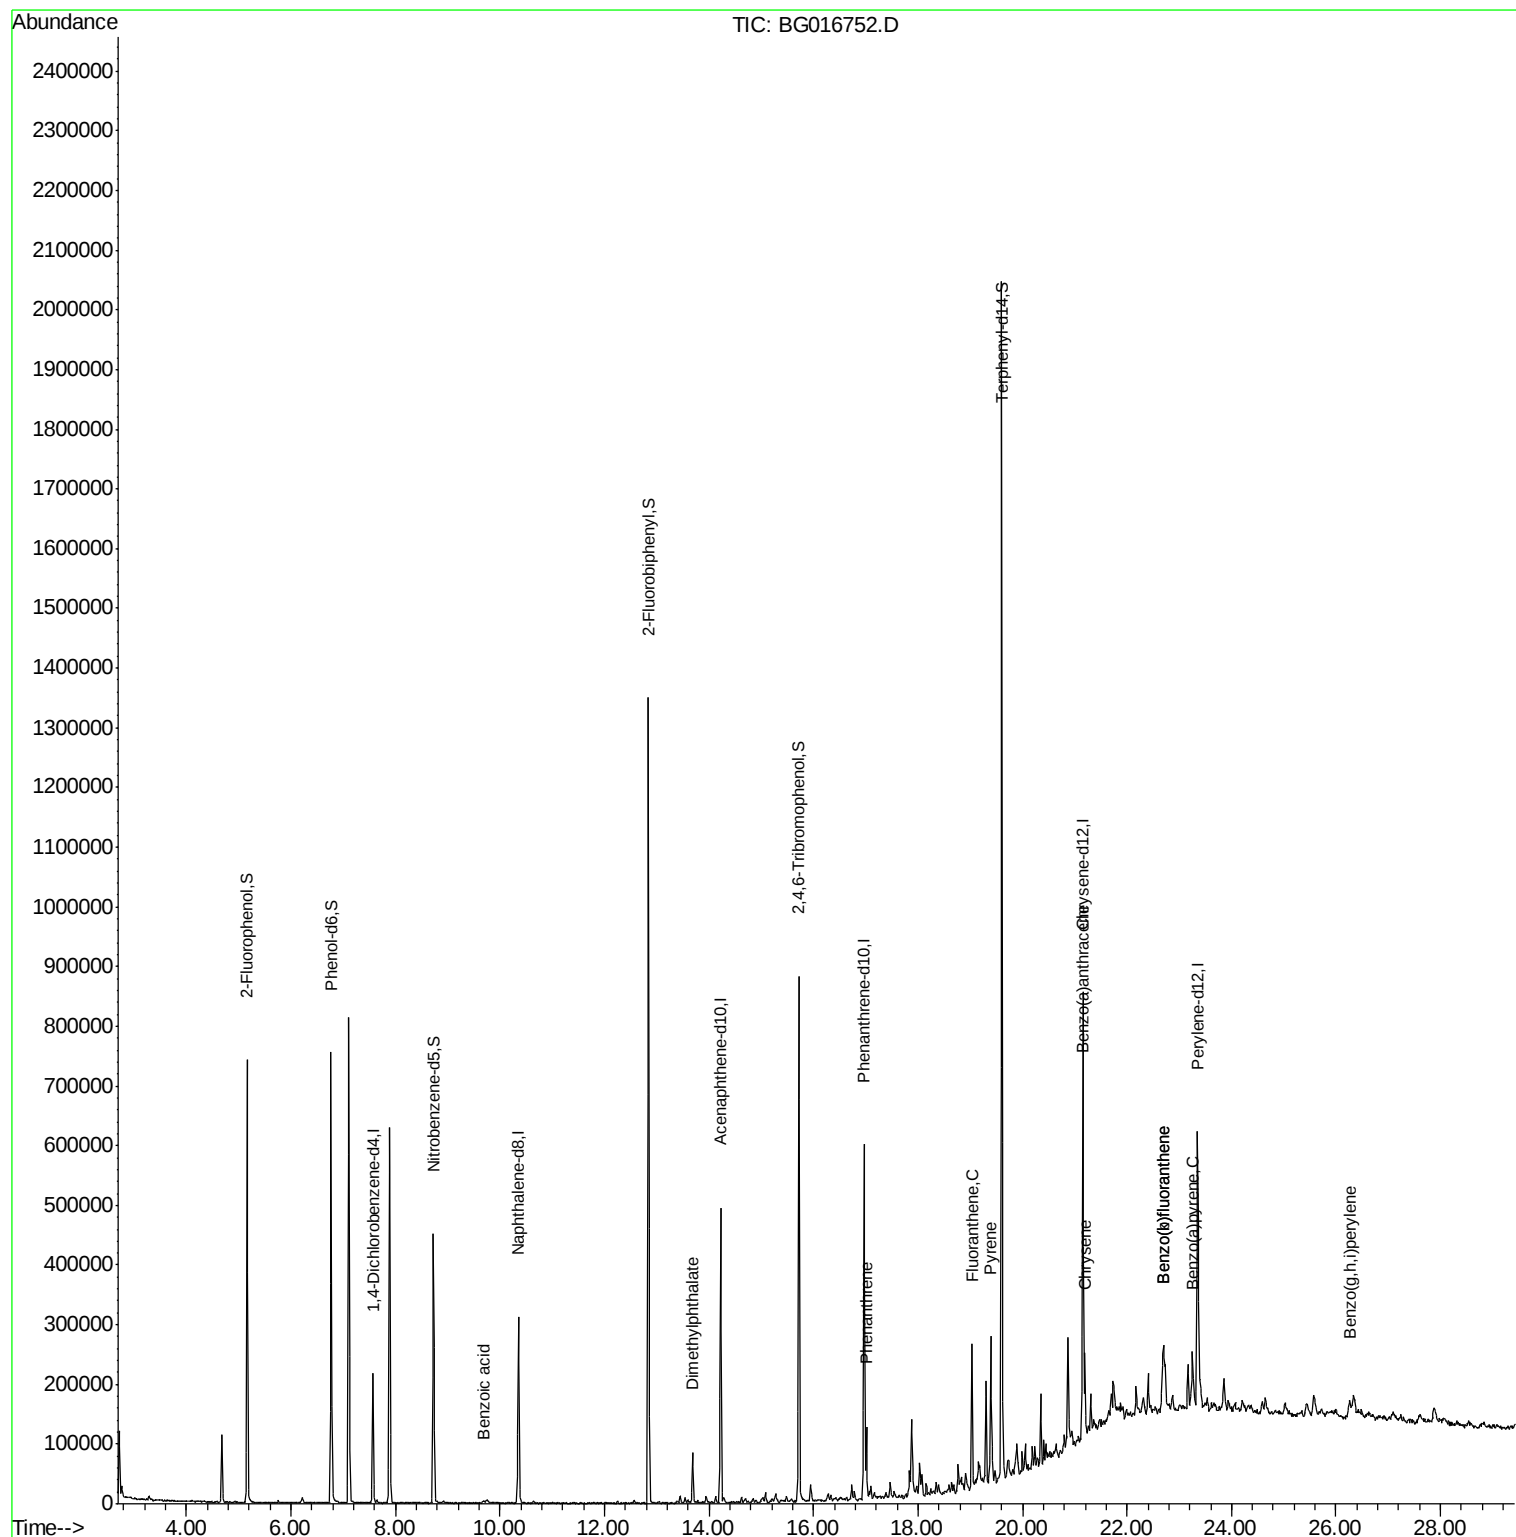

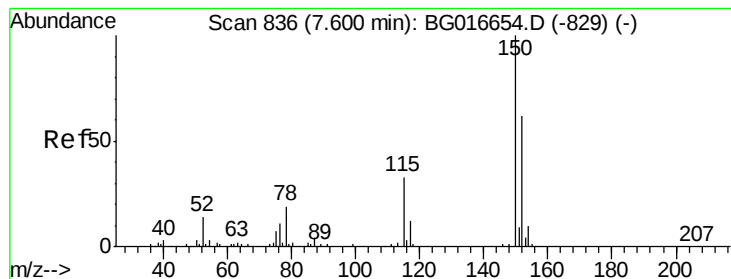

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.57 min Scan# 831

Delta R.T. 0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35

Instrument :

BNA_G

ClientSampleId :

TEC01


Tgt Ion:152 Resp: 61625

Ion Ratio Lower Upper

152 100

150 153.1 129.6 194.4




115 51.3 43.0 64.6

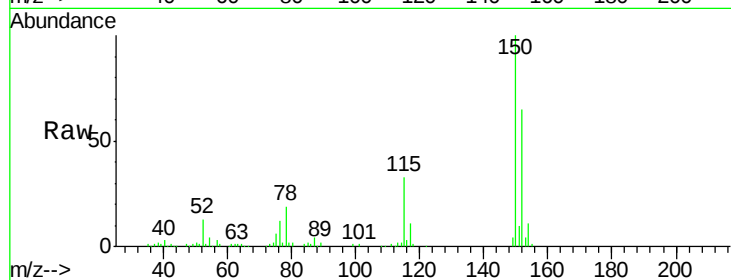

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

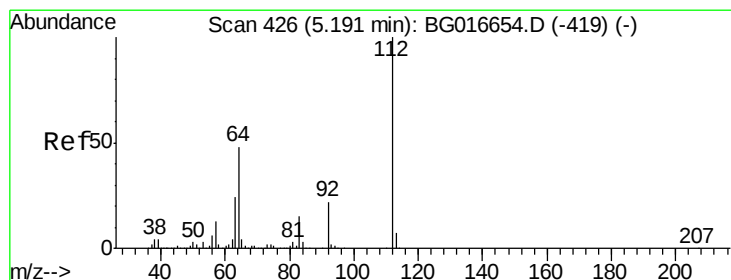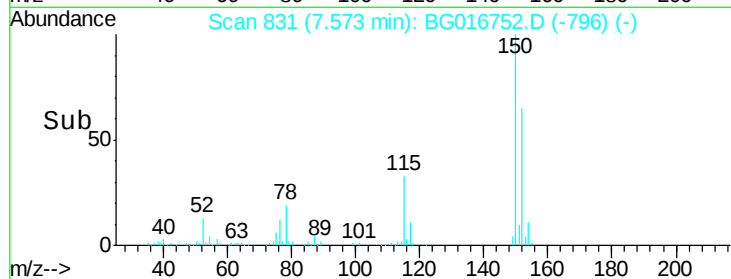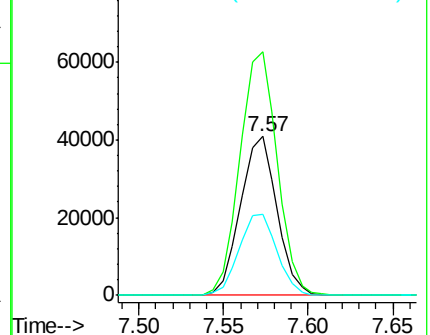

#5

2-Fluorophenol

Concen: 97.02 ng

RT: 5.16 min Scan# 421

Delta R.T. 0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35


Tgt Ion:112 Resp: 368436

Ion Ratio Lower Upper

112 100

64 46.1 38.3 57.5



63 22.8 18.9 28.3

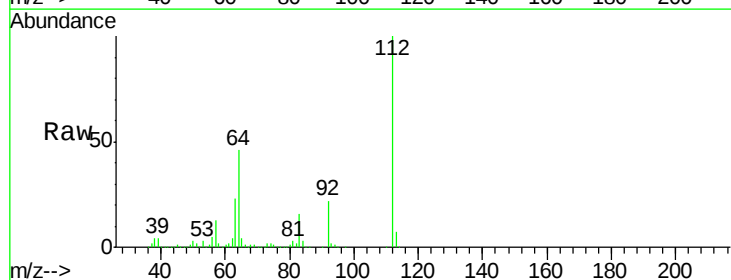

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

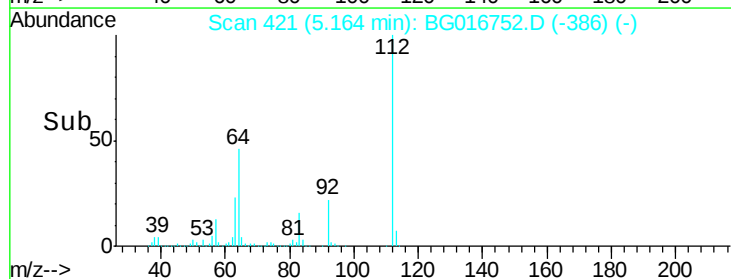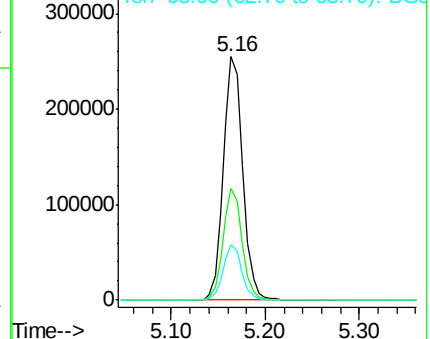



#7

Phenol-d6

Concen: 96.22 ng

RT: 6.77 min Scan# 695

Delta R.T. -0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35

Instrument :

BNA_G

ClientSampleId :

TEC01


Tgt Ion: 99 Resp: 512634

Ion Ratio Lower Upper




99 100

42 10.9 8.8 13.2

71 25.1 19.9 29.9



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

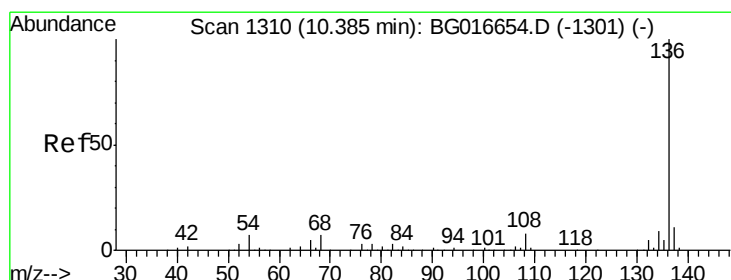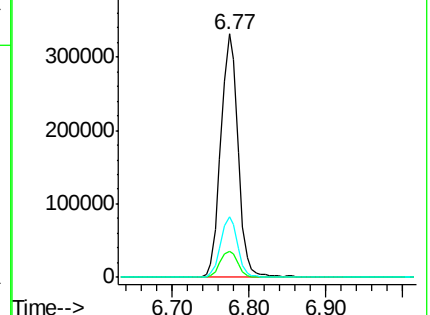

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.36 min Scan# 1305

Delta R.T. 0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35

Tgt Ion: 136 Resp: 272599


Ion Ratio Lower Upper

136 100



137 10.6 8.5 12.7

54 5.5 5.4 8.2

68 5.4 5.2 7.8

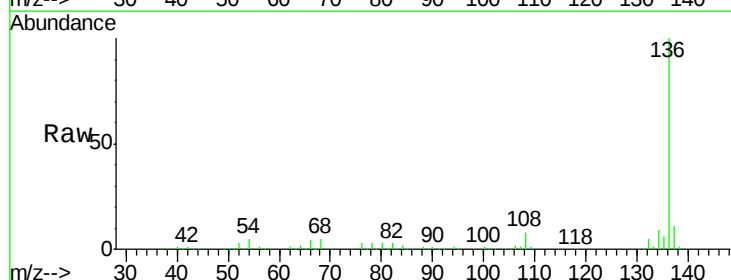

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



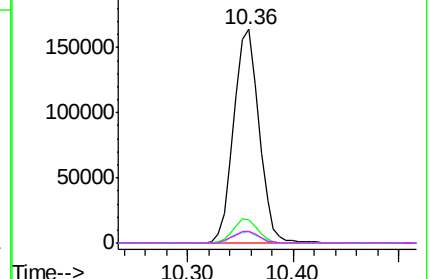
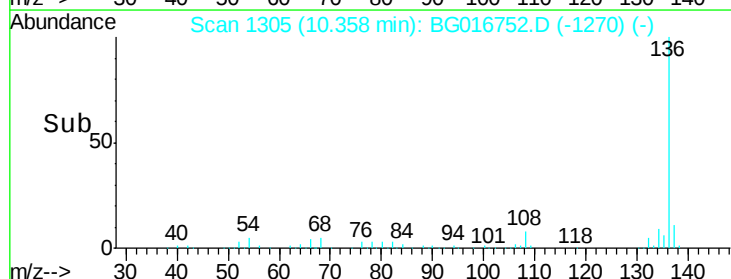




#23
 Nitrobenzene-d5
 Concen: 59.74 ng
 RT: 8.73 min Scan# 1028
 Delta R.T. -0.00 min
 Lab File: BG016752.D
 Acq: 28 Apr 2015 4:35




Instrument :
 BNA_G
 ClientSampleId :
 TEC01


Tgt Ion: 82 Resp: 257730
 Ion Ratio Lower Upper
 82 100
 128 56.4 44.7 67.1
 54 38.1 30.9 46.3

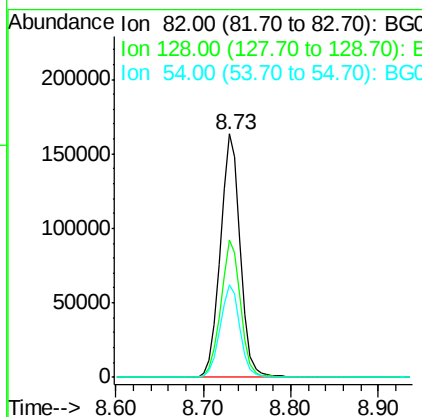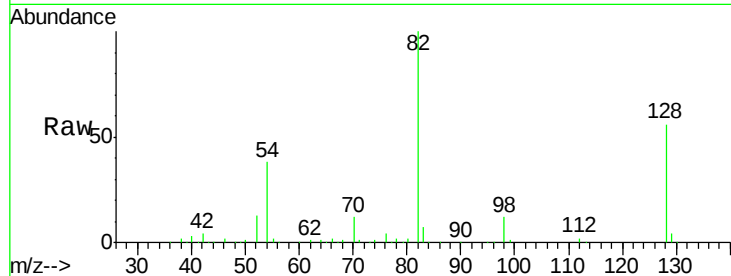

#32
 Benzoic acid
 Concen: 9.64 ng
 RT: 9.69 min Scan# 1191
 Delta R.T. -0.04 min
 Lab File: BG016752.D
 Acq: 28 Apr 2015 4:35

Tgt Ion: 122 Resp: 2294
 Ion Ratio Lower Upper
 122 100
 105 126.5 97.2 137.2
 77 88.5 58.4 98.4

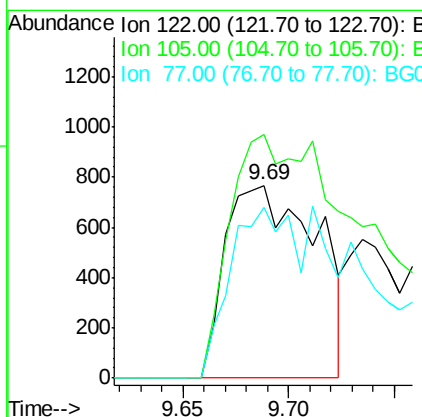

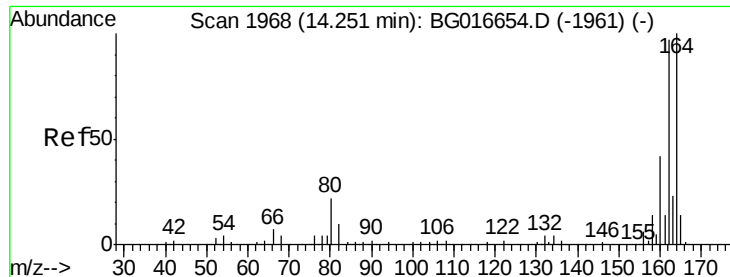

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.22 min Scan# 1963

Delta R.T. -0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35

Instrument :

BNA_G

ClientSampleId :

TEC01


Tgt Ion:164 Resp: 162461

Ion Ratio Lower Upper

164 100

162 98.0 77.3 115.9




160 45.8 33.7 50.5

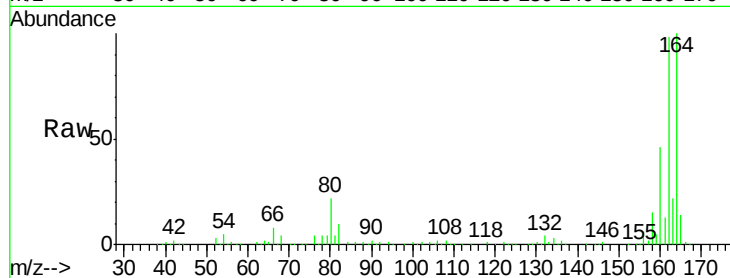

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

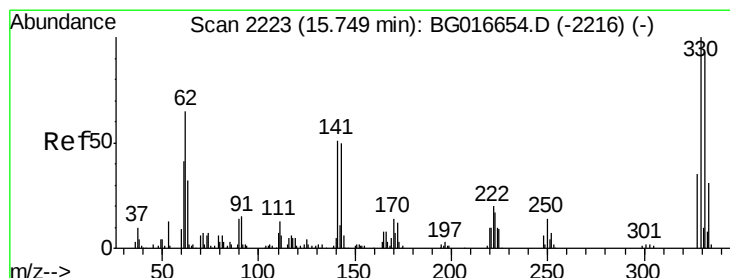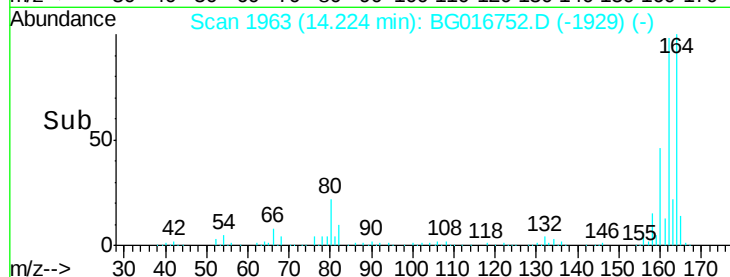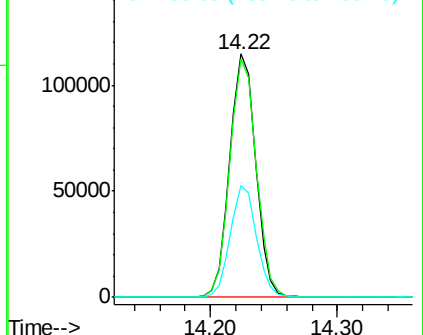

#41

2,4,6-Tribromophenol

Concen: 104.82 ng

RT: 15.72 min Scan# 2218

Delta R.T. -0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35


Tgt Ion:330 Resp: 126329

Ion Ratio Lower Upper

330 100

332 97.4 76.2 114.4



141 48.6 43.0 64.6

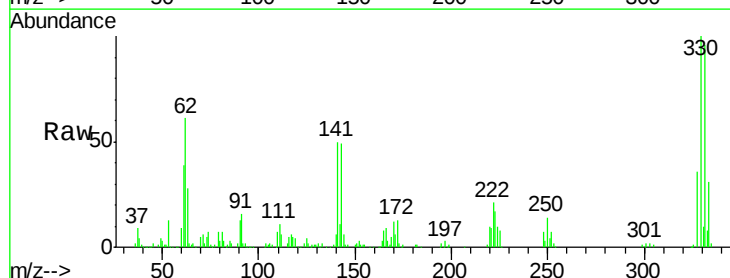


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



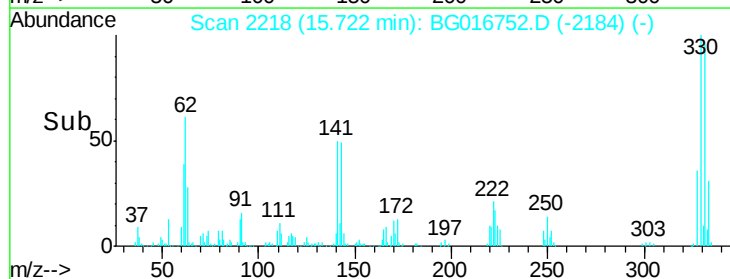
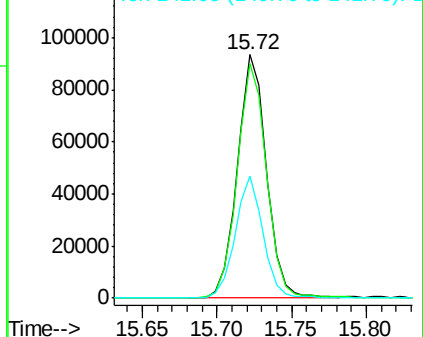




#44
2-Fluorobiphenyl
Concen: 64.47 ng
RT: 12.84 min Scan# 1728
Delta R.T. 0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35




Instrument :
BNA_G
ClientSampleId :
TEC01


Tgt Ion:172 Resp: 651895
Ion Ratio Lower Upper
172 100
171 36.9 29.9 44.9
170 23.9 19.8 29.8

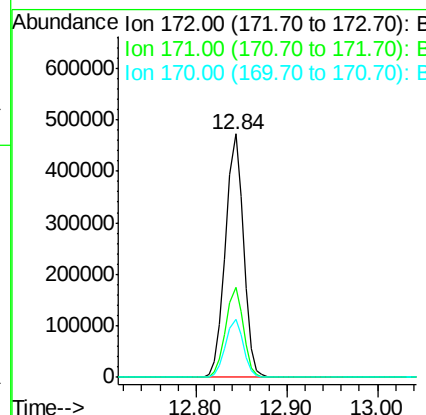

#49
Dimethylphthalate
Concen: 4.86 ng
RT: 13.69 min Scan# 1872
Delta R.T. -0.01 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Tgt Ion:163 Resp: 59095
Ion Ratio Lower Upper
163 100
194 5.7 5.0 7.4
164 10.4 7.8 11.8

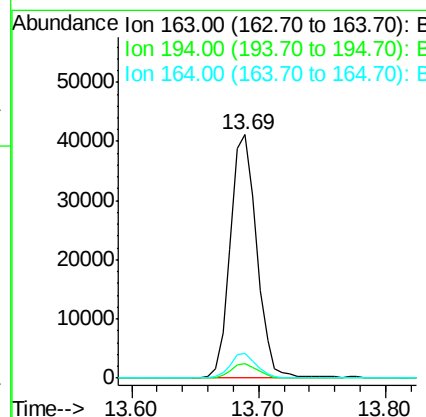


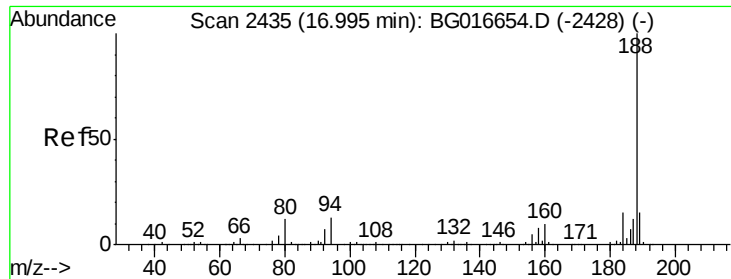




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.97 min Scan# 2431
Delta R.T. 0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Instrument :
BNA_G
ClientSampleId :
TEC01

Tgt Ion:188 Resp: 325726
Ion Ratio Lower Upper
188 100
94 10.9 10.7 16.1
80 10.7 9.9 14.9




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC


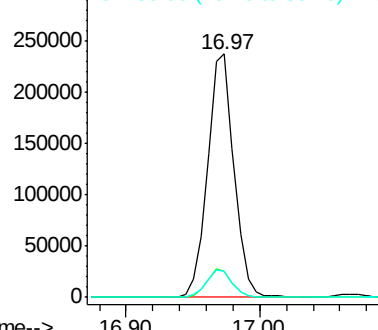



#70
Phenanthrene
Concen: 3.72 ng
RT: 17.01 min Scan# 2438
Delta R.T. -0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Tgt Ion:178 Resp: 69572
Ion Ratio Lower Upper
178 100
176 20.9 15.8 23.6
179 16.5 12.8 19.2



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

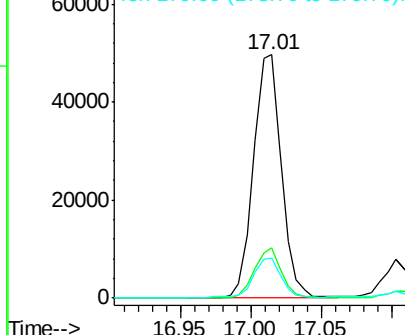



#74

Fluoranthene

Concen: 6.21 ng

RT: 19.04 min Scan# 2782

Delta R.T. 0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35

Instrument :

BNA_G

ClientSampleId :

TEC01


Tgt Ion:202 Resp: 123211

Ion Ratio Lower Upper

202 100

101 14.5 0.0 38.1




203 17.4 0.0 38.4



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

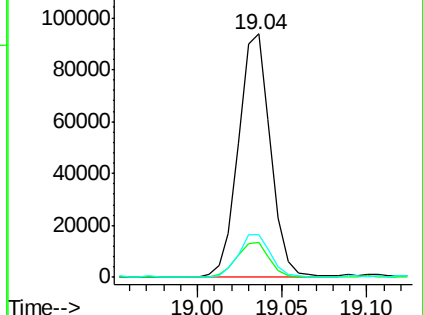

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.16 min Scan# 3143

Delta R.T. -0.00 min

Lab File: BG016752.D

Acq: 28 Apr 2015 4:35


Tgt Ion:240 Resp: 295263

Ion Ratio Lower Upper

240 100

120 19.2 16.3 24.5



236 25.8 21.1 31.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

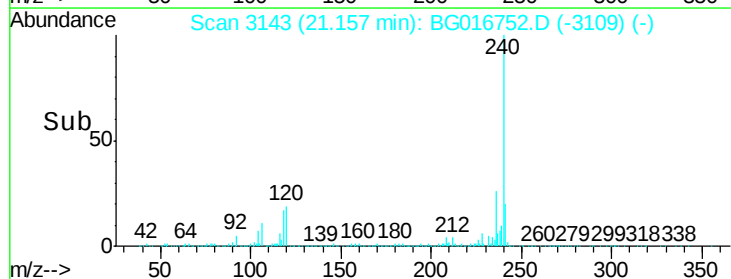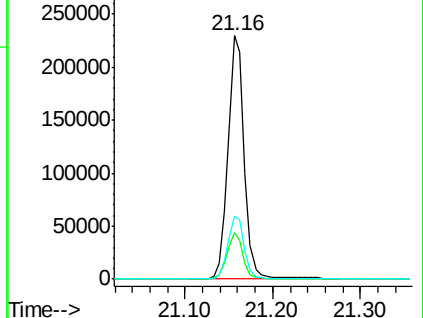







#77
 Pyrene
 Concen: 6.81 ng
 RT: 19.40 min Scan# 2844
 Delta R.T. 0.00 min
 Lab File: BG016752.D
 Acq: 28 Apr 2015 4:35

Instrument :
 BNA_G
 ClientSampleId :
 TEC01

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.3	18.0	27.0
203	17.7	14.9	22.3




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E


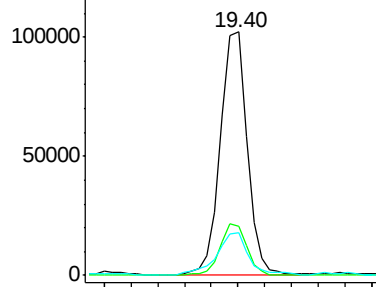



#78
 Terphenyl-d14
 Concen: 57.50 ng
 RT: 19.61 min Scan# 2879
 Delta R.T. -0.00 min
 Lab File: BG016752.D
 Acq: 28 Apr 2015 4:35

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.0	6.4	9.6
122	18.7	15.9	23.9



Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

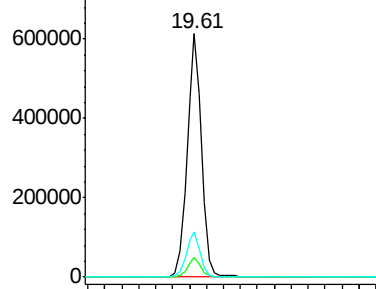


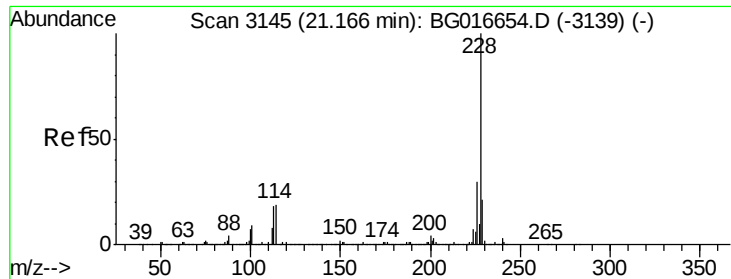




#80
Benzo(a)anthracene
Concen: 3.40 ng
RT: 21.15 min Scan# 3141
Delta R.T. -0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Instrument :
BNA_G
ClientSampleId :
TEC01

Tgt Ion:228 Resp: 60936
Ion Ratio Lower Upper
228 100
226 29.9 23.8 35.6
229 24.0 17.0 25.4




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

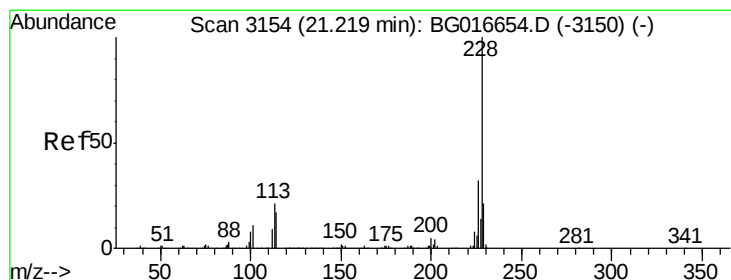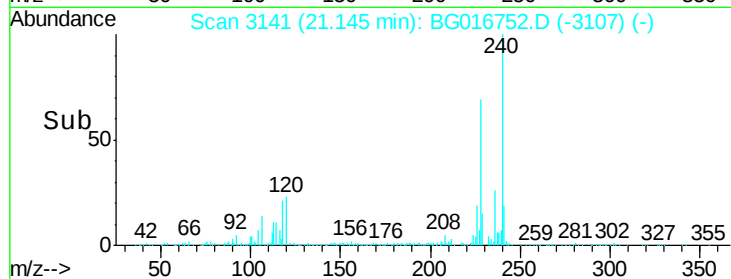
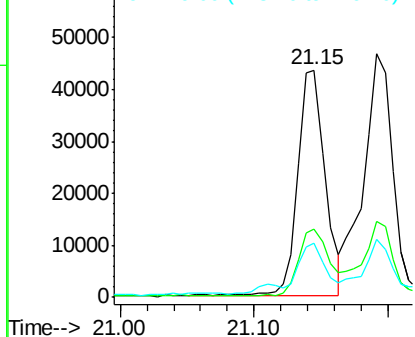



#82
Chrysene
Concen: 4.11 ng
RT: 21.19 min Scan# 3149
Delta R.T. -0.01 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Tgt Ion:228 Resp: 70568
Ion Ratio Lower Upper
228 100
226 31.3 25.4 38.0
229 23.7 16.5 24.7

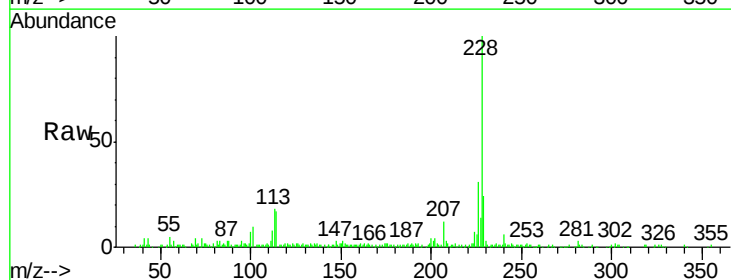

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

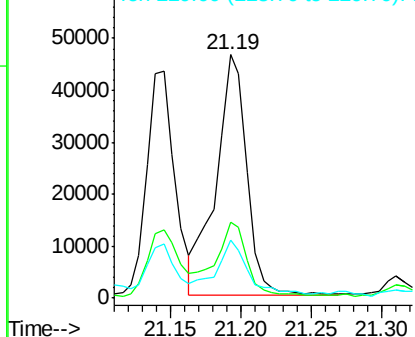







#86
Perylene-d12
Concen: 20.00 ng
RT: 23.35 min Scan# 3517
Delta R.T. -0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Instrument :
BNA_G
ClientSampleId :
TEC01

Tgt Ion: 264 Resp: 284218




Ion	Ratio	Lower	Upper
264	100		
260	24.9	20.0	30.0
265	21.7	16.8	25.2

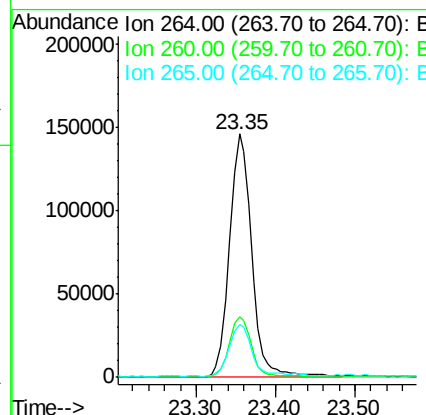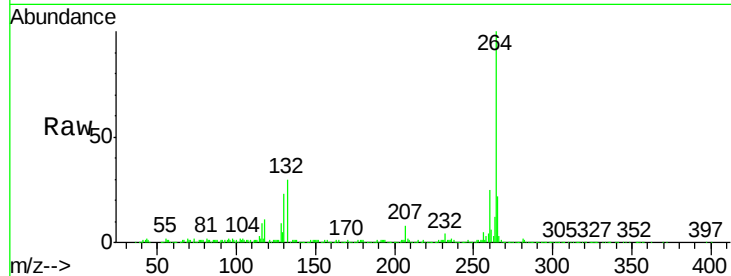


#87
Benzo(b)fluoranthene
Concen: 6.51 ng
RT: 22.70 min Scan# 3405
Delta R.T. -0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Tgt Ion: 252 Resp: 112382

Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.9	26.9
125	18.7	15.8	23.8



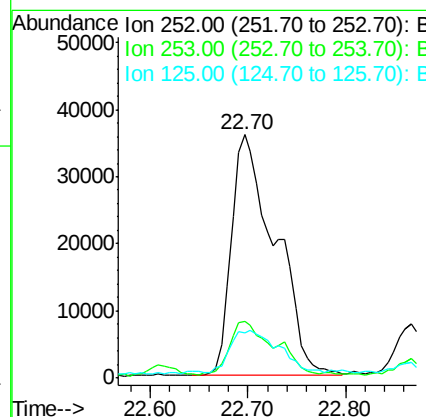
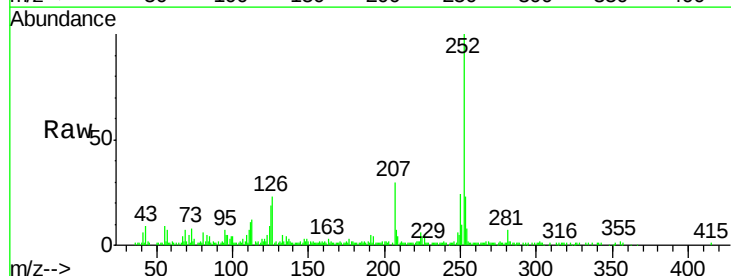


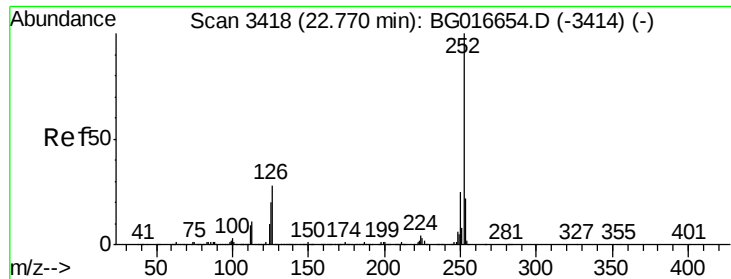

#88
Benzo(k)fluoranthene
Concen: 6.67 ng
RT: 22.70 min Scan# 3405
Delta R.T. -0.04 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35




Instrument :
BNA_G
ClientSampleId :
TEC01


Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.6	26.4
125	18.7	15.5	23.3

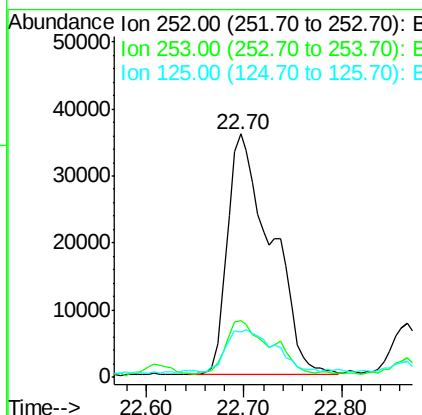

#89
Benzo(a)pyrene
Concen: 3.62 ng
RT: 23.26 min Scan# 3501
Delta R.T. -0.00 min
Lab File: BG016752.D
Acq: 28 Apr 2015 4:35

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.2	25.8
125	18.4	16.3	24.5

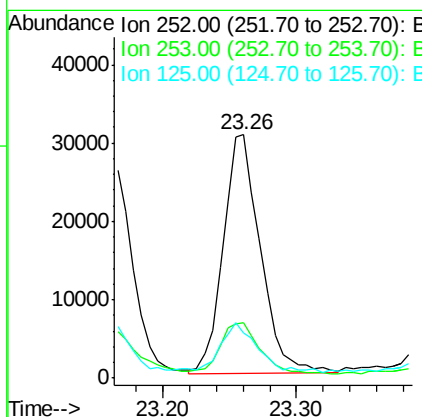




#91
 Benzo(g,h,i)perylene
 Concen: 2.18 ng
 RT: 26.26 min Scan# 4012
 Delta R.T. -0.00 min
 Lab File: BG016752.D
 Acq: 28 Apr 2015 4:35

Instrument :
 BNA_G
 ClientSampleId :
 TEC01

Tgt Ion	Ratio	Lower	Upper
276	100		
277	27.6	19.3	28.9
138	45.1	32.8	49.2

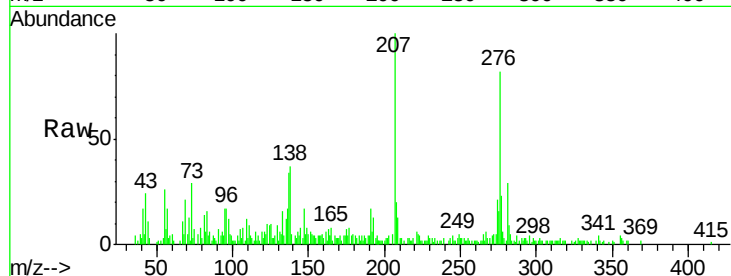

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

