


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
 Data File : BG016746.D
 Acq On : 28 Apr 2015 00:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 28 00:54:32 2015

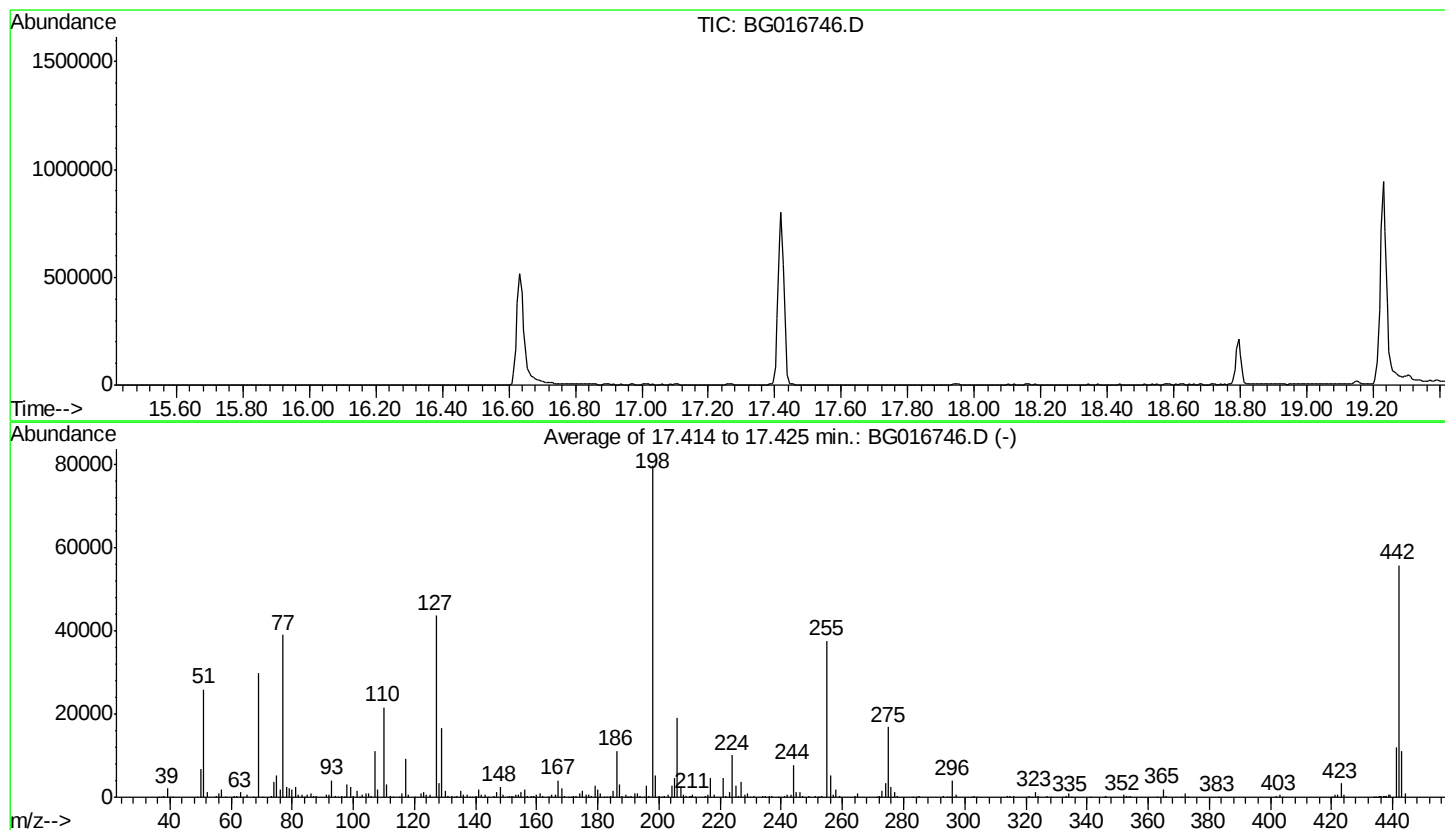

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	26024	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	30045	PASS
70	69	0.00	2	0.5	154	PASS
127	198	10	80	54.7	43688	PASS
197	198	0.00	2	0.3	215	PASS
198	198	100	100	100.0	79829	PASS
199	198	5	9	6.4	5128	PASS
275	198	10	60	21.1	16818	PASS
365	198	1	100	2.4	1895	PASS
441	442	0.01	24	21.5	12039	PASS
442	198	50	100	70.0	55885	PASS
443	442	15	24	20.0	11183	PASS