
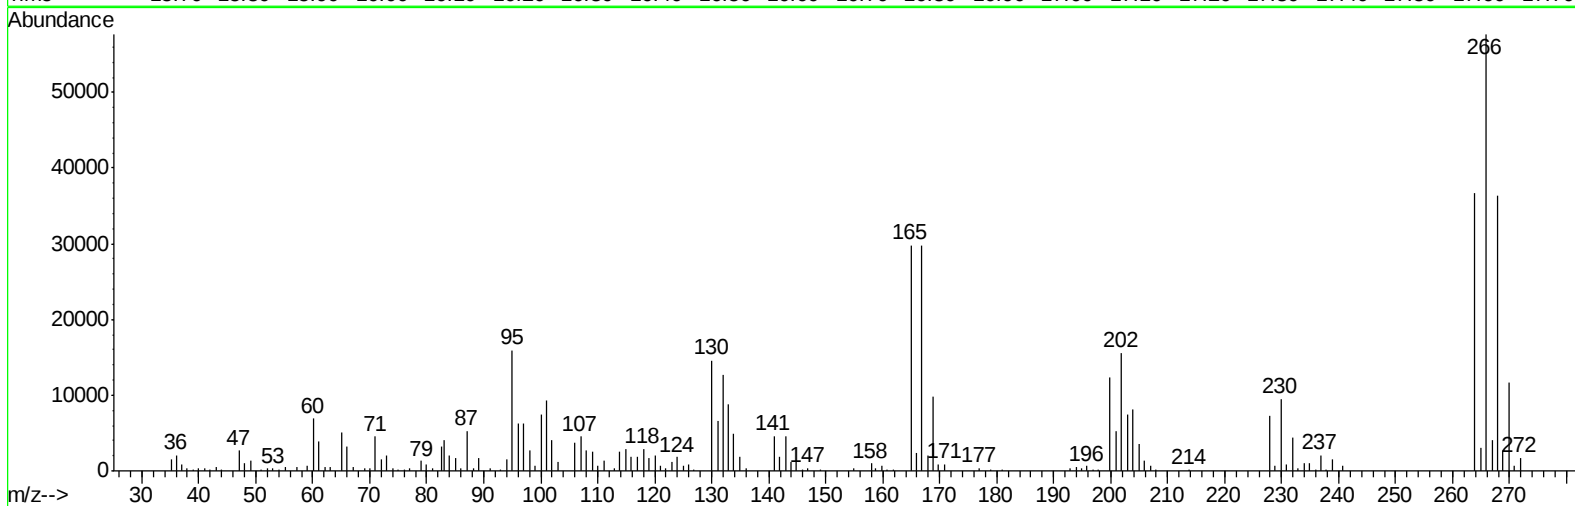


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
Data File : BG016729.D
Acq On : 27 Apr 2015 10:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:54:09 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 28 01:49:03 2015
Response via : Initial Calibration

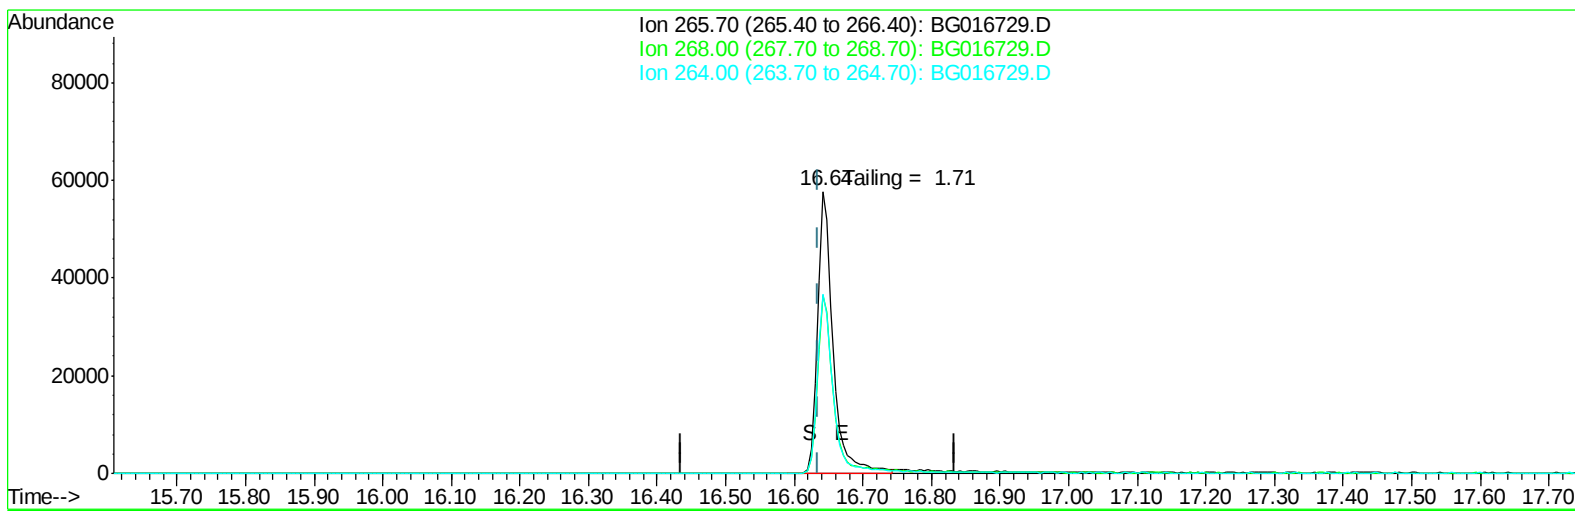

TIC: BG016729.D

(69) Pentachlorophenol (C)



16.642min (+0.006) 32871.78ng

response 91495

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	63.03
264.00	64.70	63.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
Data File : BG016729.D
Acq On : 27 Apr 2015 10:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:54:09 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 28 01:49:03 2015
Response via : Initial Calibration

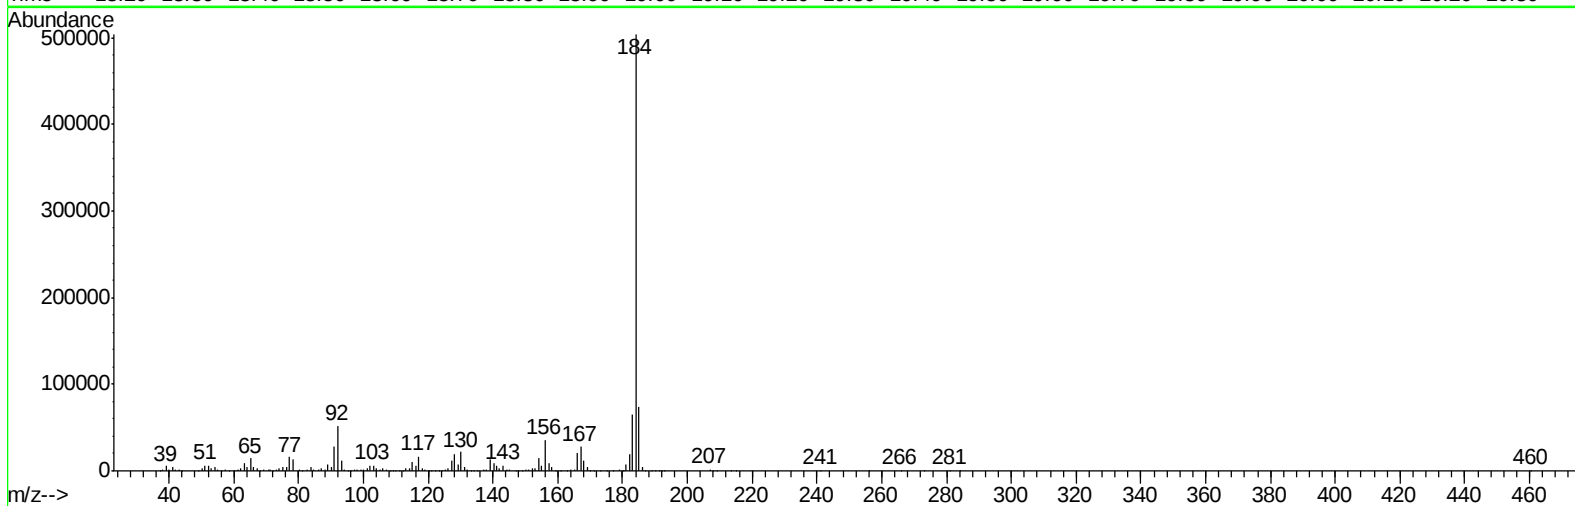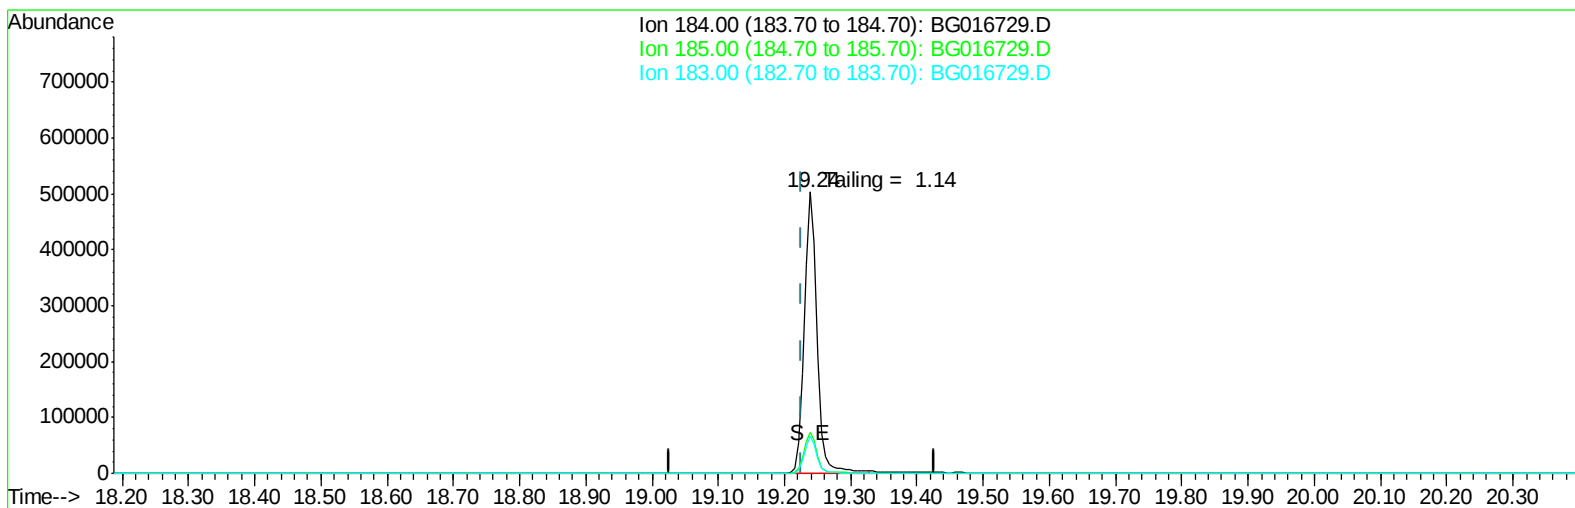

TIC: BG016729.D

(76) Benzidine

19.239min (+0.012) 15361.05ng

response 684843

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.74
183.00	12.60	13.01
0.00	0.00	0.00