
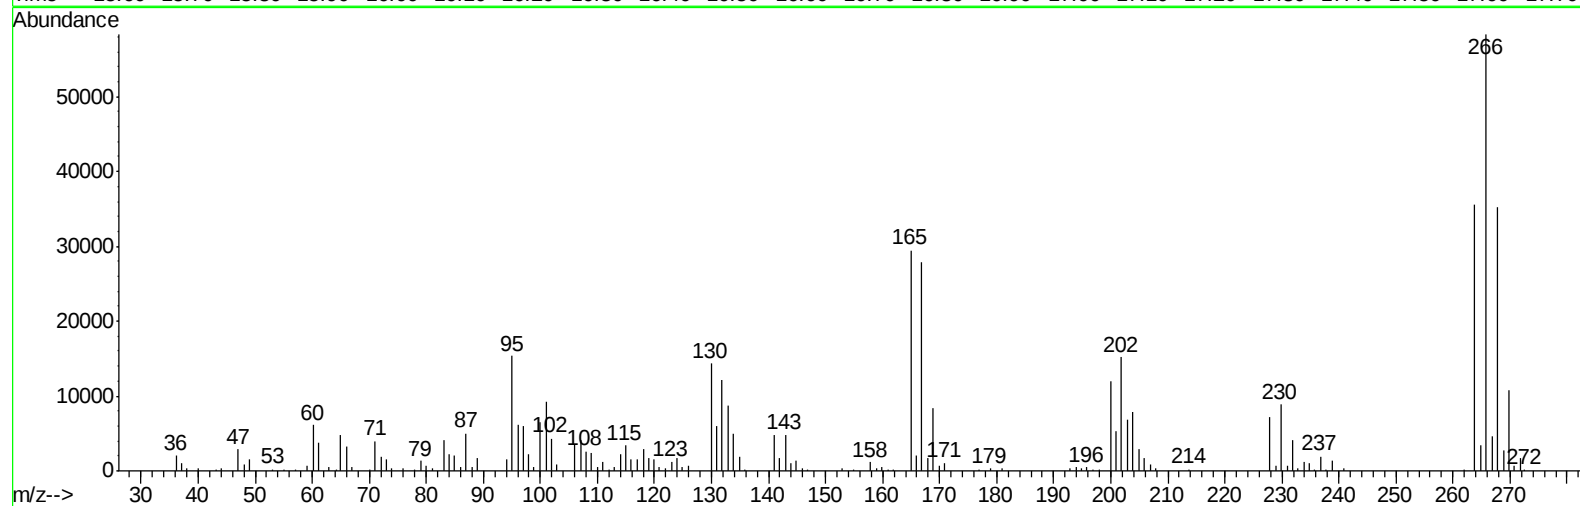


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
Data File : BG016746.D
Acq On : 28 Apr 2015 00:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:56:07 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 28 01:49:03 2015
Response via : Initial Calibration

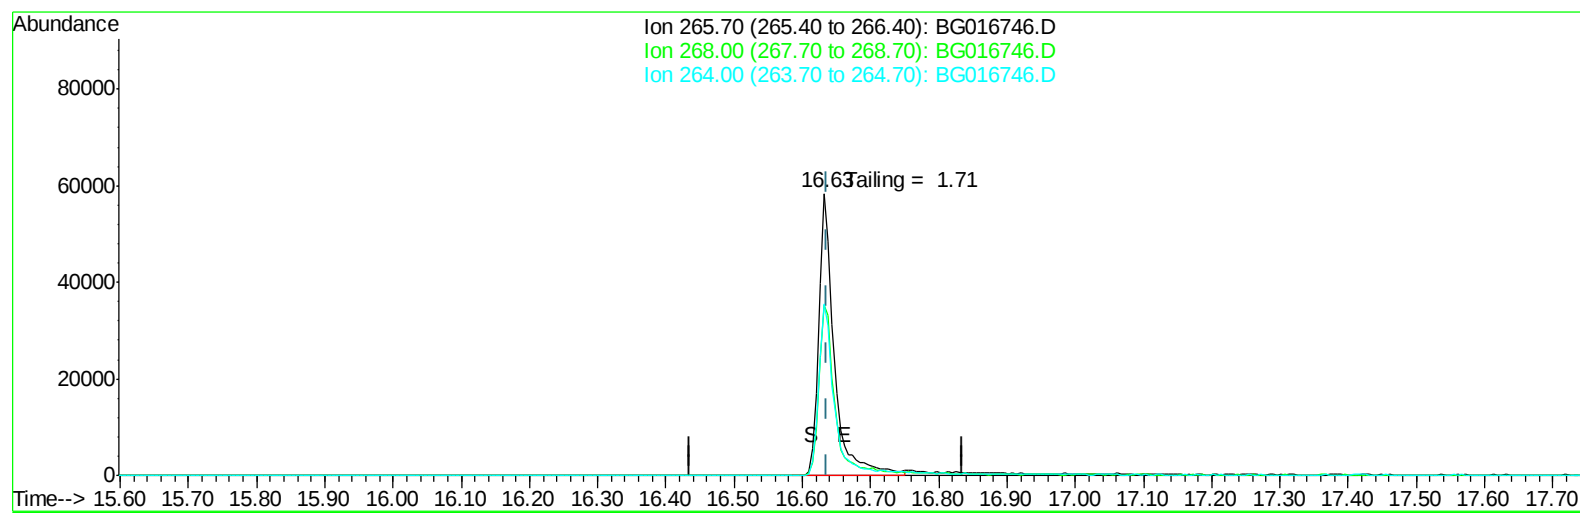

TIC: BG016746.D

(69) Pentachlorophenol (C)



16.632min (-0.004) 44827.88ng

response 92598

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	60.42
264.00	64.70	60.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042715\
 Data File : BG016746.D
 Acq On : 28 Apr 2015 00:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:56:07 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 01:49:03 2015
 Response via : Initial Calibration

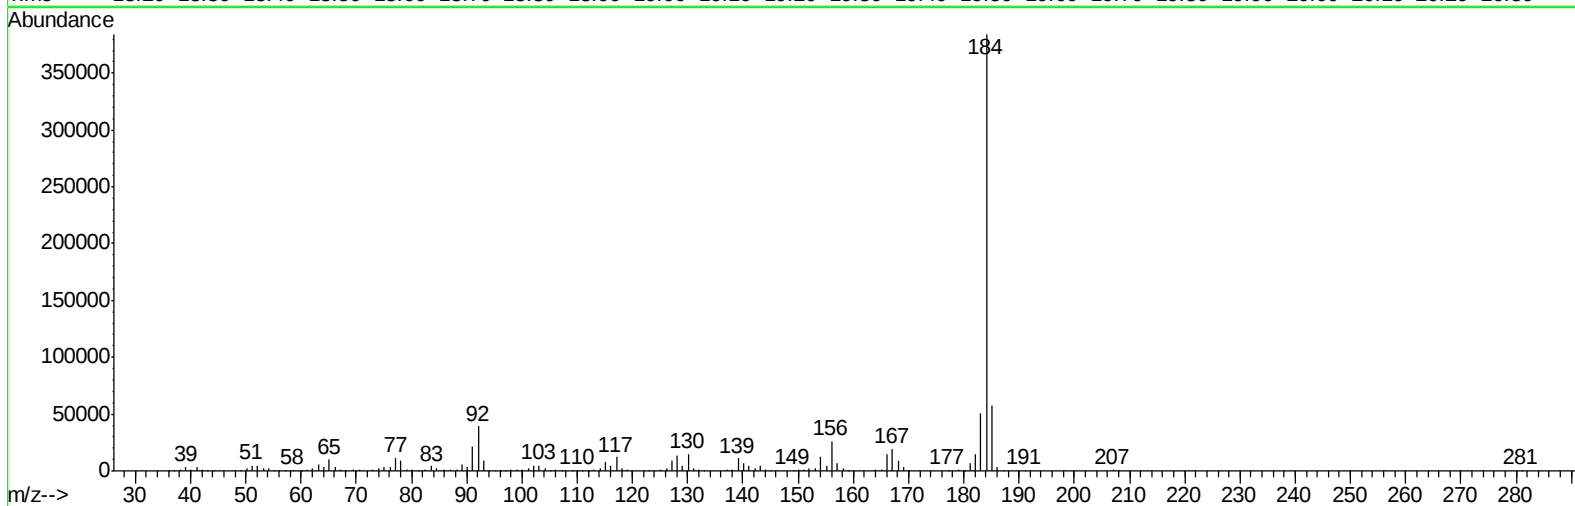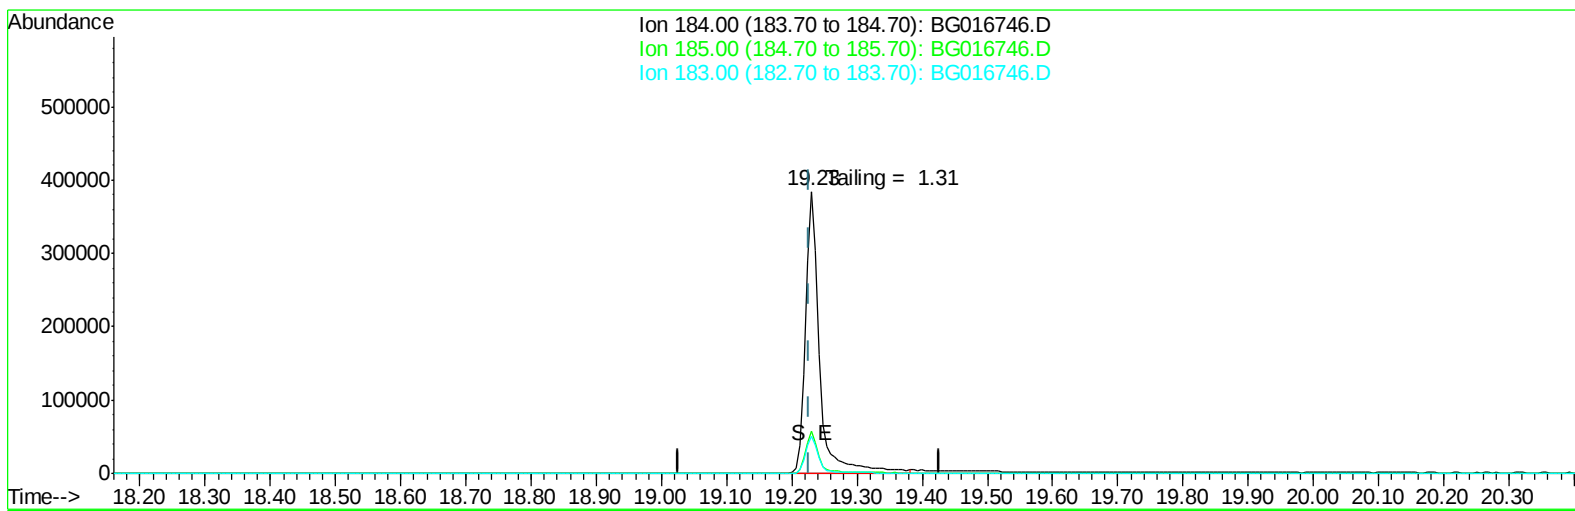

TIC: BG016746.D

(76) Benzidine

19.229min (+0.002) 19412.19ng

response 587108

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.96
183.00	12.60	13.11
0.00	0.00	0.00