


Data Path : Z:\HPCHEM1\BNA G\Data\BG042715\
 Data File : BG016729.D
 Acq On : 27 Apr 2015 10:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 19:19:11 2015

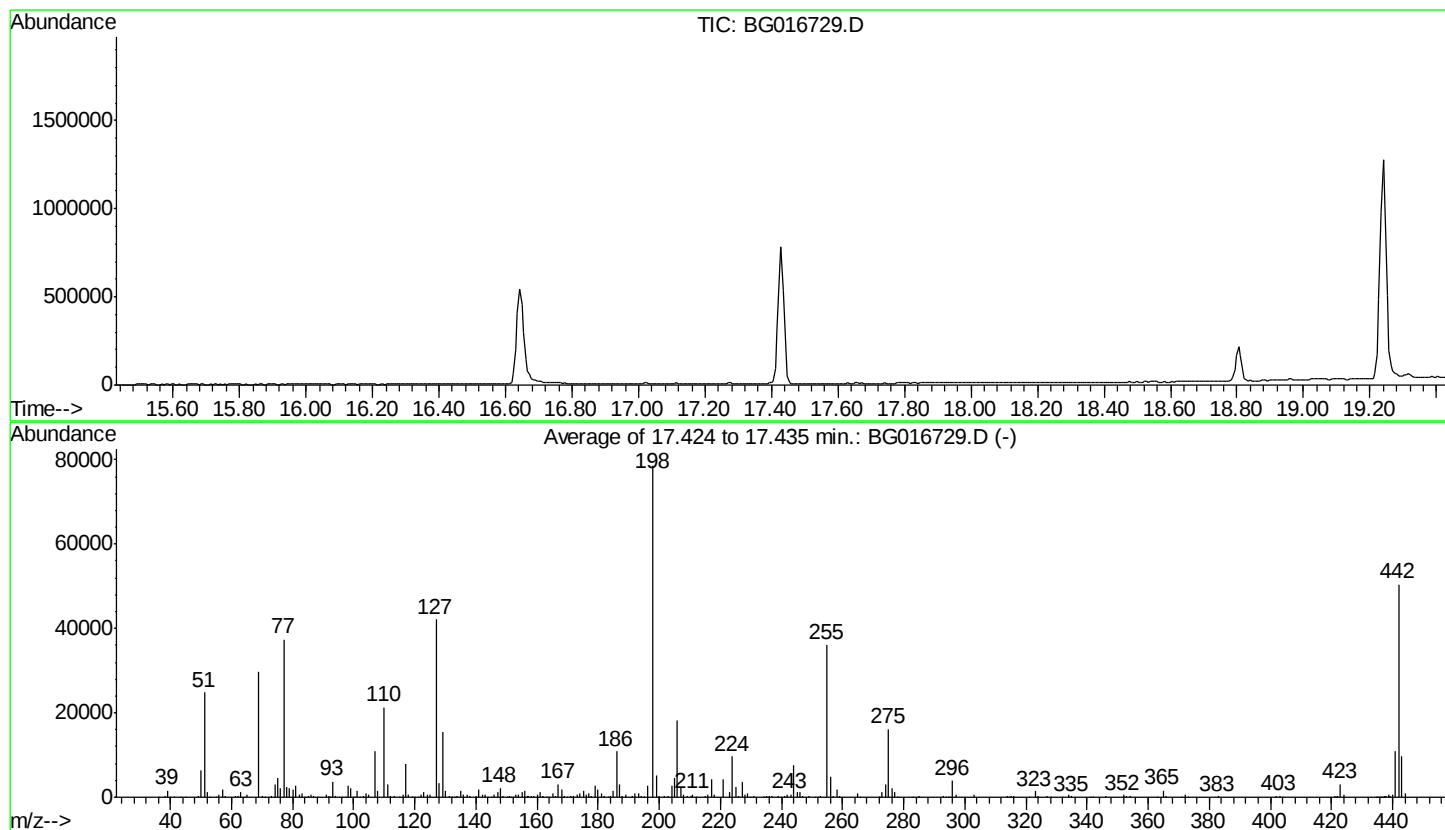

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	24879	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.7	29625	PASS
70	69	0.00	2	0.9	274	PASS
127	198	10	80	53.6	42101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78608	PASS
199	198	5	9	6.8	5317	PASS
275	198	10	60	20.6	16174	PASS
365	198	1	100	2.0	1576	PASS
441	442	0.01	24	21.8	10991	PASS
442	198	50	100	64.2	50453	PASS
443	442	15	24	19.1	9619	PASS