

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\
Quantitation Report (Qedit)




Data File : BG026725.D
Acq On : 27 Apr 2017 23:15
Operator : SJ/MA
Sample : I2807-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 28 01:48:27 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:45:47 2017
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
JHT69

Manual Integrations
APPROVED

mohammad
4/28/2017 1:44:28 PM

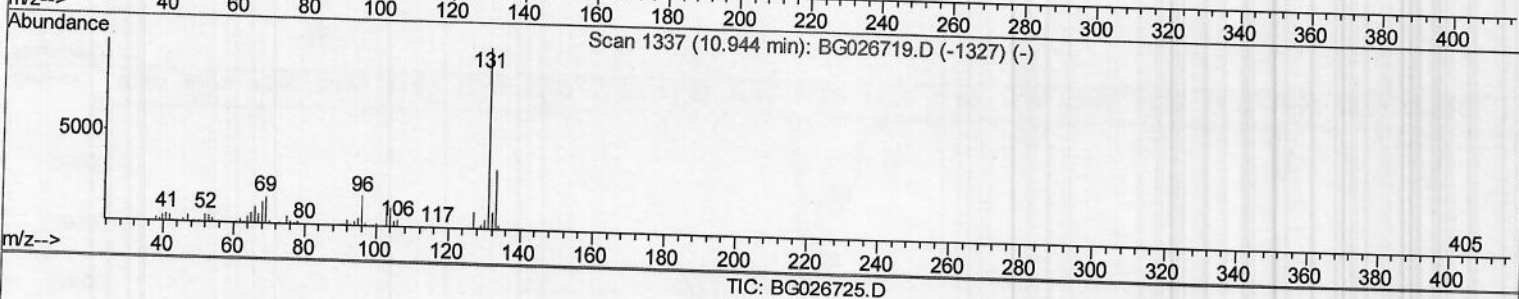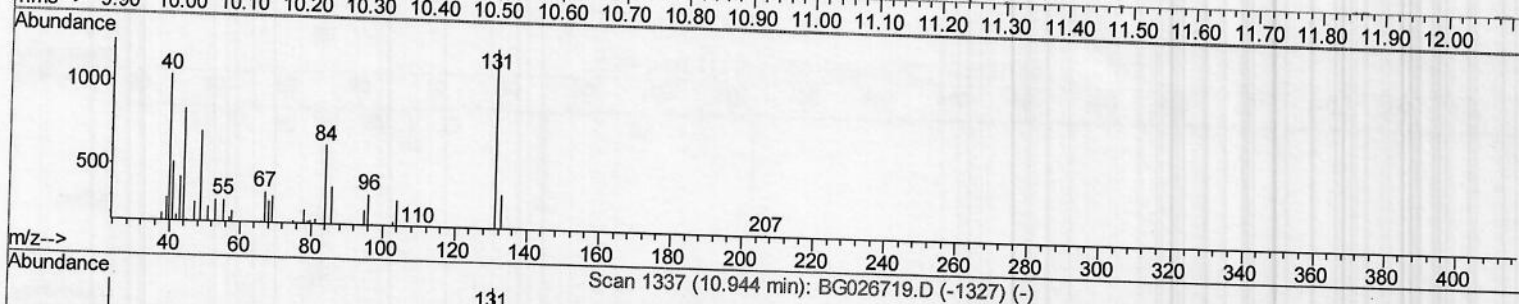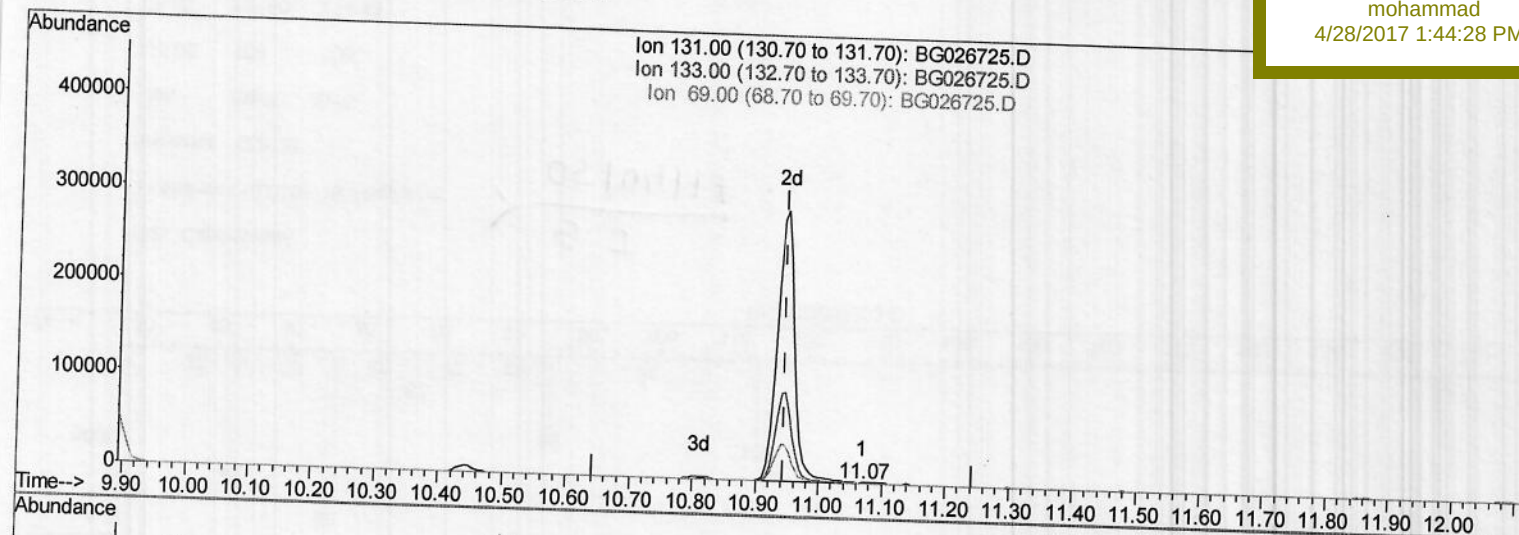

(29) 4-Chloroaniline-d4 (S)

11.069min (+0.126) 0.09ng/ul

response 1498

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	29.06
69.00	23.80	25.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\
Quantitation Report (Qedit)




Data File : BG026725.D
Acq On : 27 Apr 2017 23:15
Operator : SJ/MA
Sample : I2807-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 28 01:48:27 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:45:47 2017
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
JHT69

Manual Integrations
APPROVED

mohammad
4/28/2017 1:44:28 PM

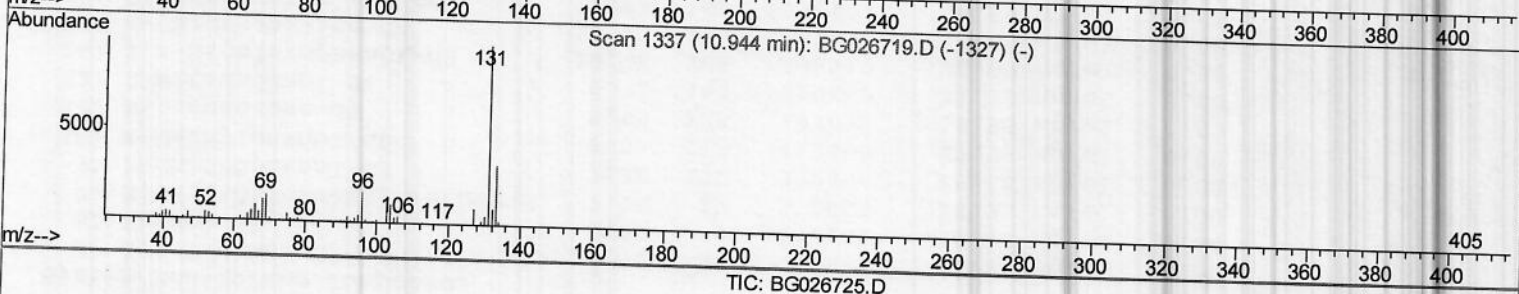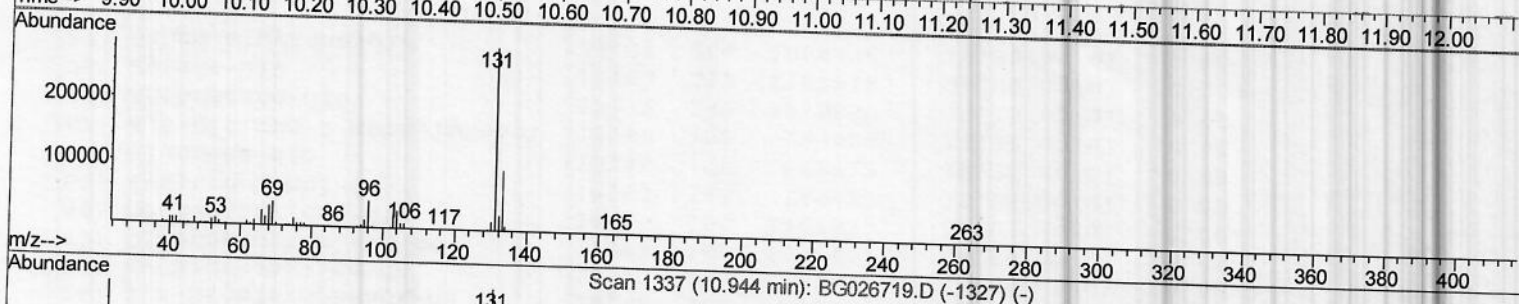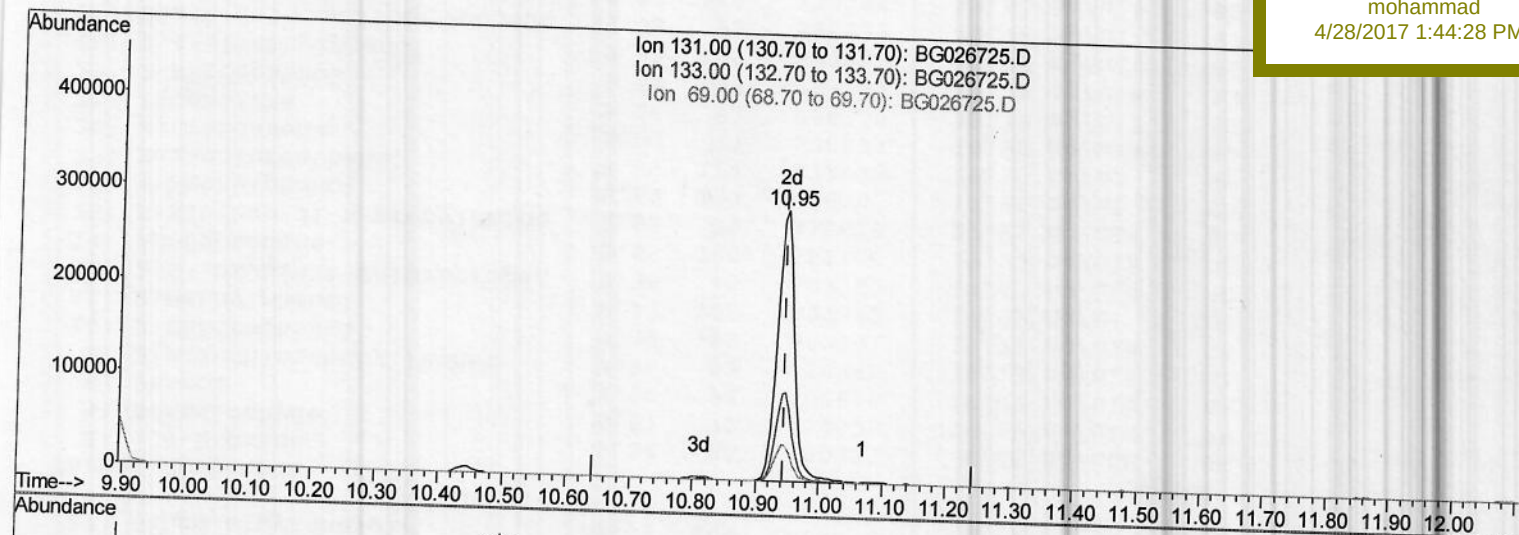

(29) 4-Chloroaniline-d4 (S)

10.946min (+0.002) 35.27ng/ul m

response 557498

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	32.77
69.00	23.80	13.40#
0.00	0.00	0.00

> $\frac{5.7}{05104117}$

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\
 Quantitation Report (QT Reviewed)

Data File : BG026725.D
 Acq On : 27 Apr 2017 23:15
 Operator : SJ/MA
 Sample : I2807-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 Client Sampled :
 JHT69

Quant Time: Apr 28 02:32:02 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 01:45:47 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 4/28/2017 1:44:28 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	171196	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	817551	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	453056	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	870111	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	771008	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	802355	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	17858	4.70	ng/uL	0.00
5) Phenol-d5	7.19	99	449317	29.41	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.33	67	270034	30.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	377698	29.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	401951	31.70	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	205884	30.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	235327	31.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	360465	30.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	557498m	35.27	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1189043	32.61	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1516030	33.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	213764	32.52	ng/ul	0.00
57) Fluorene-d10	15.61	176	1056278	33.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	167901	31.78	ng/ul	0.00
70) Anthracene-d10	17.46	188	1488602	35.25	ng/ul	0.00
76) Pyrene-d10	19.74	212	1436356	35.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1388381	36.60	ng/ul	0.00

> 5.1
 05/04/17

Target Compounds

44) Dimethylphthalate	14.07	163	223573	6.26	ng/ul#	95
-----------------------	-------	-----	--------	------	--------	----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\
Quantitation Report (QT Reviewed)

Data File : BG026725.D

Acq On : 27 Apr 2017 23:15

Operator : SJ/MA

Sample : I2807-06

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 28 02:32:02 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 01:45:47 2017

Response via : Initial Calibration

Instrument :

BNA_G

ClientSampleId :

JHT69

Manual Integrations
APPROVED

mohammad
4/28/2017 1:44:28 PM

