

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\

Quantitation Report (Qedit)

Data File : BG026732.D

Acq On : 28 Apr 2017 3:47

Operator : SJ/MA

Sample : I2807-14

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 28 04:40:48 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 01:45:47 2017

Response via : Initial Calibration

Instrument :

BNA_G

ClientSampleId :




JHSN4

Manual Integrations

APPROVED

mohammad

4/28/2017 1:44:42 PM

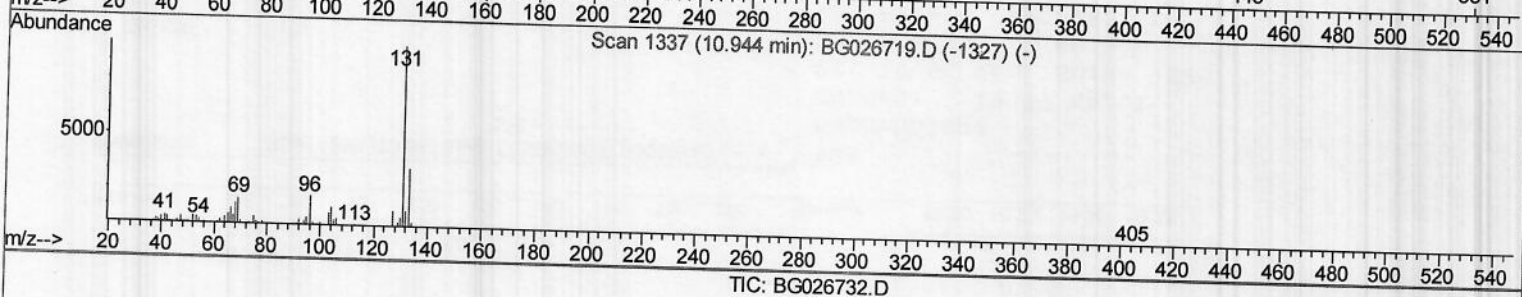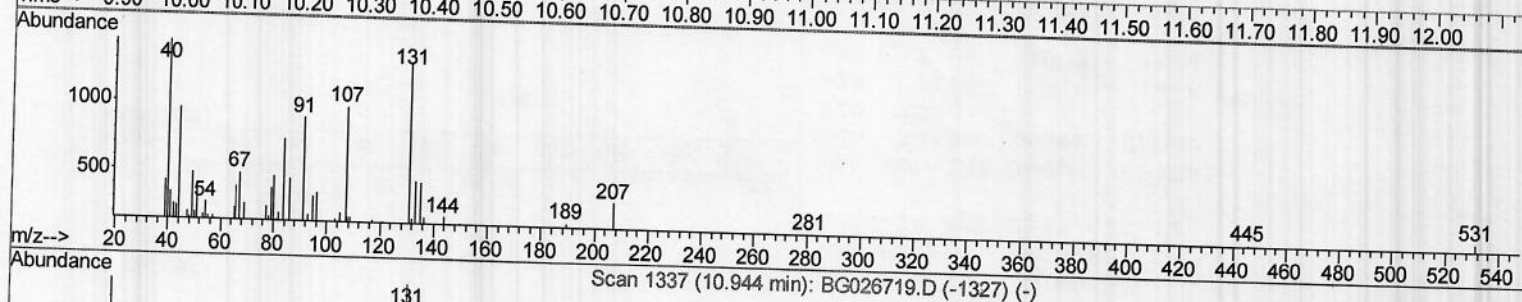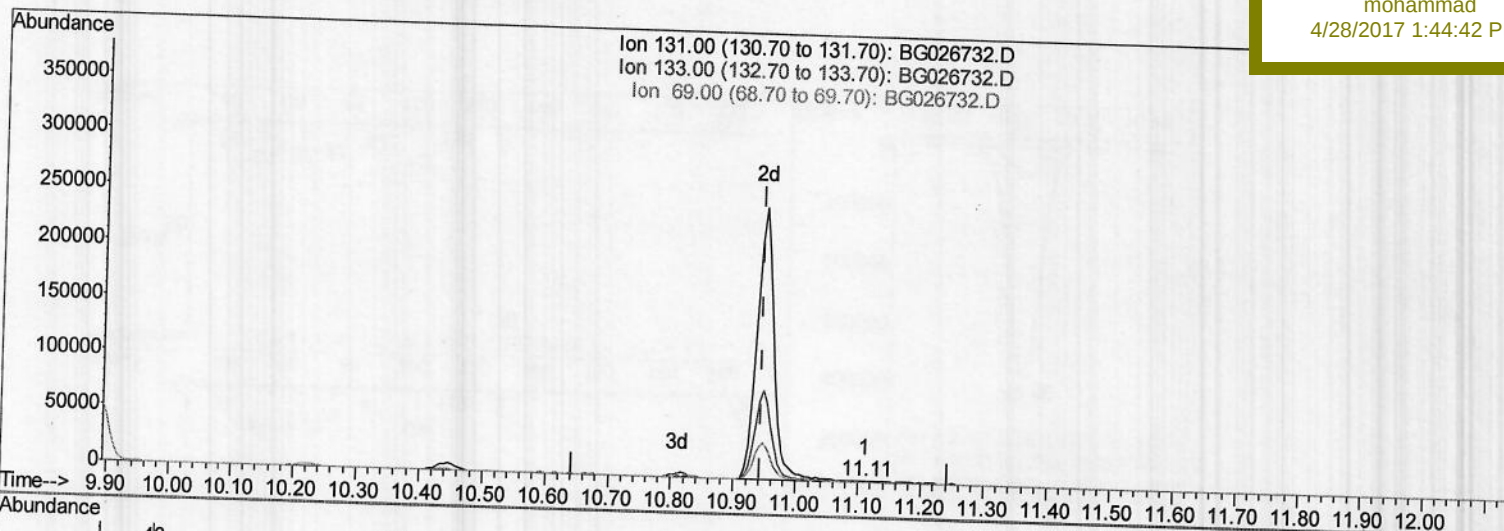

(29) 4-Chloroaniline-d4 (S)

11.110min (+0.166) 0.09ng/ul

response 1297

Ion	Exp%	Act%
-----	------	------

131.00	100	100
--------	-----	-----

133.00	35.40	34.45
--------	-------	-------

69.00	23.80	20.43
-------	-------	-------

0.00	0.00	0.00
------	------	------

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\

Quantitation Report (Qedit)

Data File : BG026732.D

Acq On : 28 Apr 2017 3:47

Operator : SJ/MA

Sample : I2807-14

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 28 04:40:48 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 01:45:47 2017

Response via : Initial Calibration

Instrument :

BNA_G




ClientSampleId :

JHSN4

Manual Integrations
APPROVED

mohammad

4/28/2017 1:44:42 PM

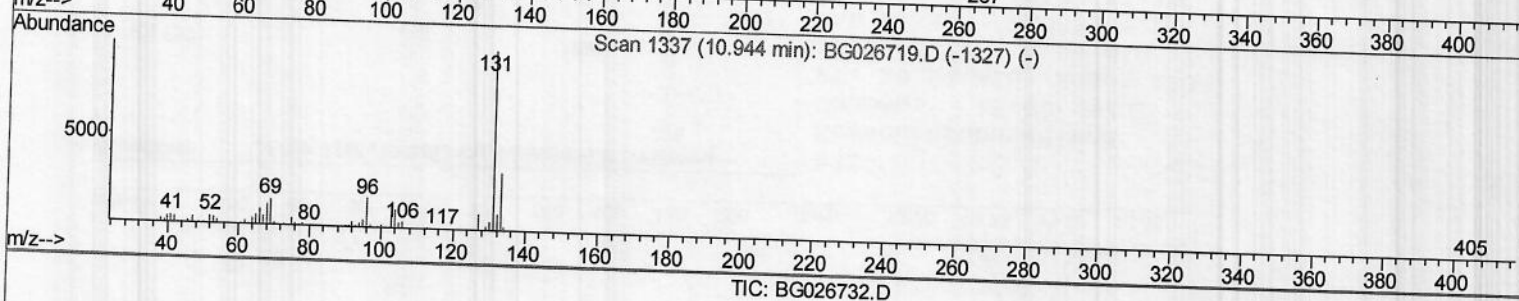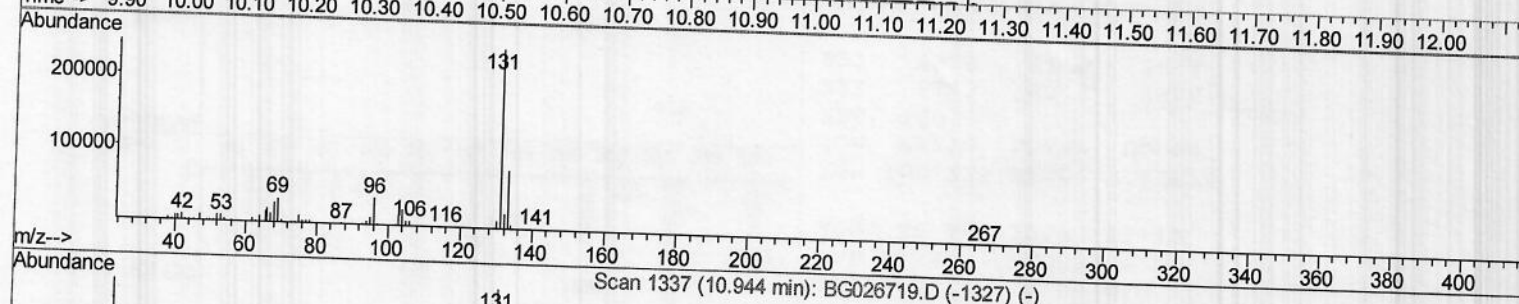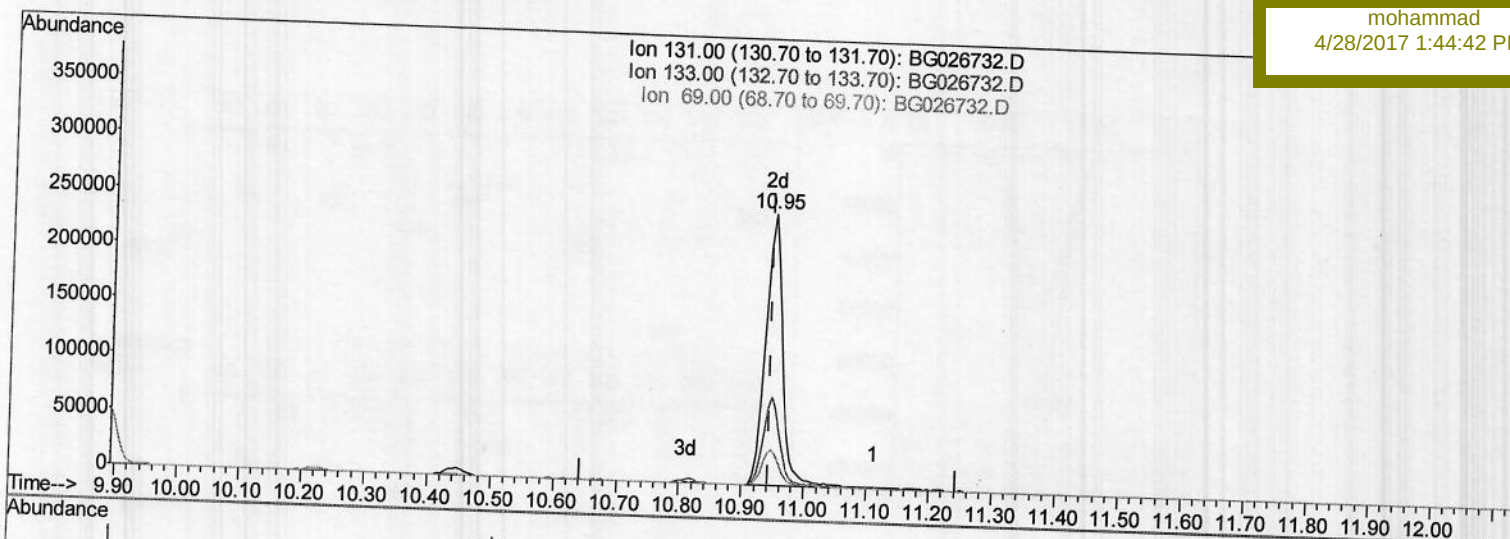

(29) 4-Chloroaniline-d4 (S)

10.946min (+0.002) 30.73ng/ul m

response 461642

Ion Exp% Act%

131.00 100 100

133.00 35.40 32.33

69.00 23.80 13.34#

0.00 0.00 0.00

> $\frac{S.J}{05104117}$

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\

Quantitation Report

(QT Reviewed)

Data File : BG026732.D

Acq On : 28 Apr 2017 3:47

Operator : SJ/MA

Sample : I2807-14

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 28 04:41:33 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 01:45:47 2017

Response via : Initial Calibration

Instrument :

BNA_G

ClientSampleId :

JHSN4

Manual Integrations

APPROVED

mohammad

4/28/2017 1:44:42 PM

Internal Standards

R.T. QIon Response Conc Units Dev(Min)

1) 1,4-Dichlorobenzene-d4	8.01	152	155068	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	776848	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	437738	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	825198	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	722665	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	743456	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	18149	5.27	ng/uL	0.00
5) Phenol-d5	7.19	99	447776	32.36	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.33	67	256729	31.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	363177	30.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	381938	33.25	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	196646	30.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	229140	32.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	363206	32.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	461642m	30.73	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1112204	31.57	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1422368	32.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	170283	26.81	ng/ul	0.00
57) Fluorene-d10	15.61	176	955962	31.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	152559	30.45	ng/ul	0.00
70) Anthracene-d10	17.46	188	1302615	32.53	ng/ul	0.00
76) Pyrene-d10	19.74	212	1212516	31.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1169782	33.28	ng/ul	0.00

Target Compounds

44) Dimethylphthalate	14.07	163	243552	7.06	ng/ul	Qvalue 99
-----------------------	-------	-----	--------	------	-------	--------------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> 5.3
05/04/17

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042717\

Quantitation Report

(QT Reviewed)

Data File : BG026732.D

Acq On : 28 Apr 2017 3:47

Operator : SJ/MA

Sample : I2807-14

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 28 04:41:33 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 01:45:47 2017

Response via : Initial Calibration

Instrument :

BNA_G

ClientSampleId :

JHSN4

Manual Integrations

APPROVED

mohammad

4/28/2017 1:44:42 PM

