

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
 Data File : BG026727.D
 Acq On : 28 Apr 2017 00:33
 Operator : SJ/MA
 Sample : I2807-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT71

Quant Time: Apr 28 01:49:27 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 01:45:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	169512	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	823739	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	453367	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	862882	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	763511	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	788994	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	19914	5.29	ng/uL	0.00
5) Phenol-d5	7.19	99	477677	31.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	278656	31.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	404287	31.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	423819	33.75	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	213110	30.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	245923	32.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	385341	32.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	578969	36.35	ng/ul	0.00
43) Dimethylphthalate-d6	14.03	166	1143621	31.34	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1483472	32.36	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	142194	21.62	ng/ul	0.00
57) Fluorene-d10	15.61	176	994680	31.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	123761	23.62	ng/ul	0.00
70) Anthracene-d10	17.46	188	1378101	32.91	ng/ul	0.00
76) Pyrene-d10	19.74	212	1304317	32.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1266290	33.95	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.07	163	205396	5.75	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
Data File : BG026727.D
Acq On : 28 Apr 2017 00:33
Operator : SJ/MA
Sample : I2807-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT71

Quant Time: Apr 28 01:49:27 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:45:47 2017
Response via : Initial Calibration

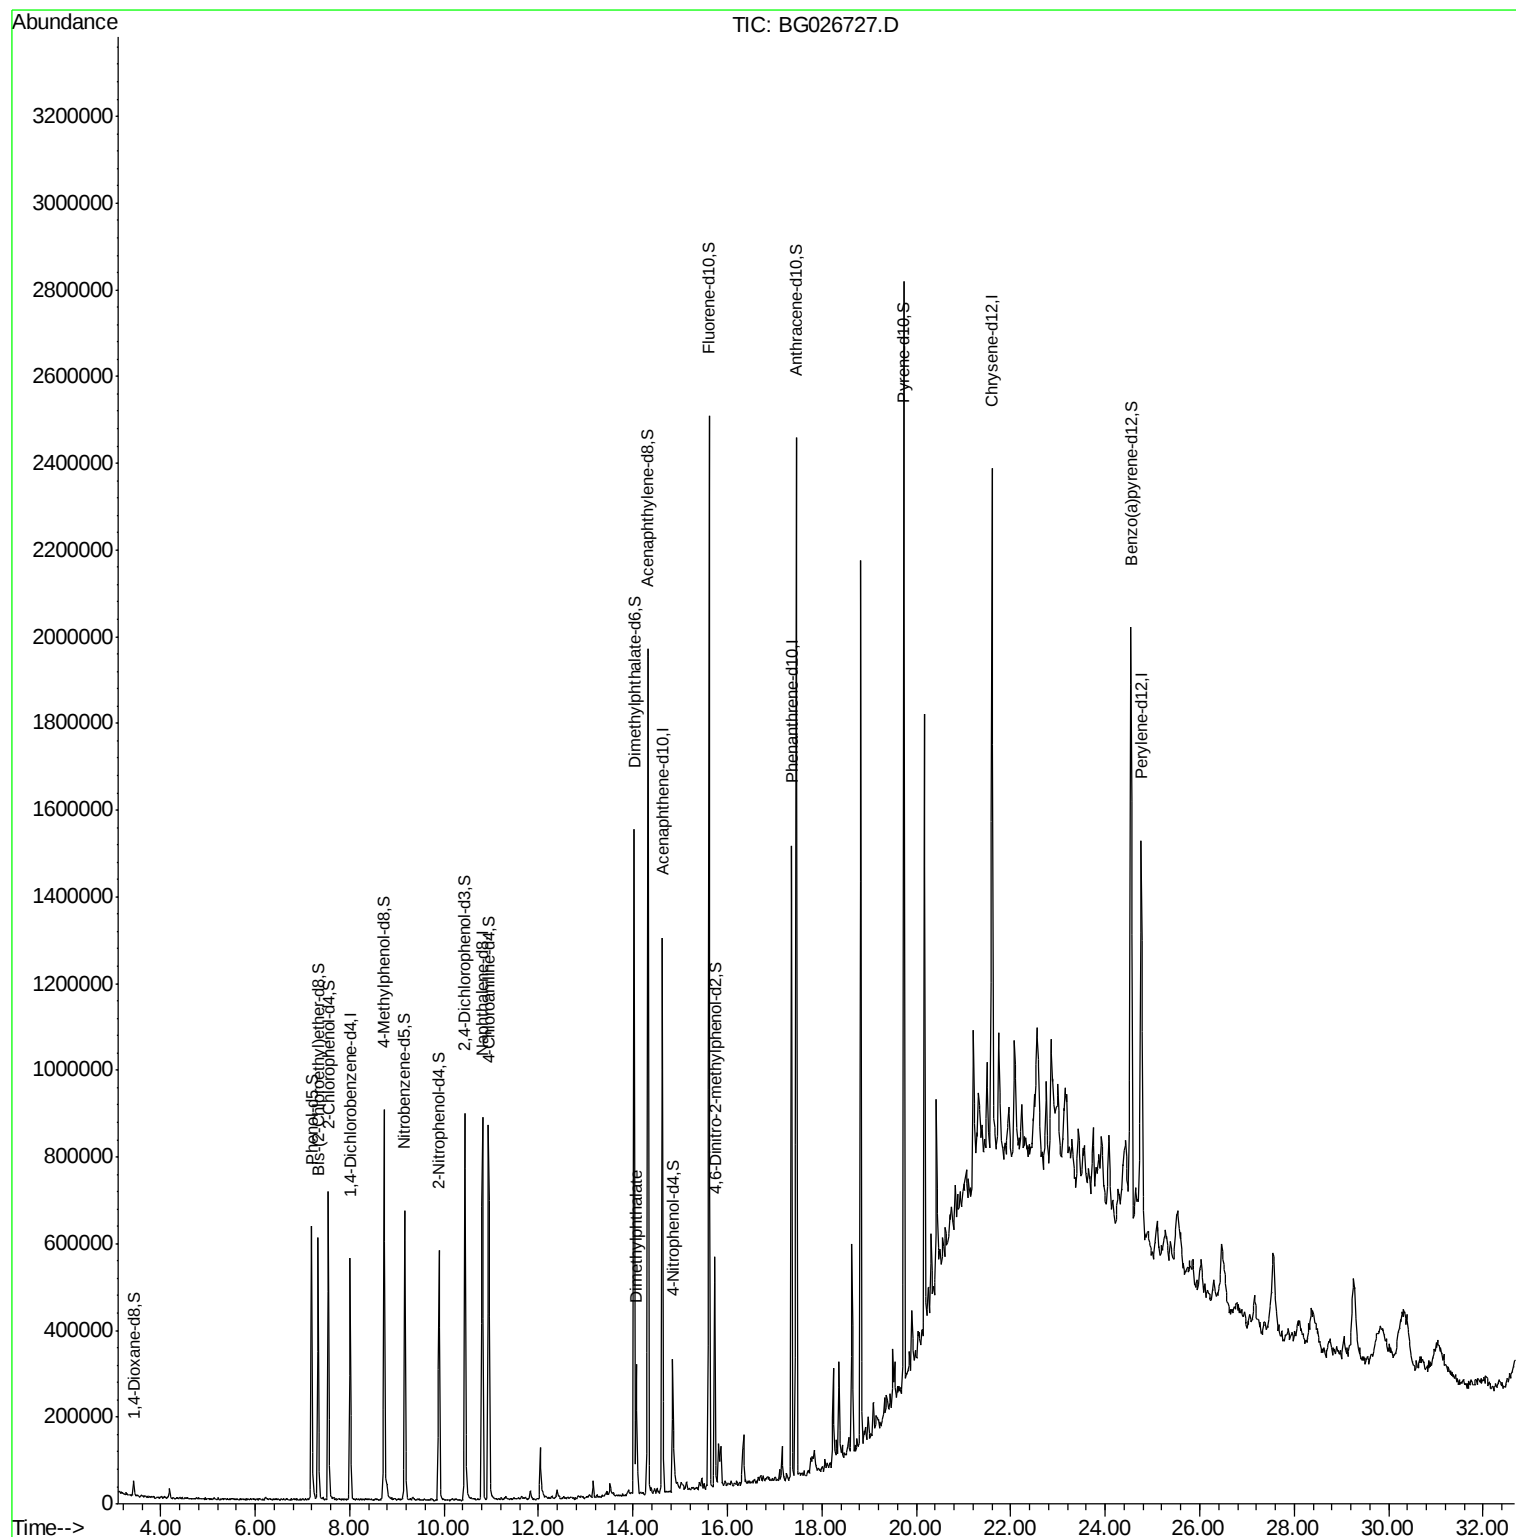

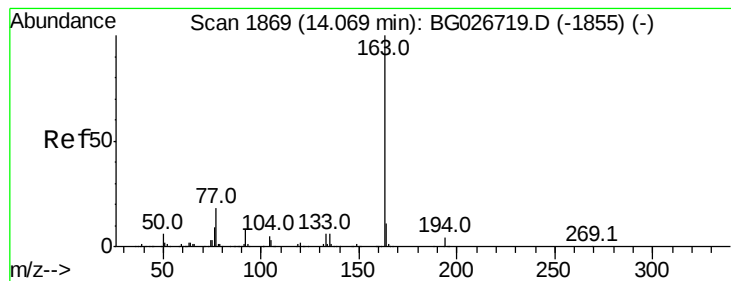

#44

Dimethylphthalate

Concen: 5.75 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. 0.00 min

Lab File: BG026727.D

Acq: 28 Apr 2017 00:33

Instrument :

BNA_G

ClientSampleId :

JHT71

Tot Ion:163 Resp: 205396

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.5 9.0 13.4

