

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
 Data File : BG026730.D
 Acq On : 28 Apr 2017 2:30
 Operator : SJ/MA
 Sample : I2807-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHSN0

Manual Integrations
 APPROVED

mohammad
 4/28/2017 1:44:38 PM

Quant Time: Apr 28 03:56:49 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 01:45:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	202274	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	951431	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	483432	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	891803	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	786774	20.00	ng/ul	0.00
83) Perylene-d12	24.79	264	800996	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	18281	4.07	ng/uL	0.00
5) Phenol-d5	7.19	99	459776	25.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	259791	24.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	379313	24.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	375286	25.05	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	197168	24.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	219628	25.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	346831	25.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	379350m	20.62	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1011847	26.00	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1304139	26.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	153989	21.96	ng/ul	0.00
57) Fluorene-d10	15.61	176	876493	25.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	114111	21.07	ng/ul	0.00
70) Anthracene-d10	17.45	188	1193615	27.58	ng/ul	0.00
76) Pyrene-d10	19.73	212	1132224	27.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.56	264	1035033	27.33	ng/ul	0.02

Target Compounds					Ovalue
44) Dimethylphthalate	14.07	163	210972	5.54 ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
Data File : BG026730.D
Acq On : 28 Apr 2017 2:30
Operator : SJ/MA
Sample : I2807-12
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHSN0

Manual Integrations
APPROVED

mohammad
4/28/2017 1:44:38 PM

Quant Time: Apr 28 03:56:49 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:45:47 2017
Response via : Initial Calibration

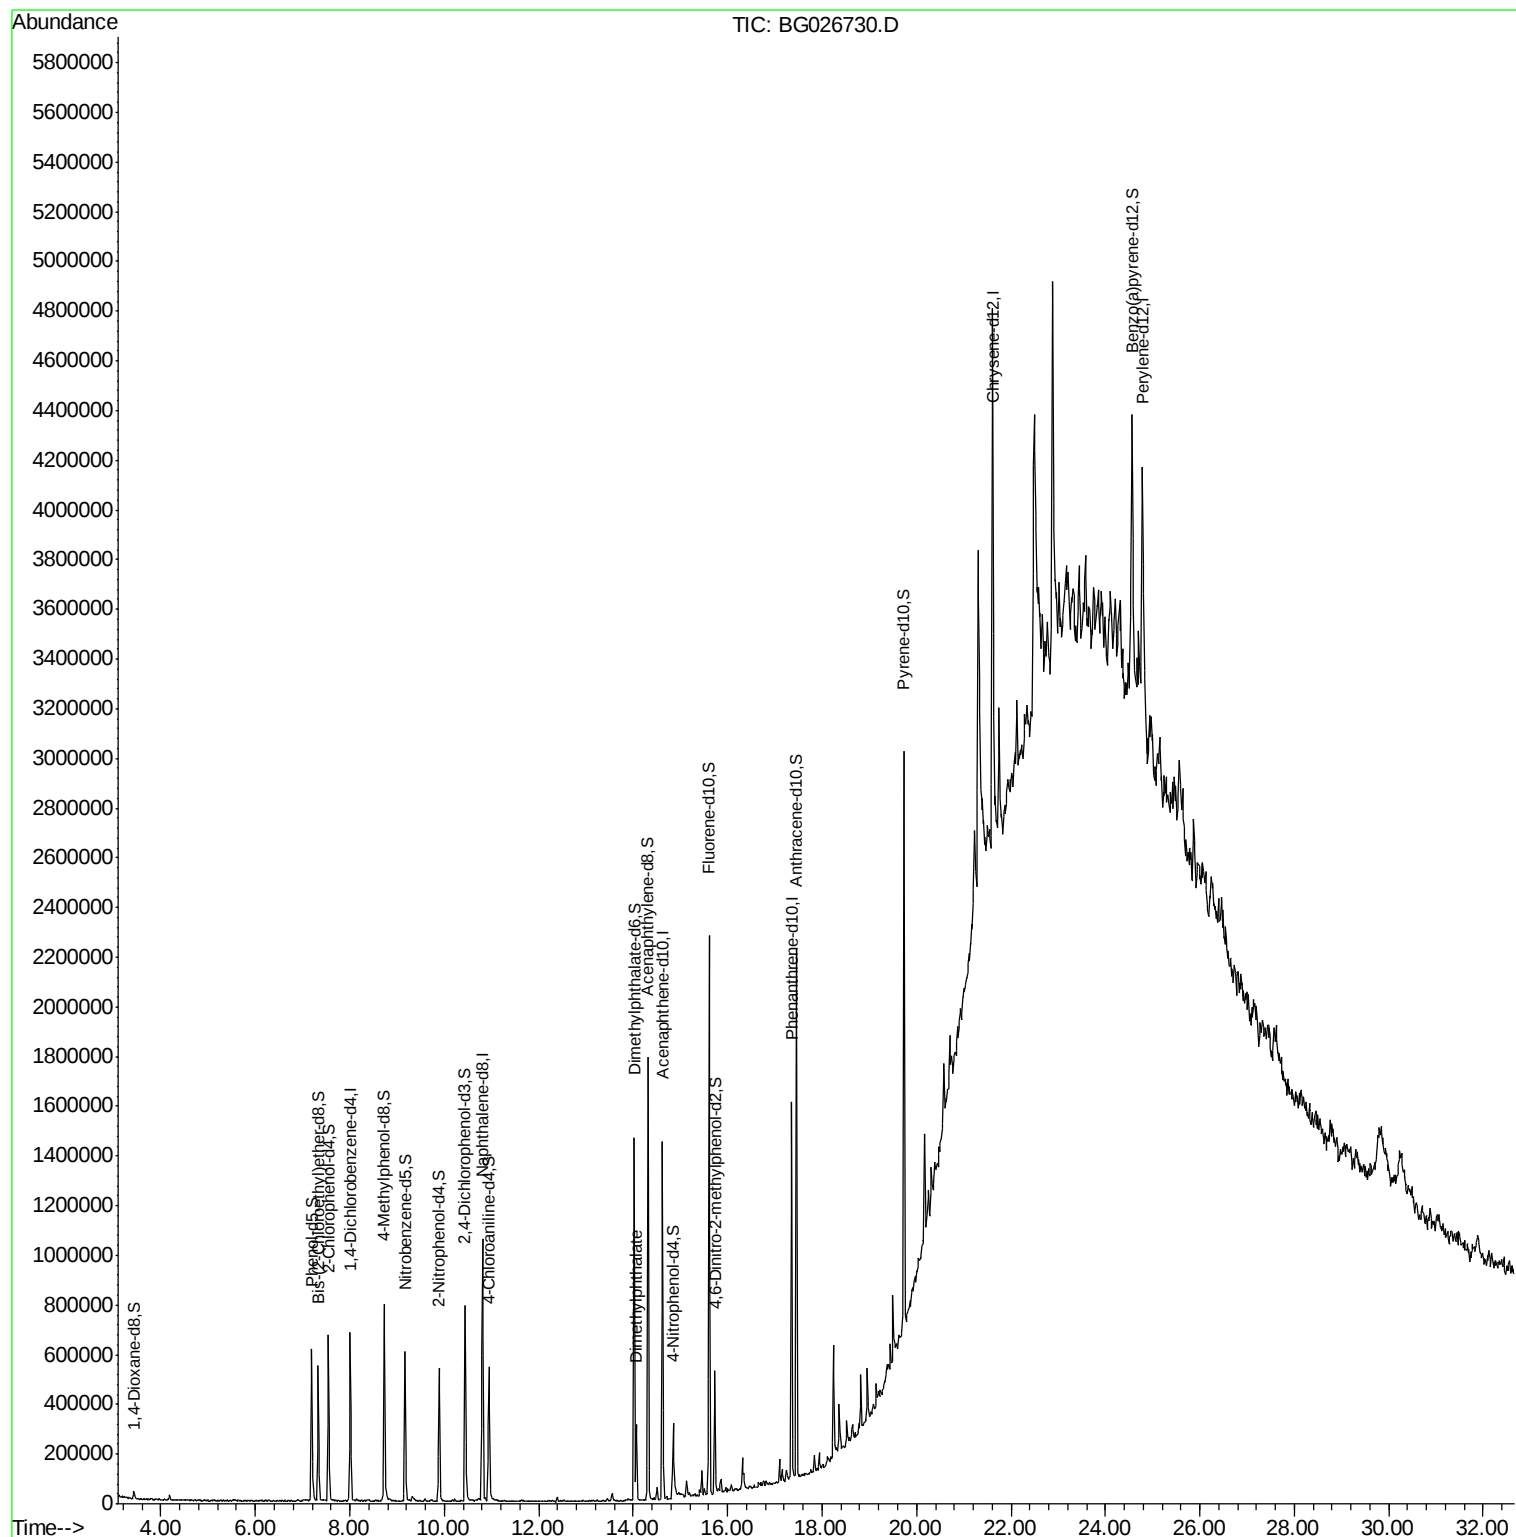

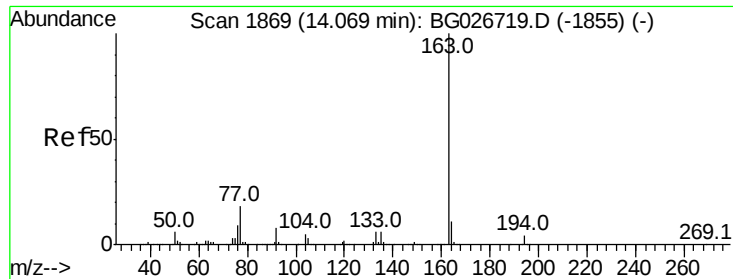

#44
 Dimethylphthalate
 Concen: 5.54 ng/ul
 RT: 14.07 min Scan# 1869
 Delta R.T. -0.00 min
 Lab File: BG026730.D
 Acq: 28 Apr 2017 2:30

Instrument :
 BNA_G
 ClientSampleId :
 JHSN0

Tot Ion:	163	Resp:	210972
Ion Ratio		Lower	Upper
163	100		
194	3.7	3.4	5.0
164	9.8	9.0	13.4

Manual Integrations
 APPROVED

mohammad
 4/28/2017 1:44:38 PM

