

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
 Data File : BG026733.D
 Acq On : 28 Apr 2017 5:05
 Operator : SJ/MA
 Sample : I2807-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHSN5

Quant Time: Apr 28 07:06:07 2017
 Quant Title :
 QLast Update : Fri Apr 28 08:38:50 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	146125	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	744921	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	426598	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	826702	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	723261	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	756811	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	19533	6.02	ng/uL	0.00
5) Phenol-d5	7.19	99	459022	35.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	256369	33.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	367622	33.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	372107	34.38	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	203351	32.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	227946	33.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	362581	33.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	568532	39.47	ng/ul	0.00
43) Dimethylphthalate-d6	14.03	166	1206584	35.14	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1511748	35.05	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	197208	31.86	ng/ul	0.00
57) Fluorene-d10	15.61	176	1039369	34.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	172259	34.31	ng/ul	0.00
70) Anthracene-d10	17.46	188	1481003	36.91	ng/ul	0.00
76) Pyrene-d10	19.74	212	1404049	36.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1373371	38.38	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.07	163	222339	6.61	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042717\
Data File : BG026733.D
Acq On : 28 Apr 2017 5:05
Operator : SJ/MA
Sample : I2807-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHSN5

Quant Time: Apr 28 07:06:07 2017
Quant Title :
QLast Update : Fri Apr 28 08:38:50 2017
Response via : Initial Calibration

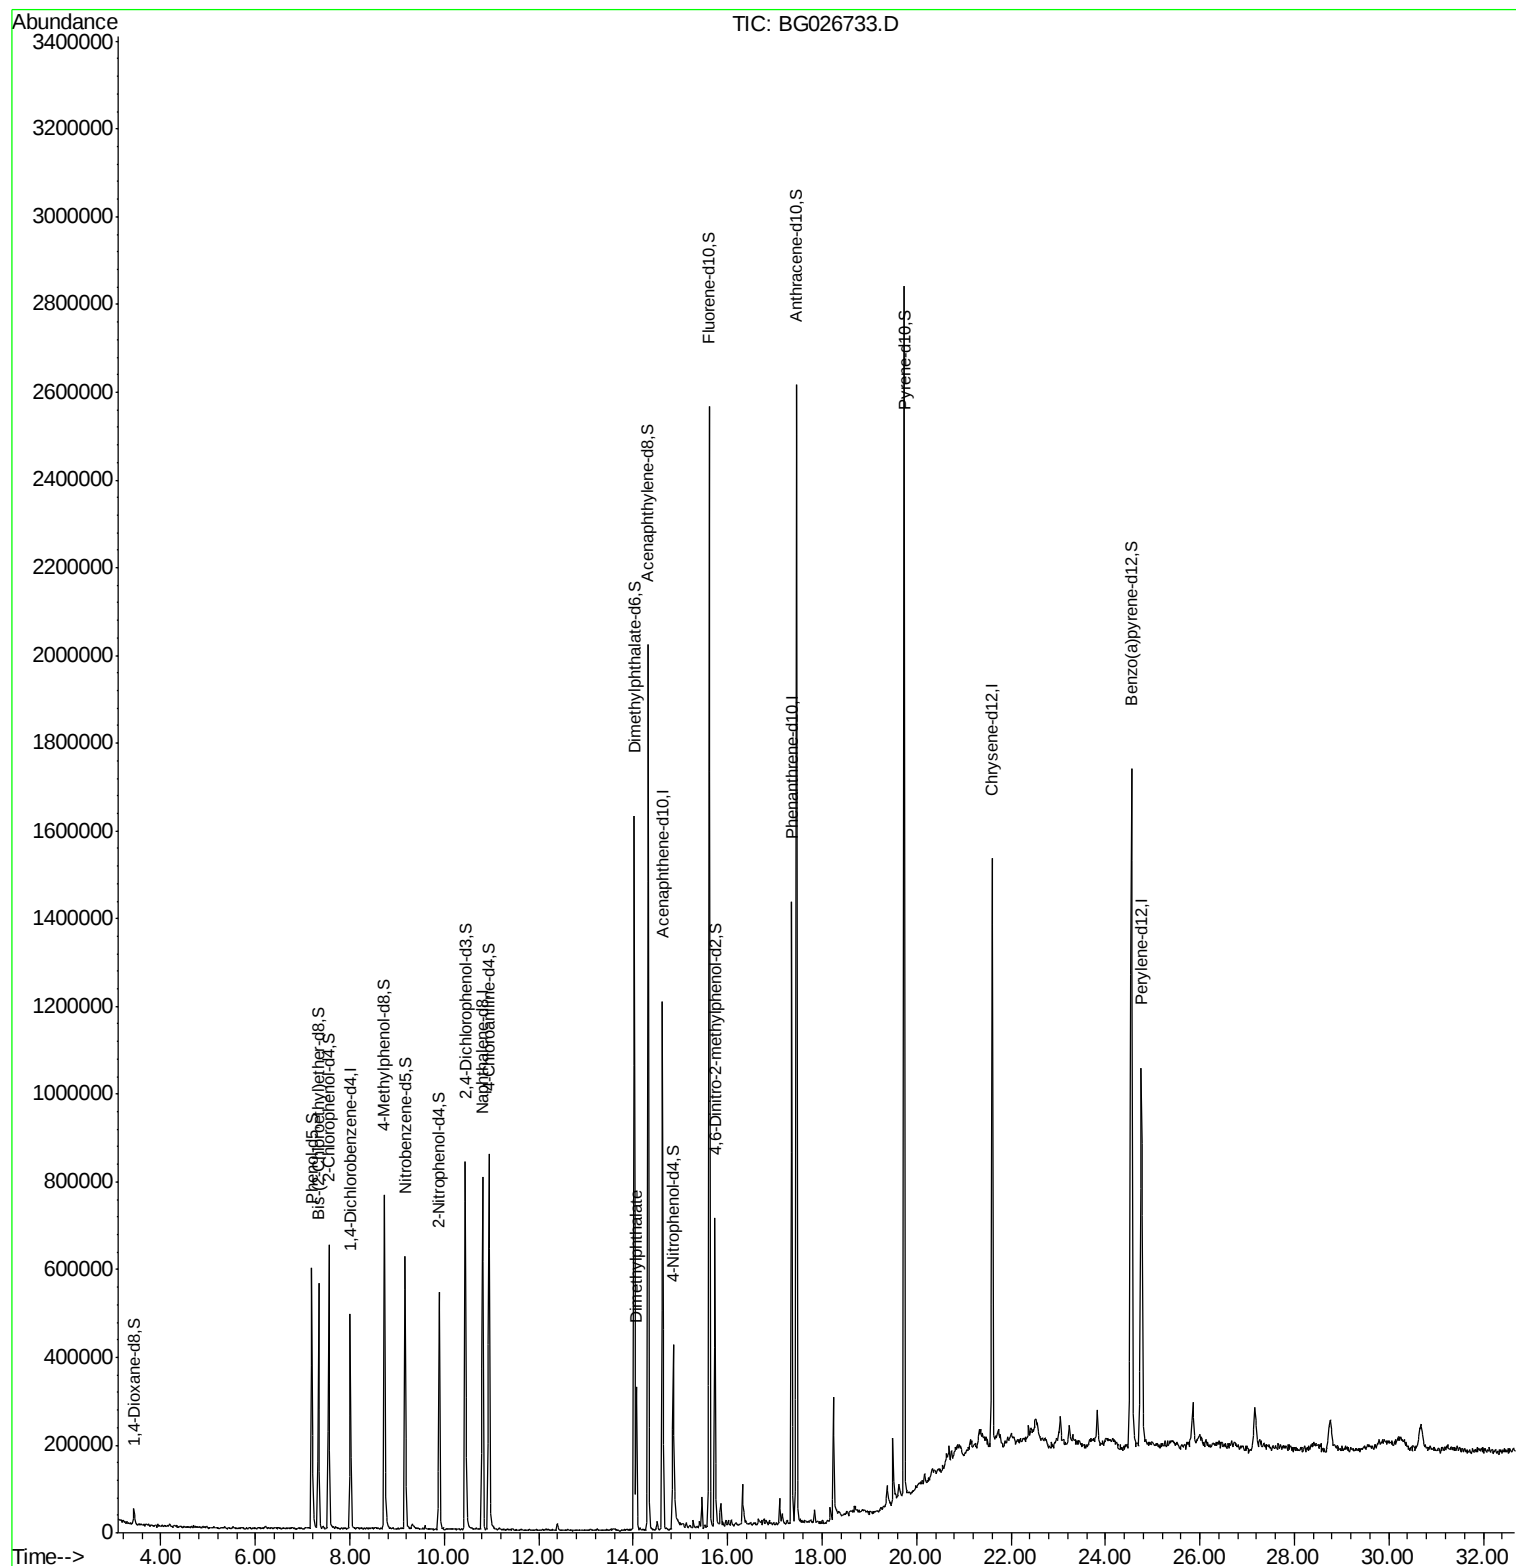

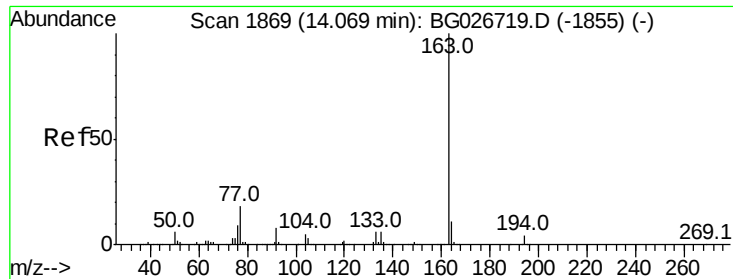

#44

Dimethylphthalate

Concen: 6.61 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG026733.D

Acq: 28 Apr 2017 5:05

Instrument :

BNA_G

ClientSampleId :

JHSN5


Tot Ion:163 Resp: 222339

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.7 9.0 13.4

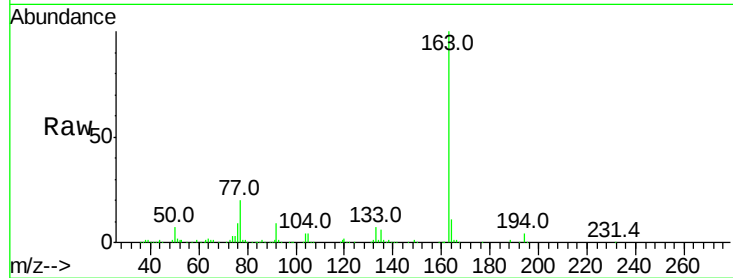

Abundance Ion 163.00 (162.70 to 163.70): E

200000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

