
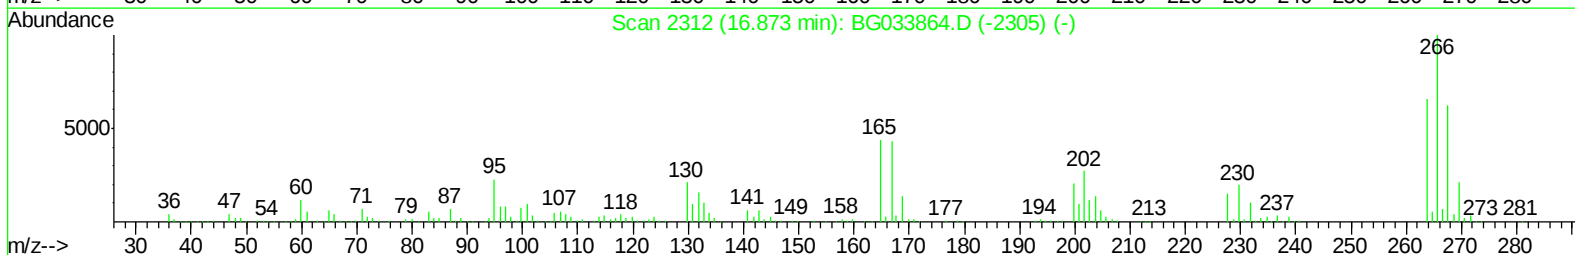
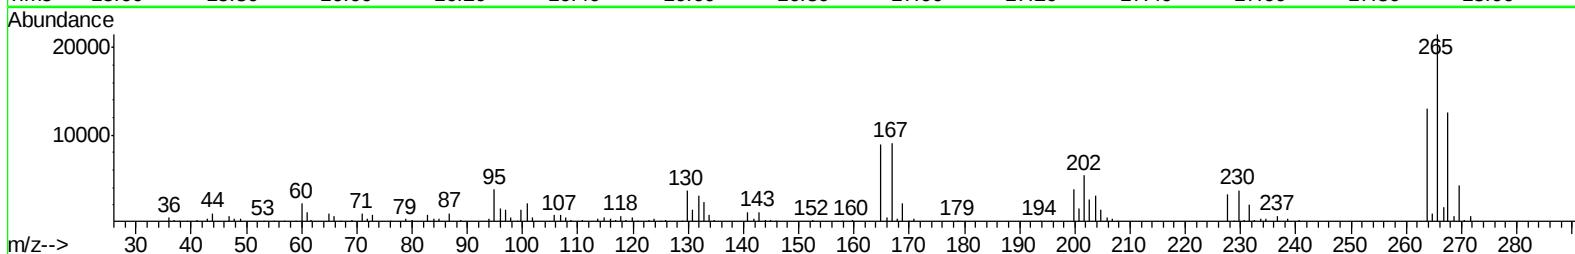


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042718\
Data File : BG034037.D
Acq On : 27 Apr 2018 13:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:57:08 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

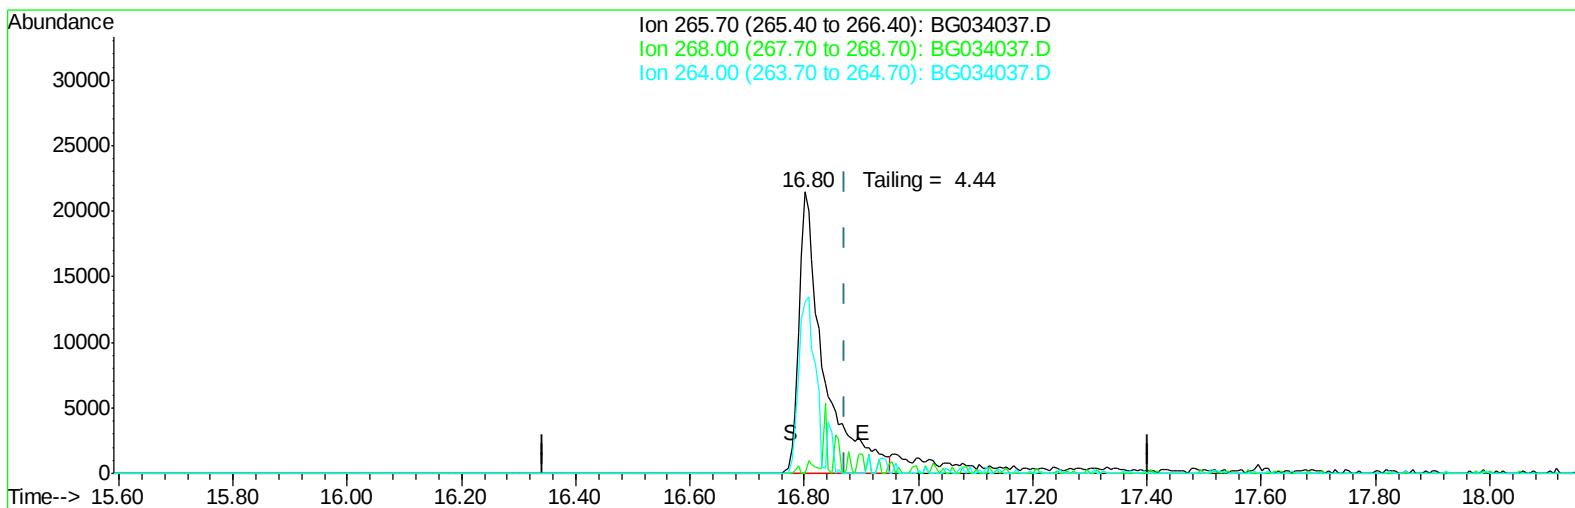

TIC: BG034037.D

(69) Pentachlorophenol (C)




16.801min (-0.072) 18724.24ng

response 64471

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	3.36#
264.00	62.00	65.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042718\
 Data File : BG034037.D
 Acq On : 27 Apr 2018 13:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:57:08 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

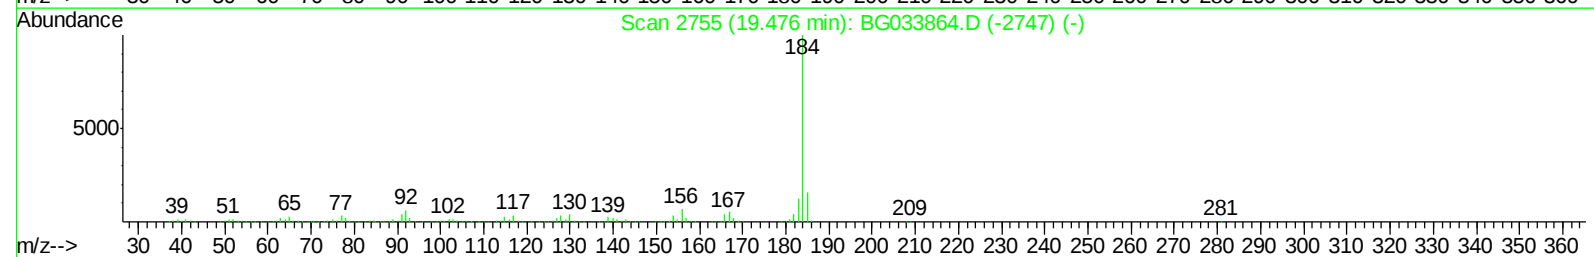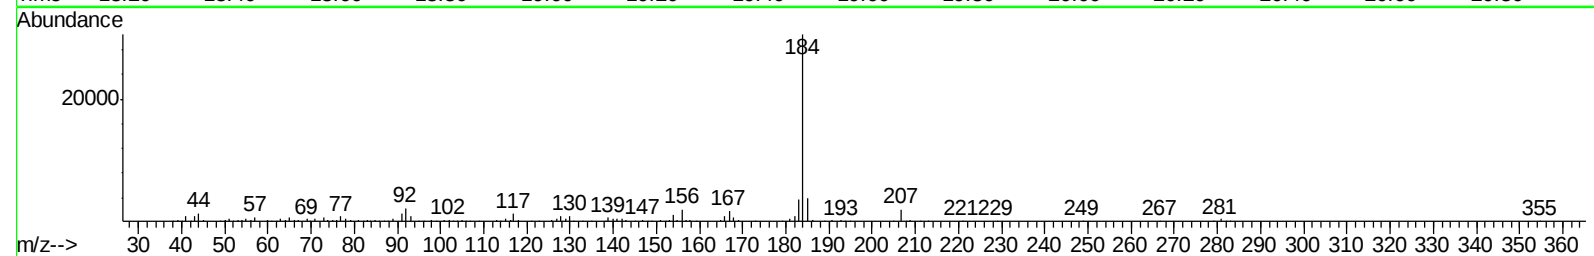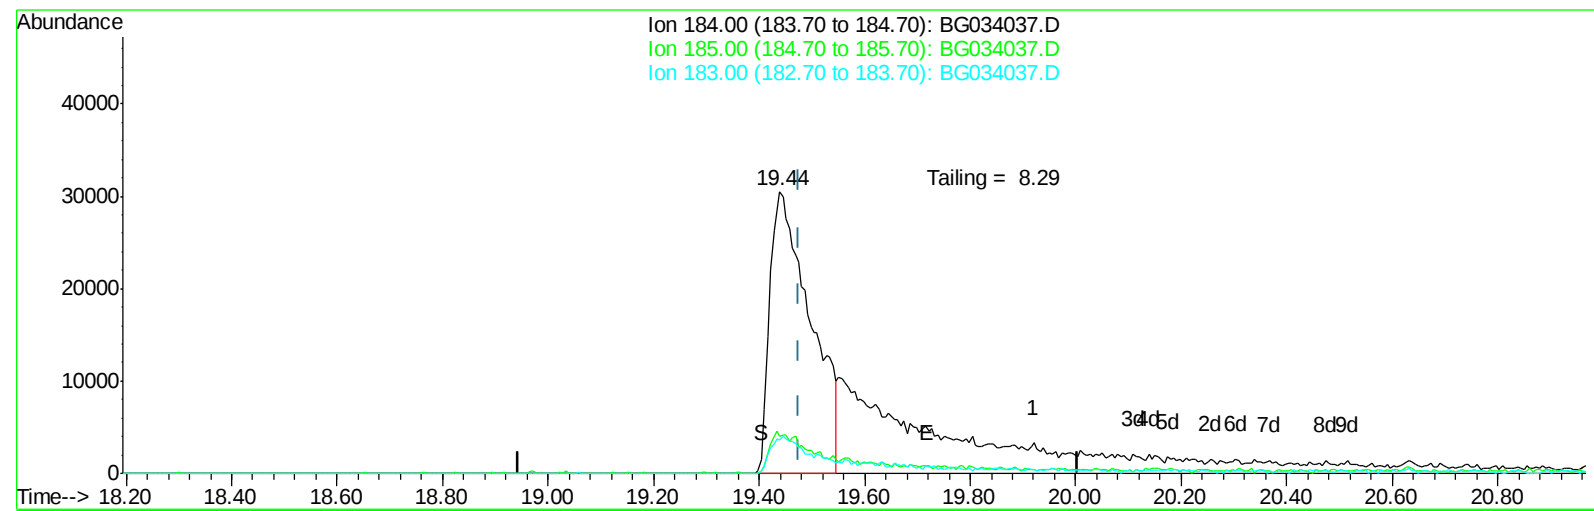

TIC: BG034037.D

(76) Benzidine

19.439min (-0.036) 90135.97ng m

response 163078

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.03
183.00	13.30	11.84
0.00	0.00	0.00