
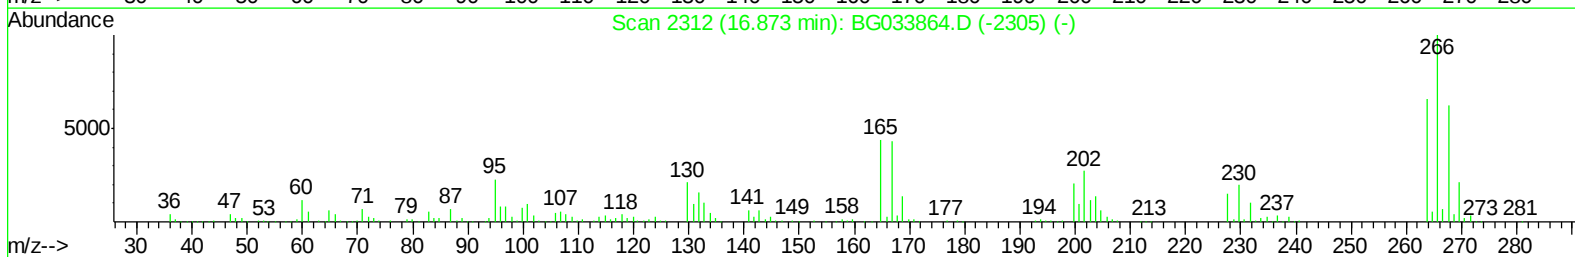
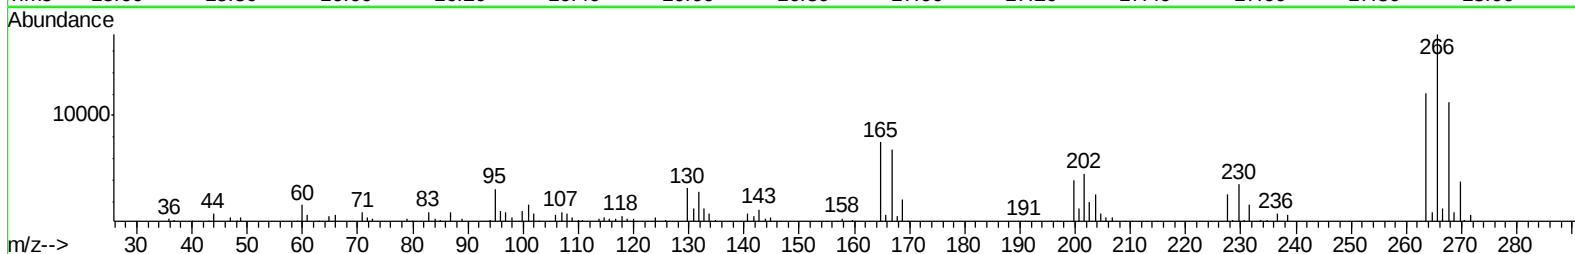


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042718\
Data File : BG034056.D
Acq On : 28 Apr 2018 3:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:59:43 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

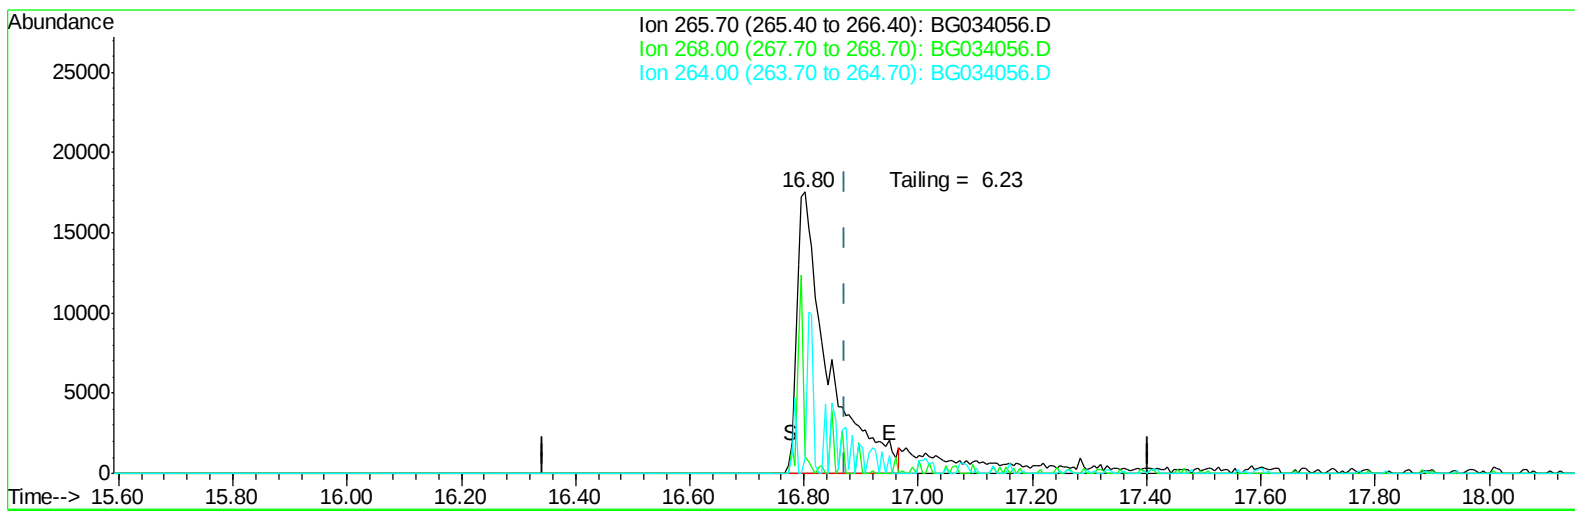

TIC: BG034056.D

(69) Pentachlorophenol (C)




16.802min (-0.071) 14087.66ng

response 65393

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	5.76#
264.00	62.00	5.59#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042718\
 Data File : BG034056.D
 Acq On : 28 Apr 2018 3:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:59:43 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

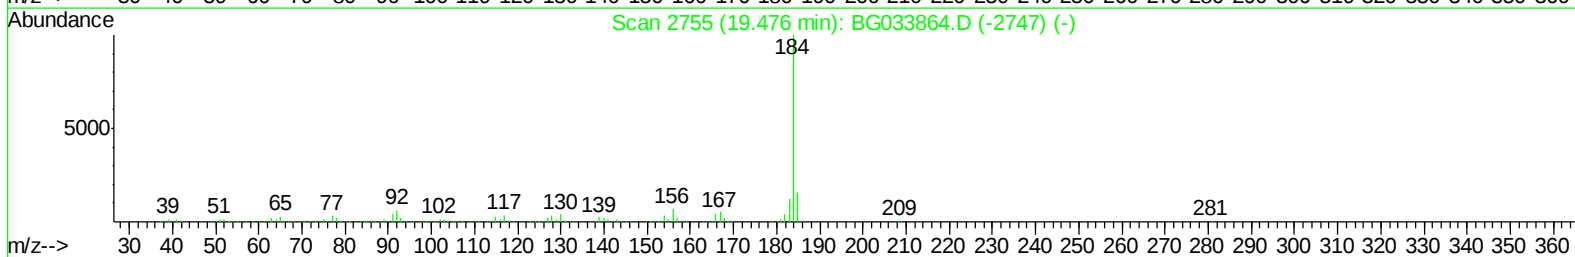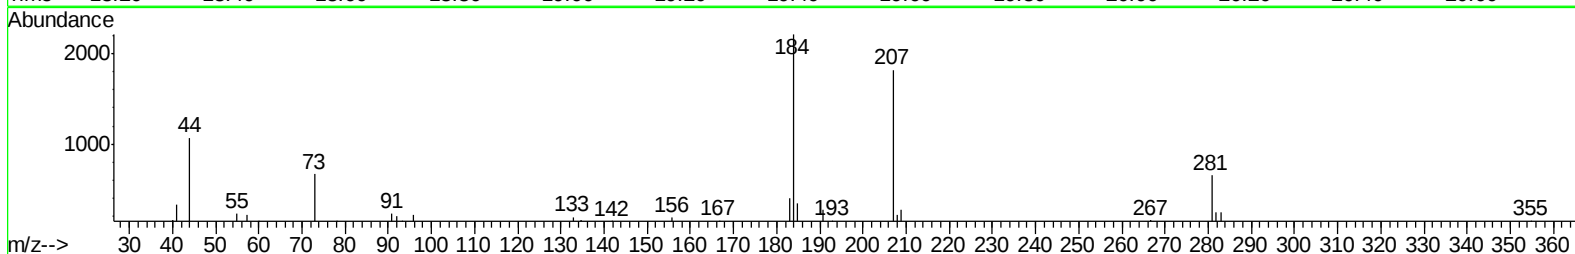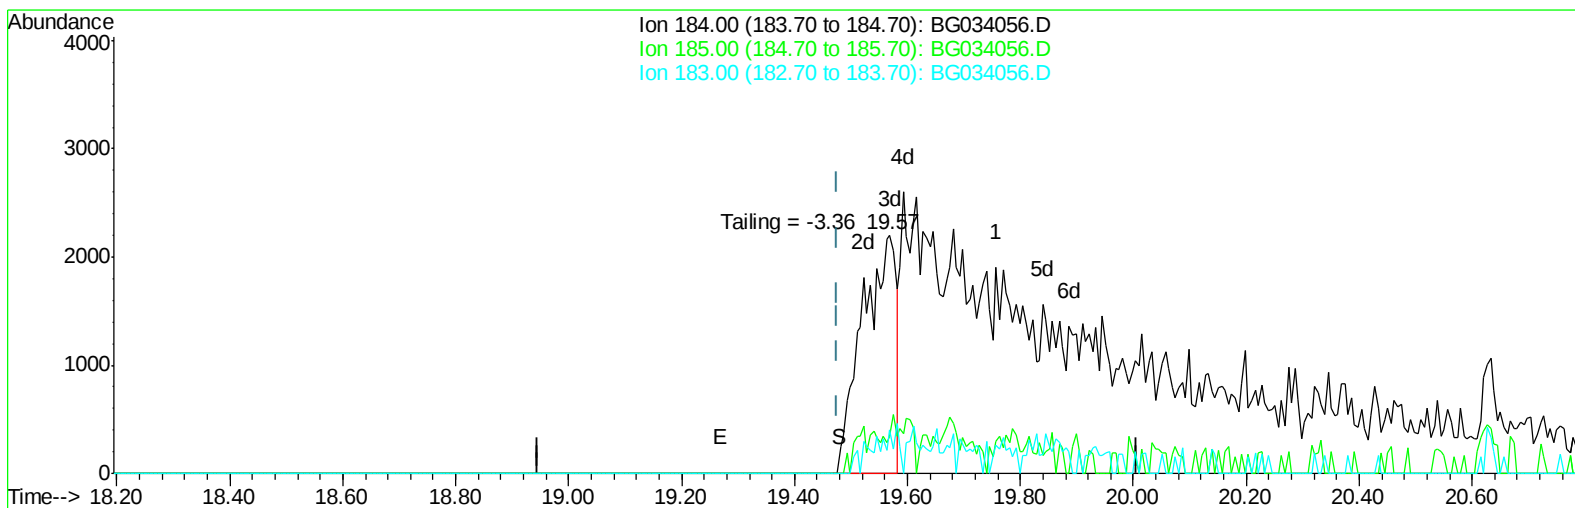

TIC: BG034056.D

(76) Benzidine

19.569min (+0.093) 0.00ng m

response 8984

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.50
183.00	13.30	18.26#
0.00	0.00	0.00