


Data Path : Z:\HPCHEM1\BNA G\Data\BG042718\
 Data File : BG034037.D
 Acq On : 27 Apr 2018 13:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

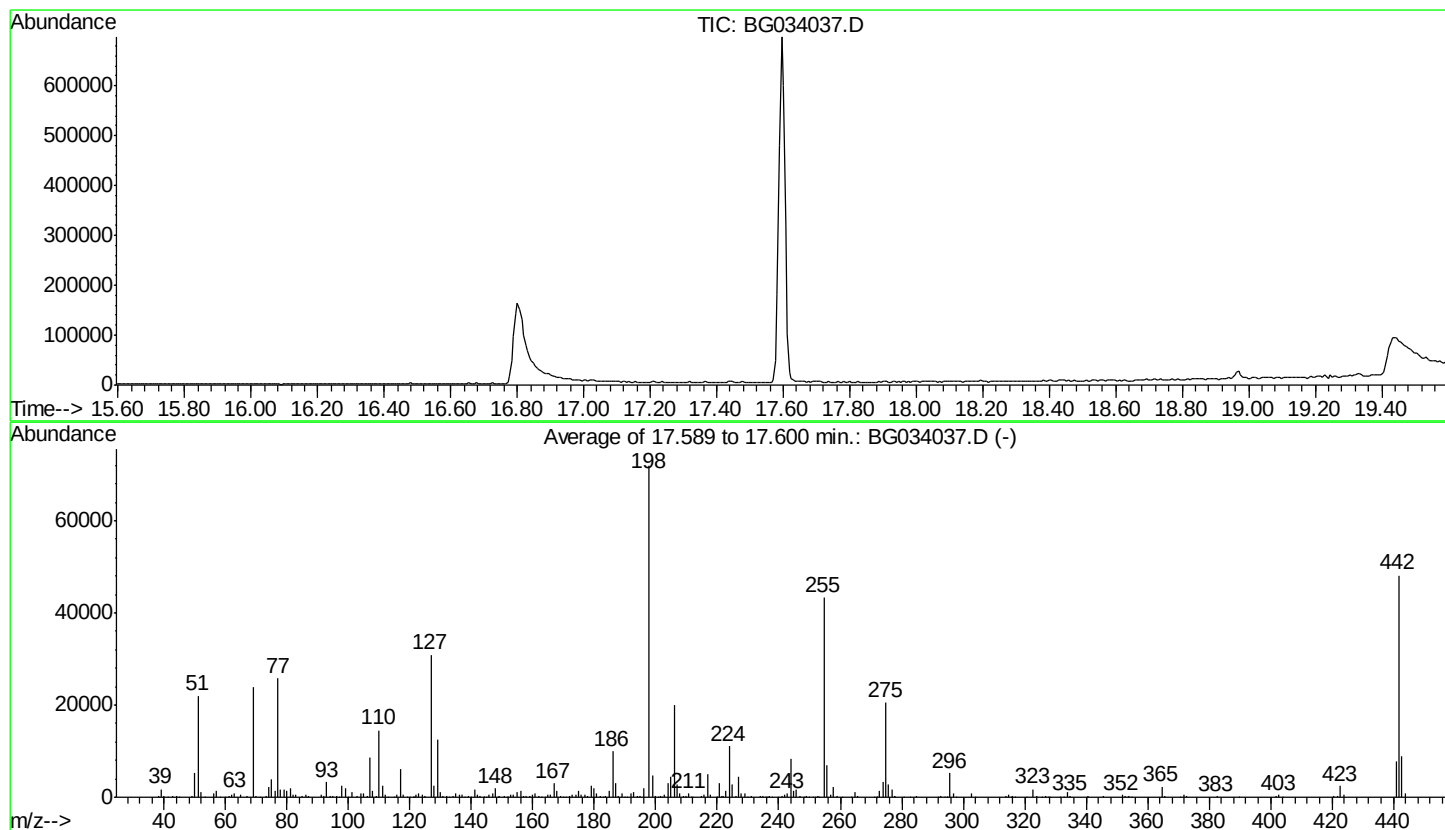

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	22000	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.1	23848	PASS
70	69	0.00	2	0.7	167	PASS
127	198	10	80	43.0	30933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71944	PASS
199	198	5	9	6.7	4842	PASS
275	198	10	60	28.4	20458	PASS
365	198	1	100	3.1	2230	PASS
441	443	0.01	100	88.2	7841	PASS
442	198	50	100	66.8	48058	PASS
443	442	15	24	18.5	8890	PASS