


Data Path : Z:\HPCHEM1\BNA G\Data\BG042718\
 Data File : BG034056.D
 Acq On : 28 Apr 2018 3:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

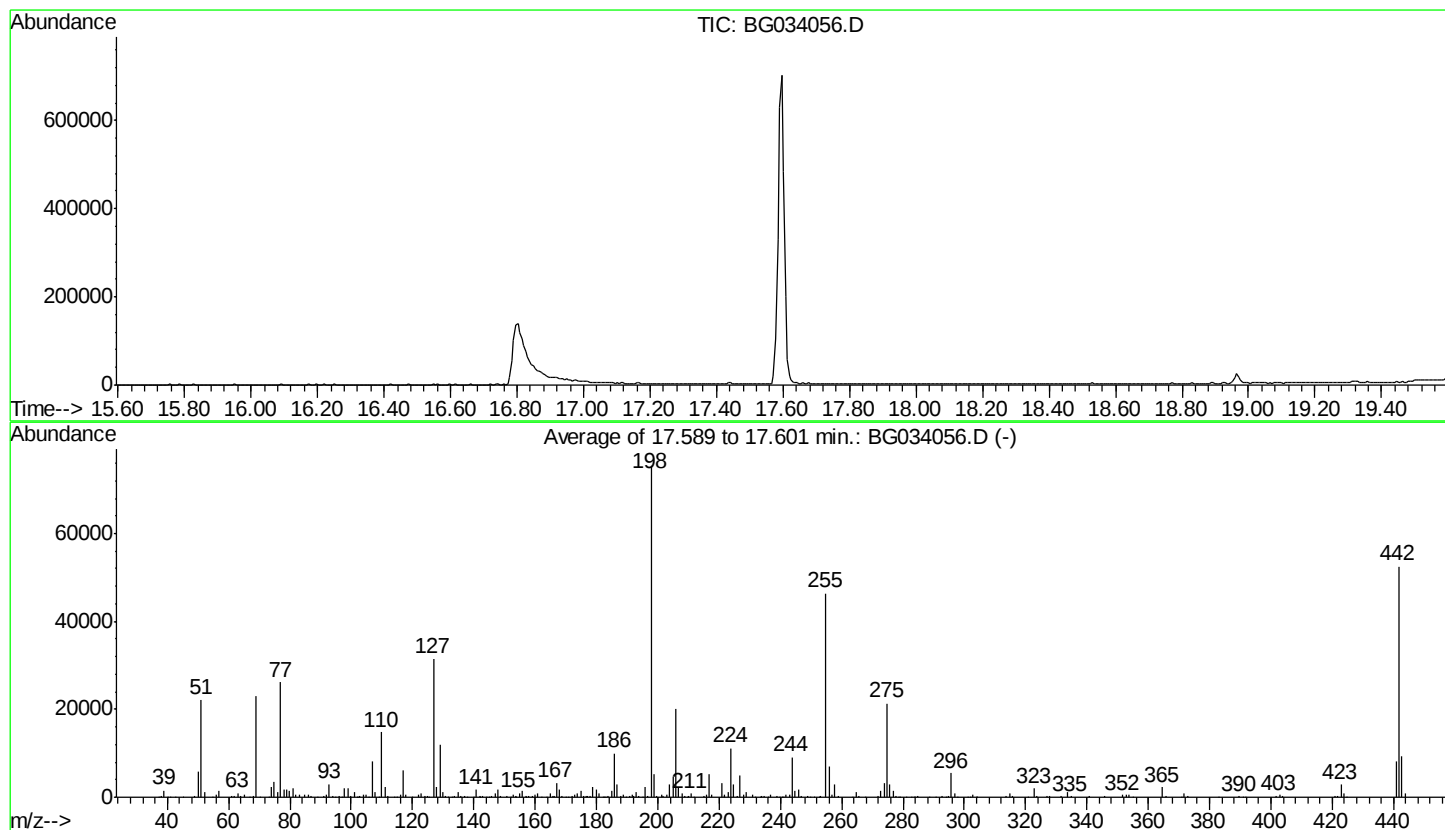

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	22287	PASS
68	69	0.00	2	0.8	183	PASS
69	198	0.00	100	30.5	23031	PASS
70	69	0.00	2	0.4	81	PASS
127	198	10	80	41.7	31469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75442	PASS
199	198	5	9	6.8	5154	PASS
275	198	10	60	28.3	21317	PASS
365	198	1	100	3.0	2296	PASS
441	443	0.01	100	88.2	8252	PASS
442	198	50	100	69.6	52530	PASS
443	442	15	24	17.8	9355	PASS