
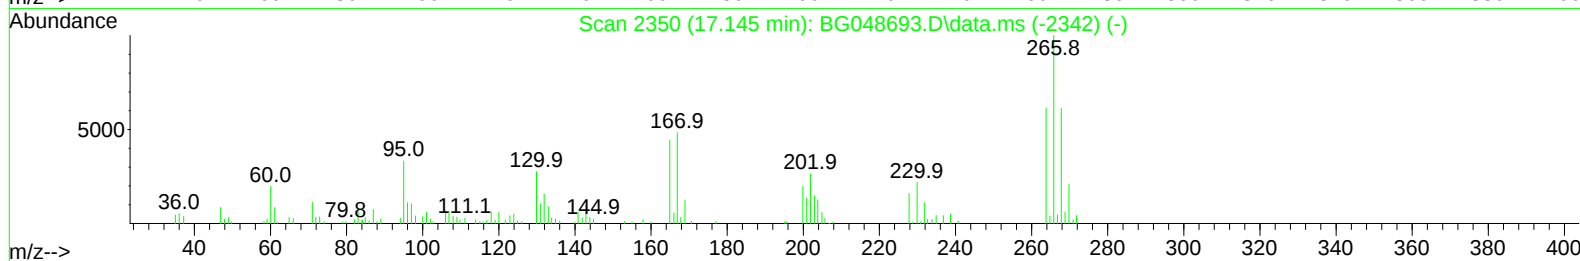
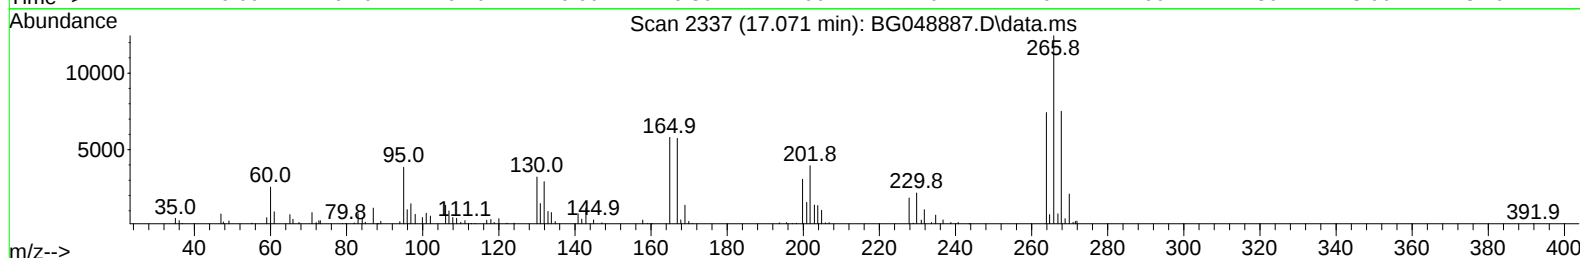


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042721\
Data File : BG048887.D
Acq On : 27 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 15:57:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 11:14:54 2021
Response via : Initial Calibration

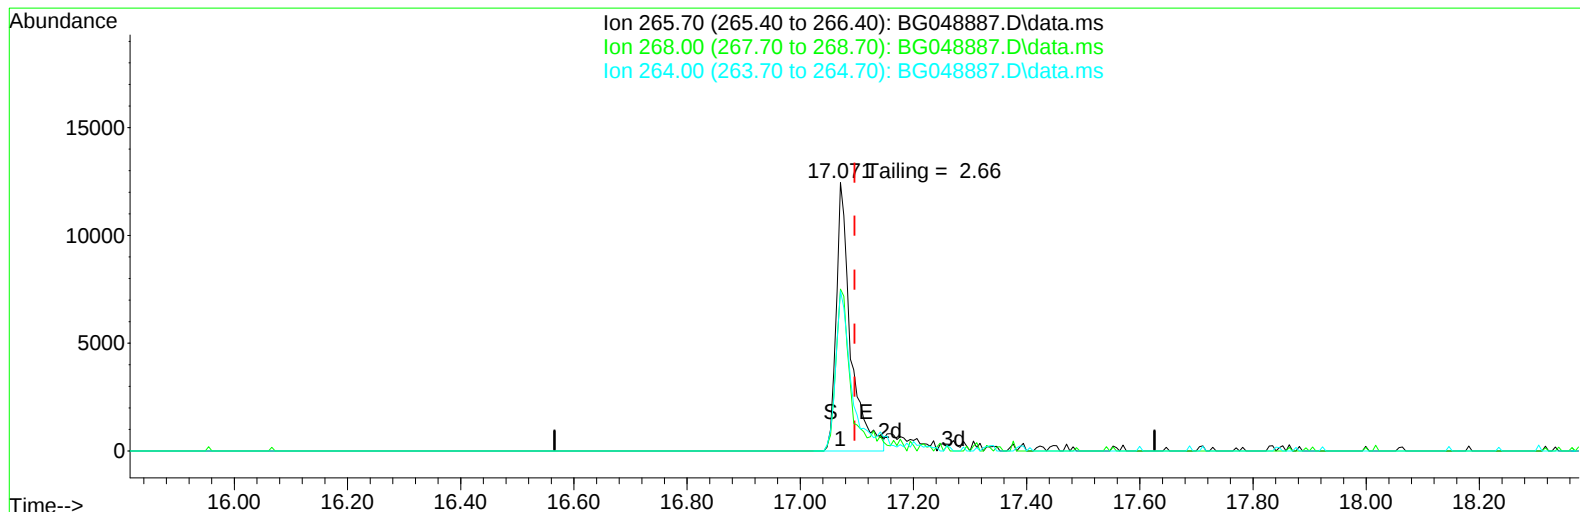

TIC: BG048887.D\data.ms

(70) Pentachlorophenol (C)




17.071min (-0.025) 50182.56 ng

response 22134

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.35
264.00	61.30	65.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042721\
Data File : BG048887.D
Acq On : 27 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 15:57:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 11:14:54 2021
Response via : Initial Calibration

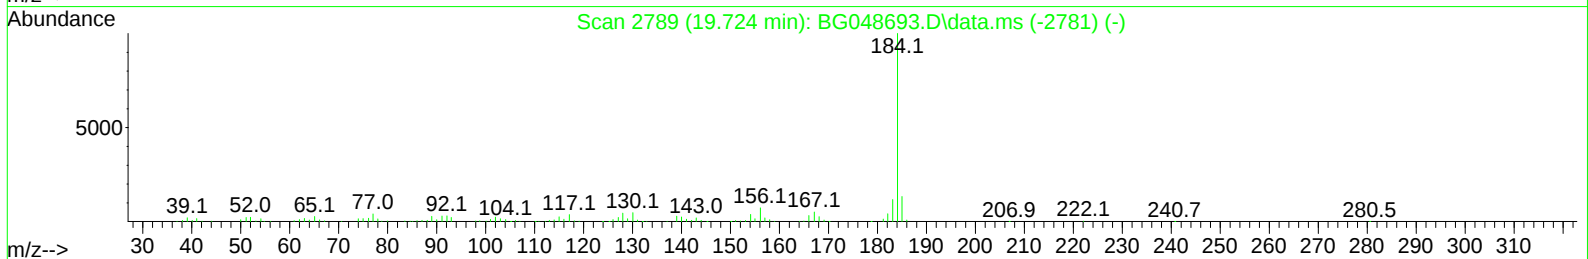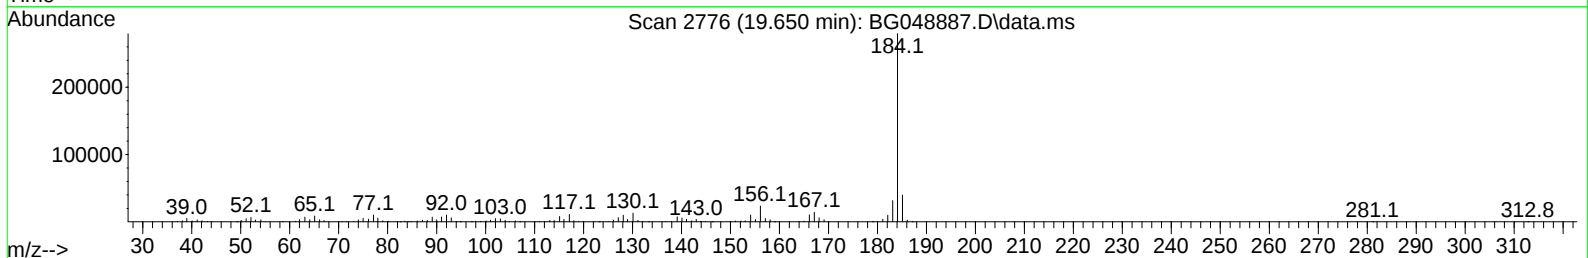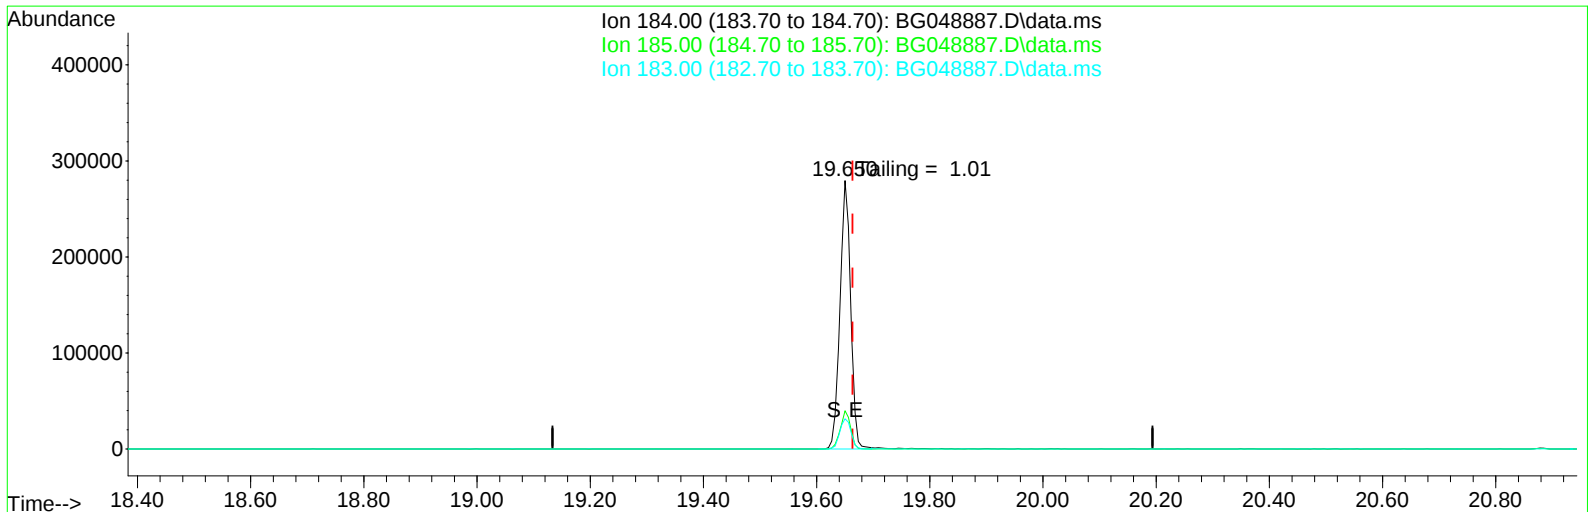

TIC: BG048887.D\data.ms

(77) Benzidine**19.650min (-0.013) 185383.48 ng****response 367506**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.24
183.00	11.70	11.27
0.00	0.00	0.00