


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042721\
 Data File : BG048887.D
 Acq On : 27 Apr 2021 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 16:50:19 2021

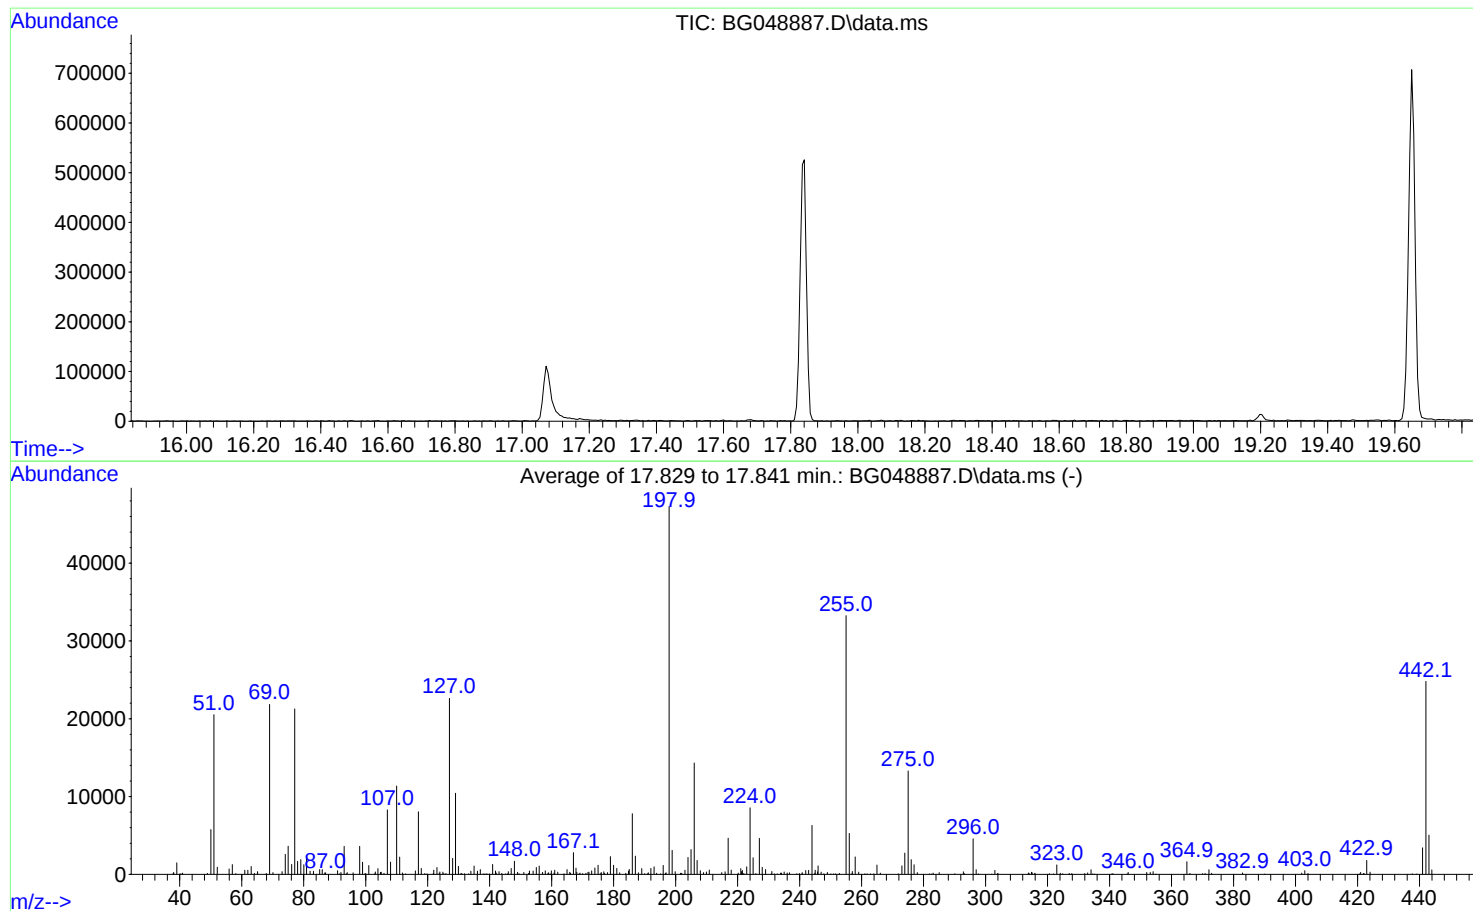




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	20524	PASS
68	69	0.00	2	0.6	128	PASS
69	198	0.00	100	46.2	21848	PASS
70	69	0.00	2	1.0	228	PASS
127	198	10	80	47.9	22632	PASS
197	198	0.00	2	0.4	204	PASS
198	198	100	100	100.0	47283	PASS
199	198	5	9	6.5	3082	PASS
275	198	10	60	28.1	13295	PASS
365	198	1	100	3.5	1635	PASS
441	198	0.01	100	7.2	3421	PASS
442	198	50	100	52.4	24799	PASS
443	442	15	24	20.3	5031	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042721\
Data File : BG048887.D
Acq On : 27 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 15:57:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 11:14:54 2021
Response via : Initial Calibration

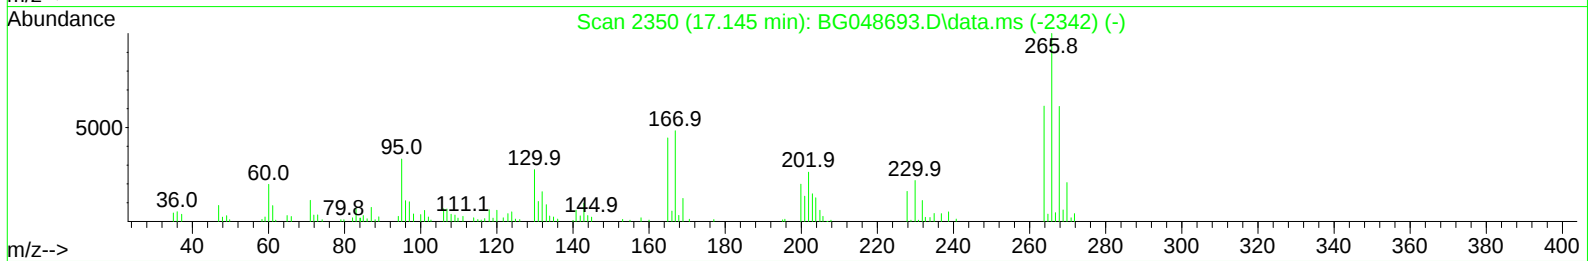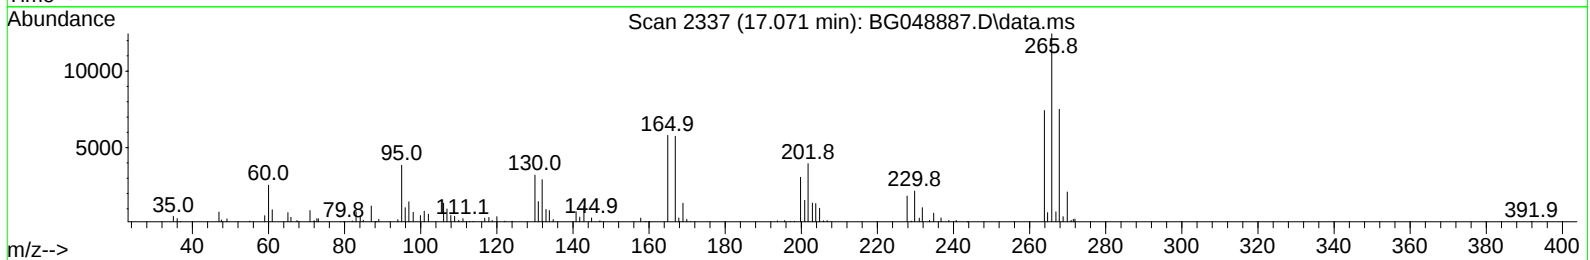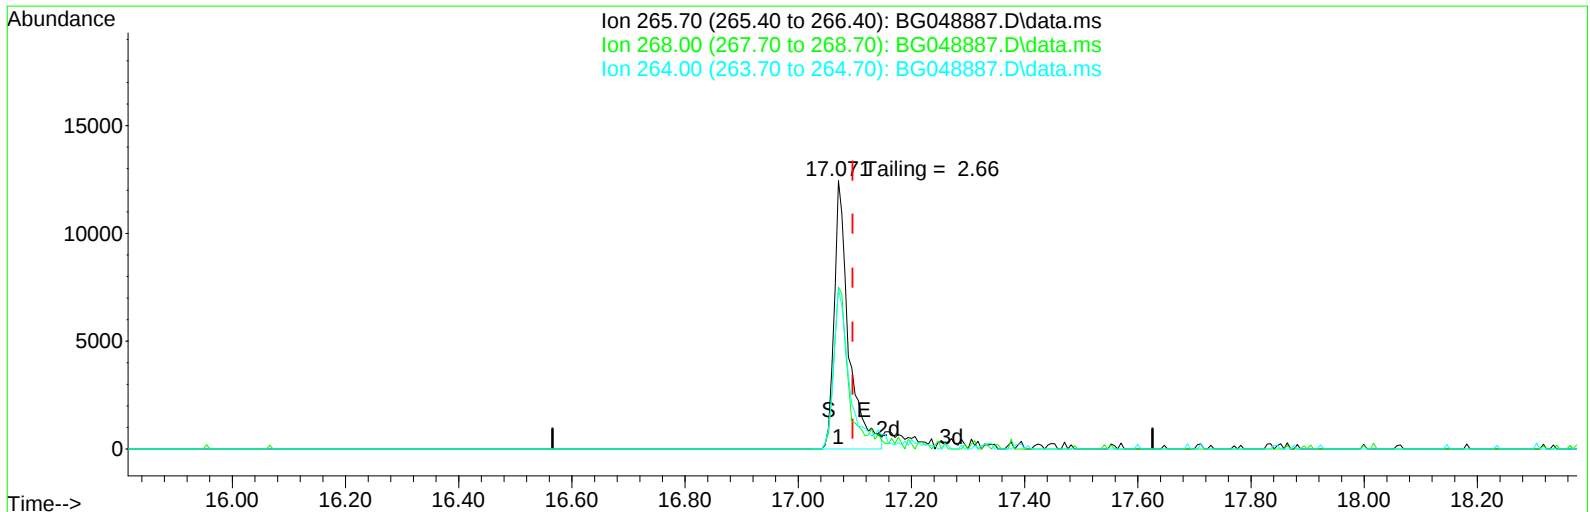

TIC: BG048887.D\data.ms

(70) Pentachlorophenol (C)

17.071min (-0.025) 50182.56 ng




response 22134

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.35
264.00	61.30	65.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042721\
Data File : BG048887.D
Acq On : 27 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 15:57:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 11:14:54 2021
Response via : Initial Calibration

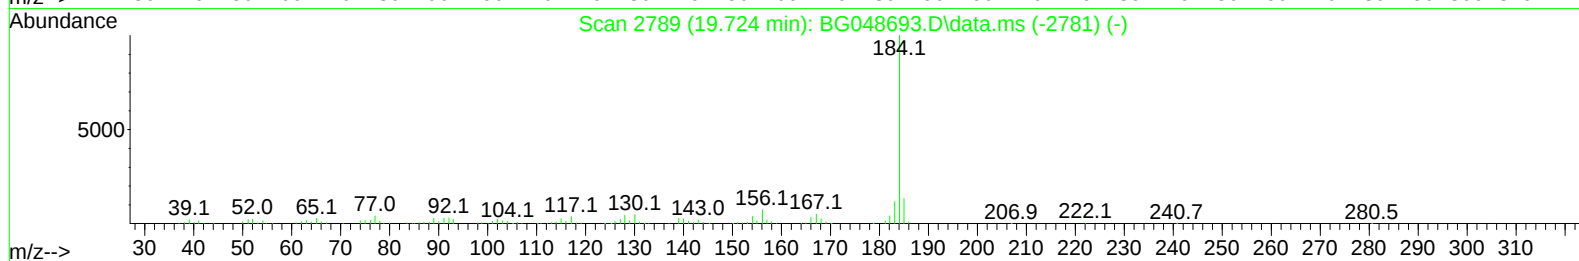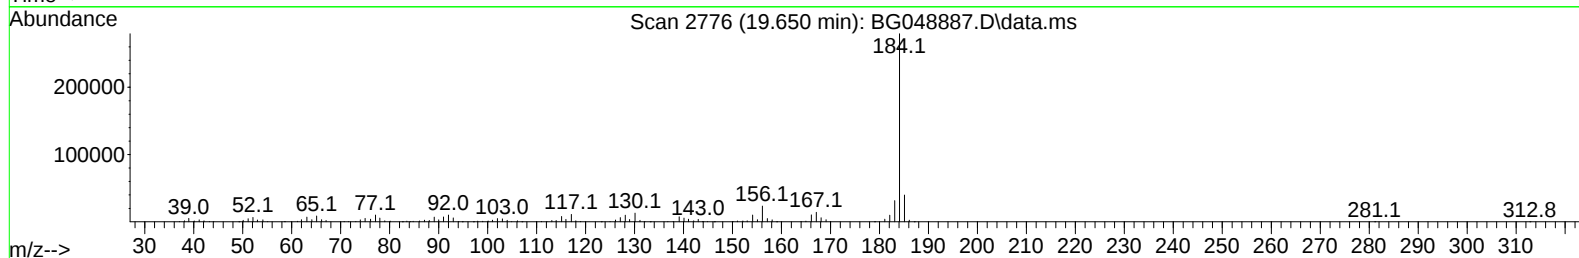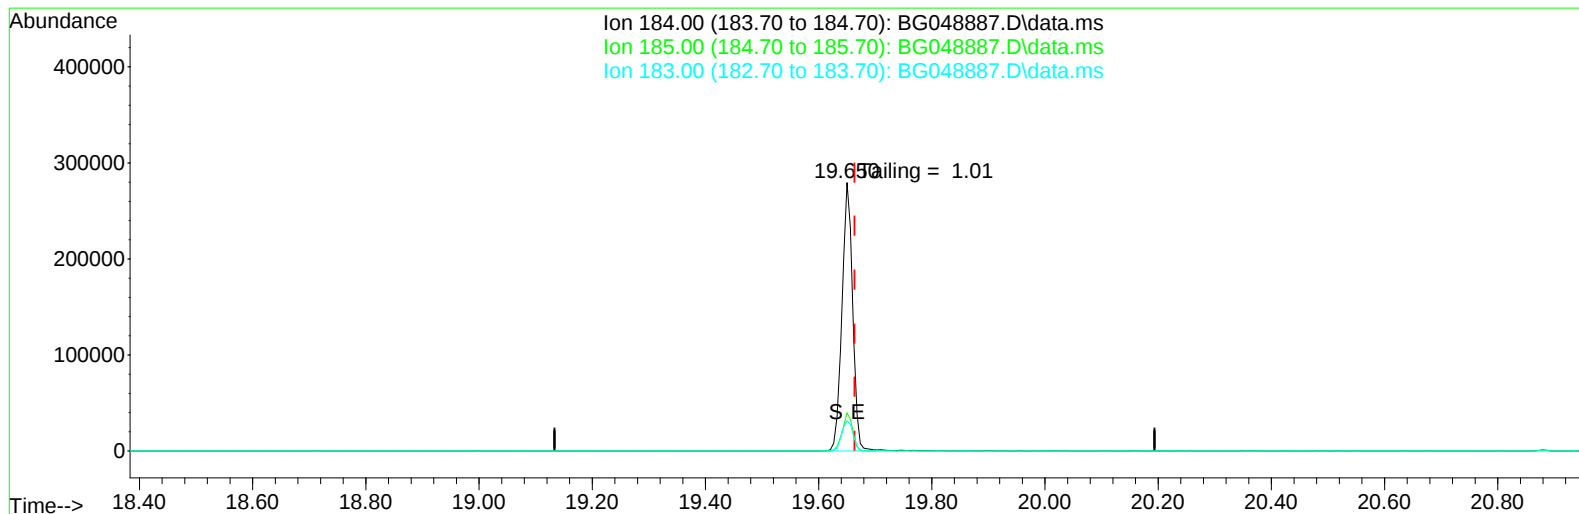

TIC: BG048887.D\data.ms

(77) Benzidine

19.650min (-0.013) 185383.48 ng

response 367506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.24
183.00	11.70	11.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2021	BNA_G	BG048887.D
Compound Name	Response	Retention Time
DDT	182051	20.87
DDD	216	20.45
DDE	338	19.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
554	182605	0.30

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP