
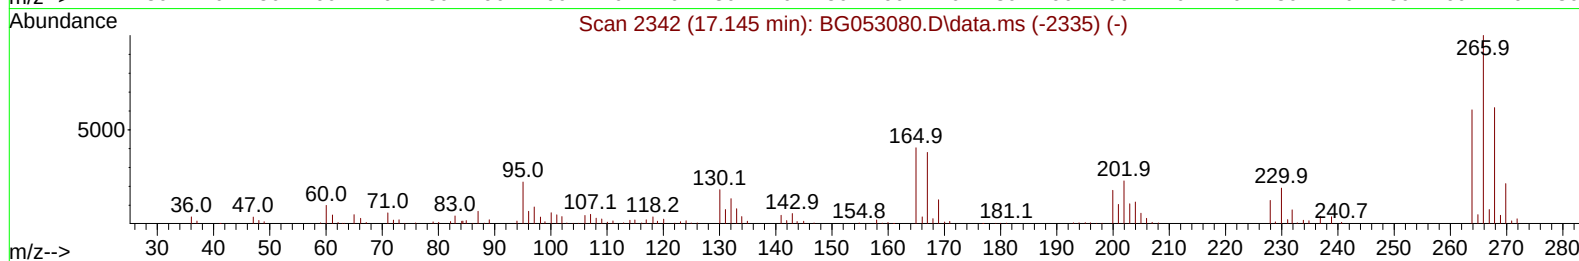
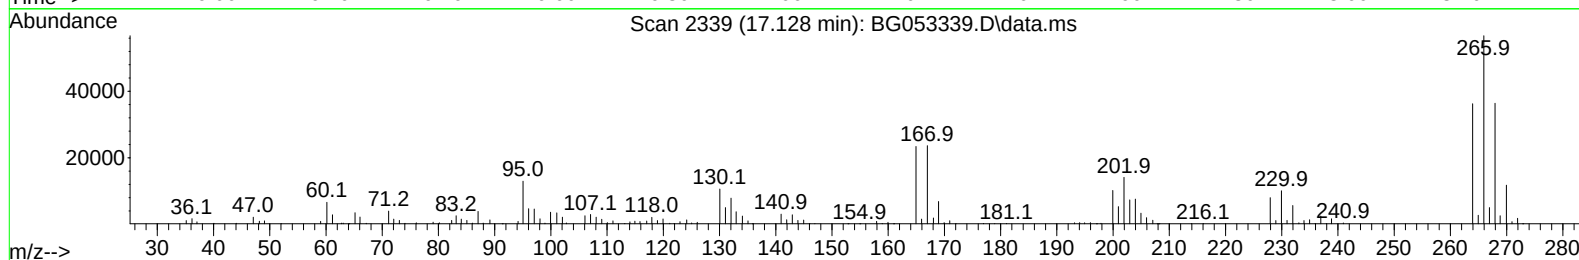


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053339.D
Acq On : 27 Apr 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 13:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

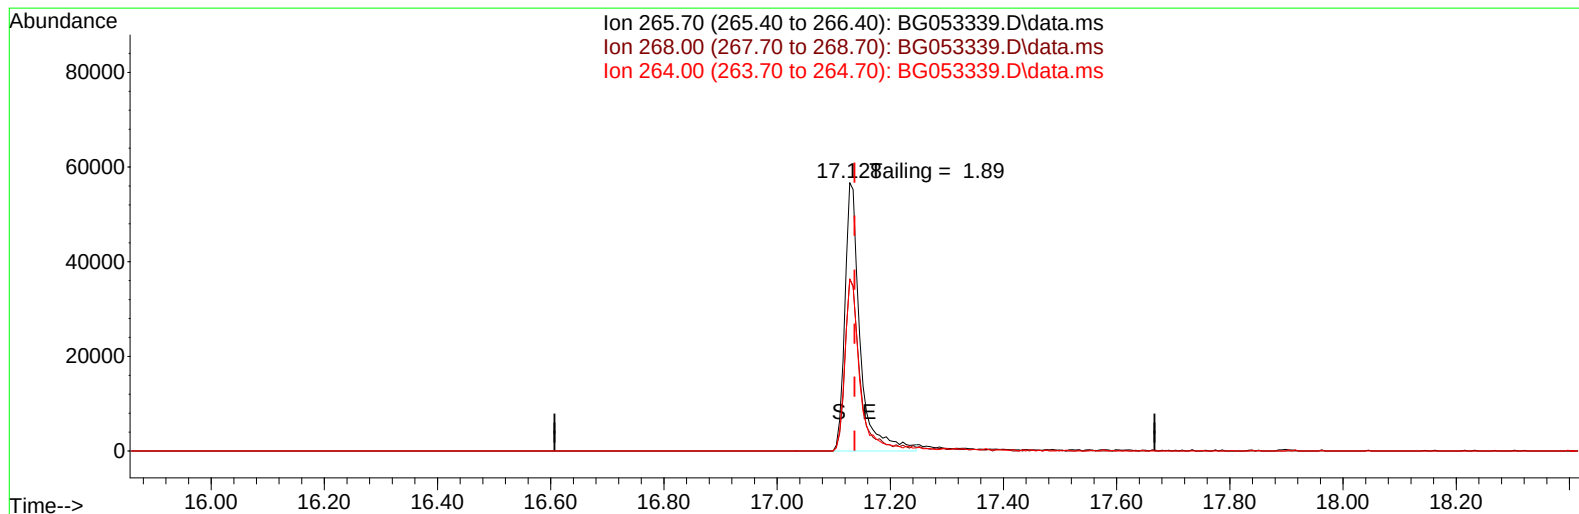

TIC: BG053339.D\data.ms

(70) Pentachlorophenol (C)




17.128min (-0.008) 25104.35 ng

response 105284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.16
264.00	56.60	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053339.D
Acq On : 27 Apr 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 13:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

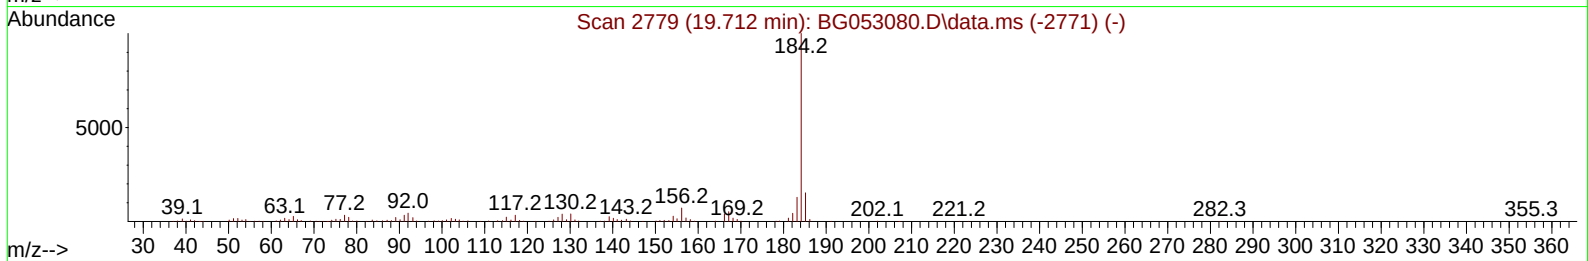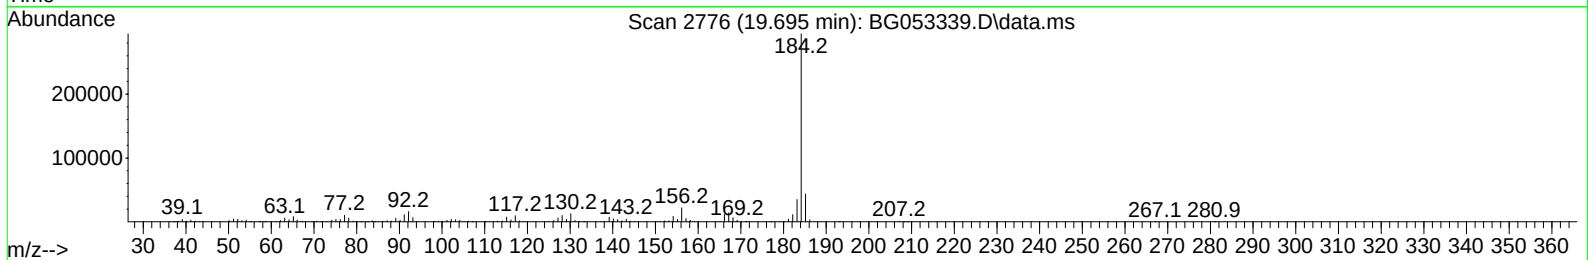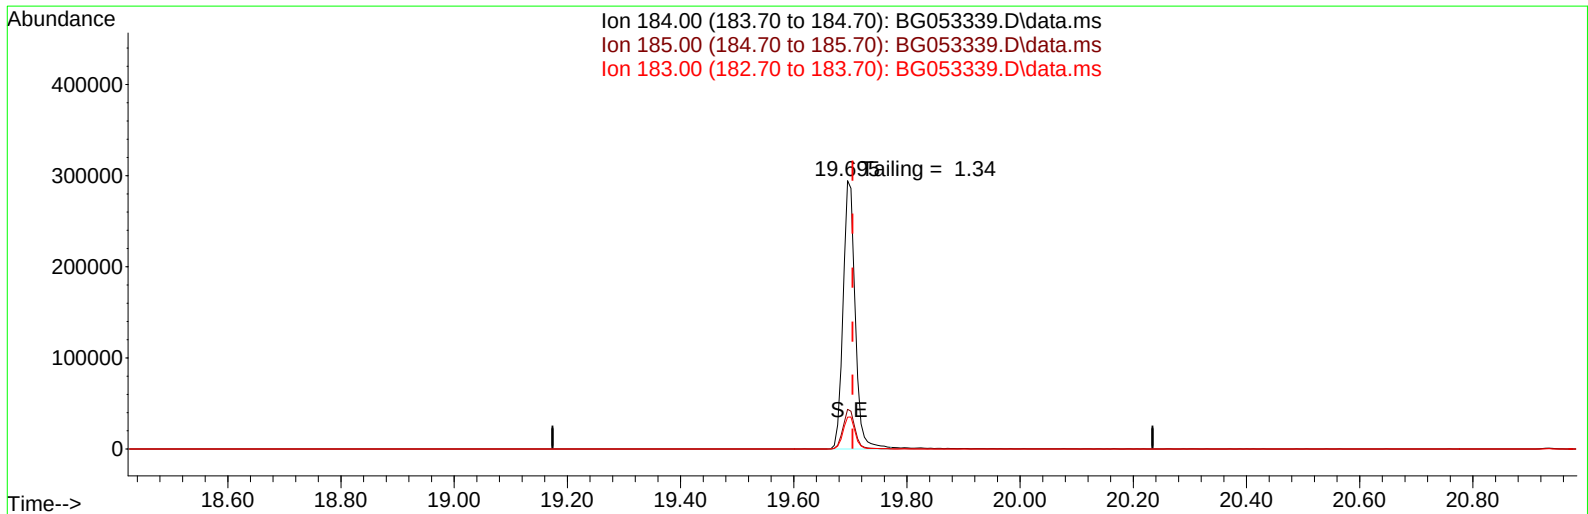

TIC: BG053339.D\data.ms

(77) Benzidine**19.695min (-0.008) 135039.88 ng****response 439231**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.77
183.00	11.80	11.88
0.00	0.00	0.00