

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
 Data File : BG053341.D
 Acq On : 27 Apr 2022 10:56
 Operator : CG/JU
 Sample : PB144386BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB144386BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.669	381	388	400	rBV	538073	886348	30.31%	8.439%
2	7.267	652	660	675	rBV	550410	983011	33.61%	9.359%
3	8.101	794	802	810	rVB	95060	166416	5.69%	1.584%
4	9.264	993	1000	1009	rBV	333326	627517	21.46%	5.974%
5	10.915	1274	1281	1292	rBV	125058	231609	7.92%	2.205%
6	13.353	1689	1696	1707	rBV	948575	1448764	49.54%	13.793%
7	14.727	1922	1930	1939	rBV	224047	350353	11.98%	3.336%
8	16.214	2176	2183	2198	rBV	728237	1203224	41.14%	11.455%
9	17.471	2391	2397	2406	rVB	315102	481827	16.47%	4.587%
10	20.079	2833	2841	2849	rBV	2204675	2924702	100.00%	27.845%
11	21.753	3120	3126	3134	rBV2	354662	606150	20.73%	5.771%
12	25.054	3677	3688	3700	rBV2	201253	593662	20.30%	5.652%




Sum of corrected areas: 10503583

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053341.D
Acq On : 27 Apr 2022 10:56
Operator : CG/JU
Sample : PB144386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144386BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

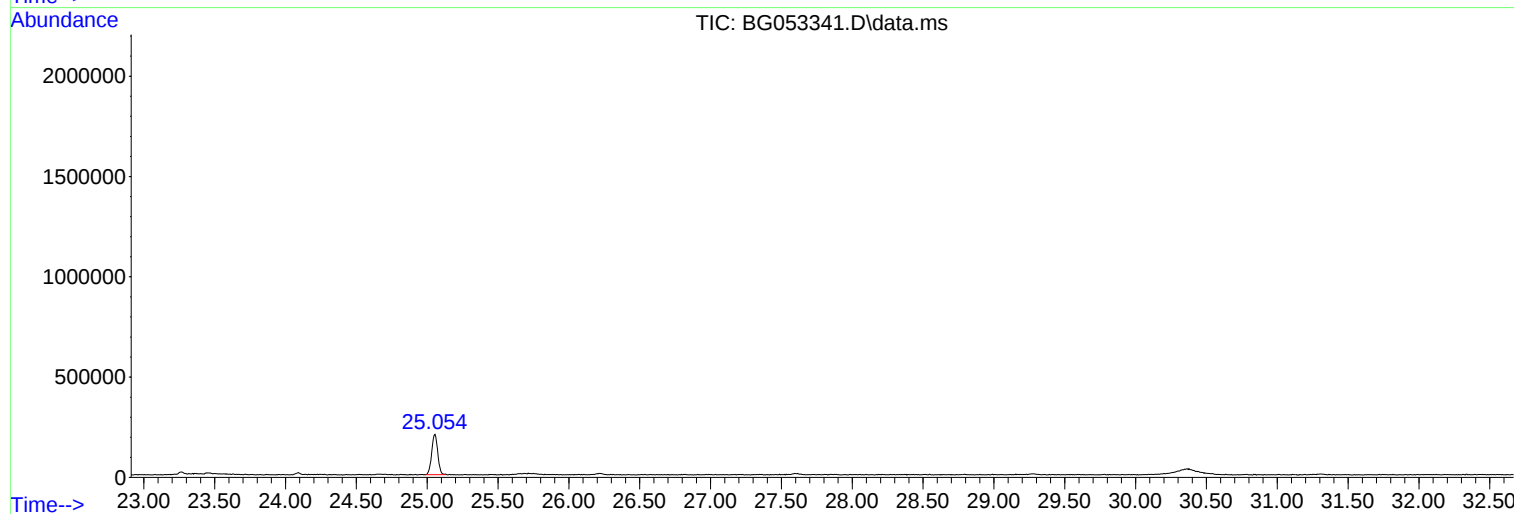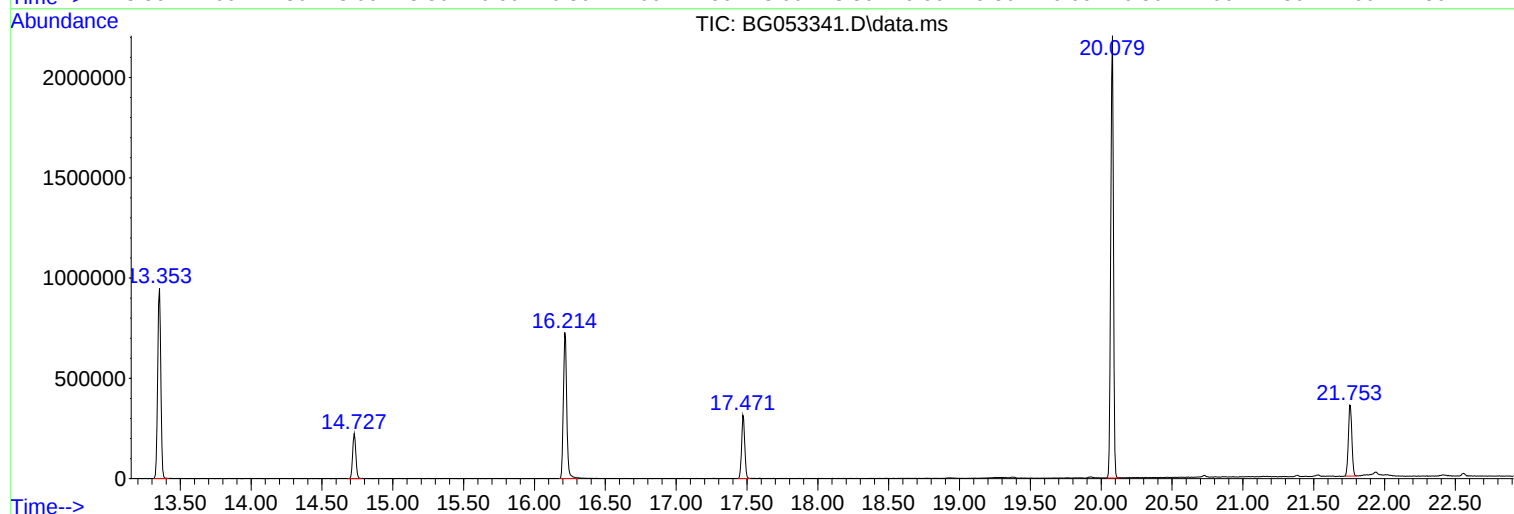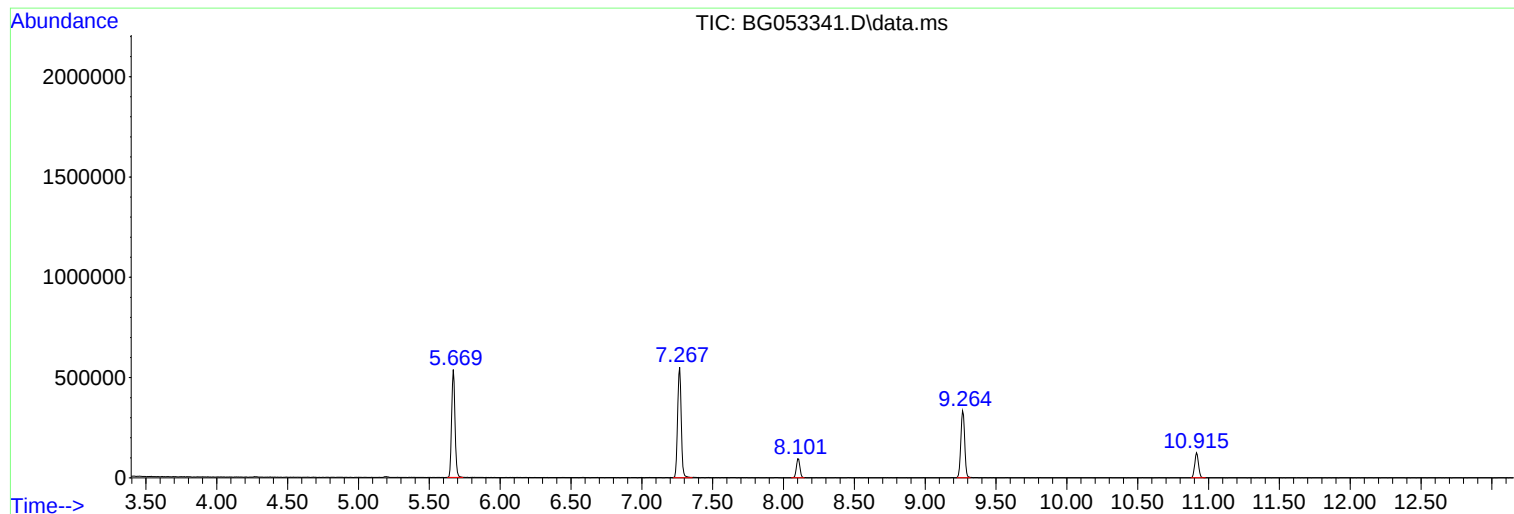

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053341.D
Acq On : 27 Apr 2022 10:56
Operator : CG/JU
Sample : PB144386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144386BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053341.D
Acq On : 27 Apr 2022 10:56
Operator : CG/JU
Sample : PB144386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144386BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------