

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
 Data File : BG053347.D
 Acq On : 27 Apr 2022 14:53
 Operator : CG/JU
 Sample : N2521-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-FB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.189	301	306	315	rBV	25380	40903	1.59%	0.474%
2	5.670	378	388	397	rBV	184005	310675	12.04%	3.600%
3	7.262	653	659	669	rBV	108338	198510	7.70%	2.300%
4	8.102	792	802	809	rBV	98507	165771	6.43%	1.921%
5	9.266	992	1000	1010	rBV	318668	587893	22.79%	6.812%
6	10.916	1271	1281	1291	rVB	119873	226097	8.77%	2.620%
7	13.348	1688	1695	1704	rBV	853470	1367922	53.03%	15.850%
8	14.729	1922	1930	1936	rBV	217341	344403	13.35%	3.991%
9	16.215	2176	2183	2198	rBV	763060	1233783	47.83%	14.296%
10	17.472	2391	2397	2404	rBV	321316	489371	18.97%	5.670%
11	20.074	2834	2840	2846	rBV	2046283	2579394	100.00%	29.888%
12	21.755	3119	3126	3133	rBV2	316233	530242	20.56%	6.144%
13	25.050	3677	3687	3700	rVB2	184018	555265	21.53%	6.434%




Sum of corrected areas: 8630229

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053347.D
Acq On : 27 Apr 2022 14:53
Operator : CG/JU
Sample : N2521-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

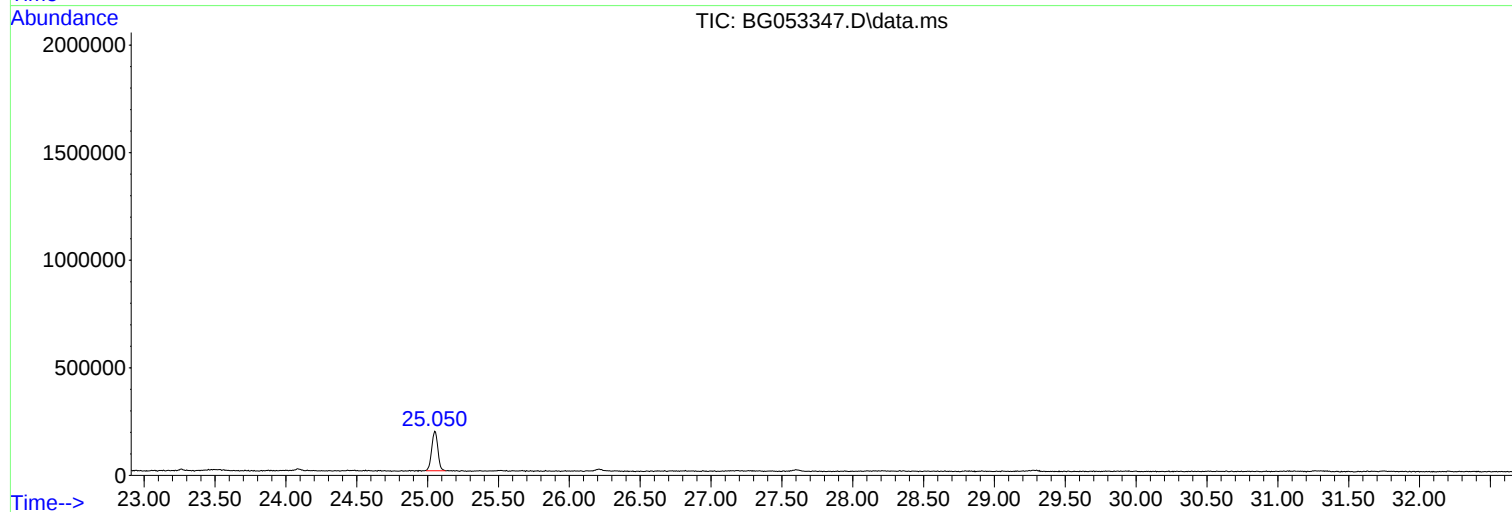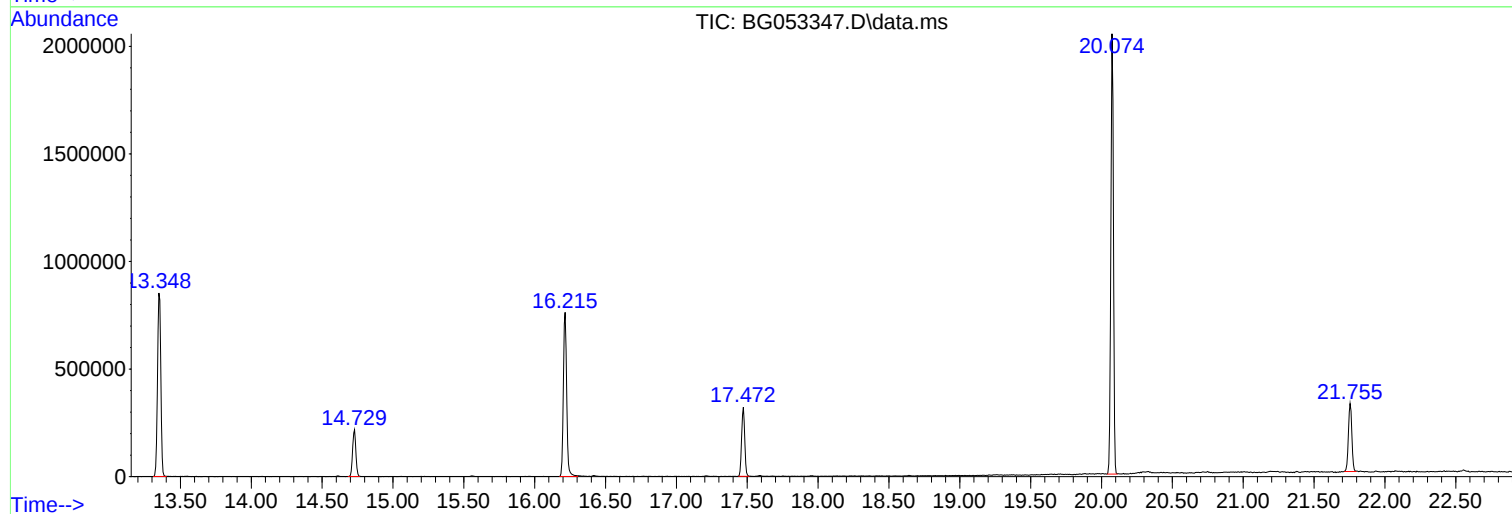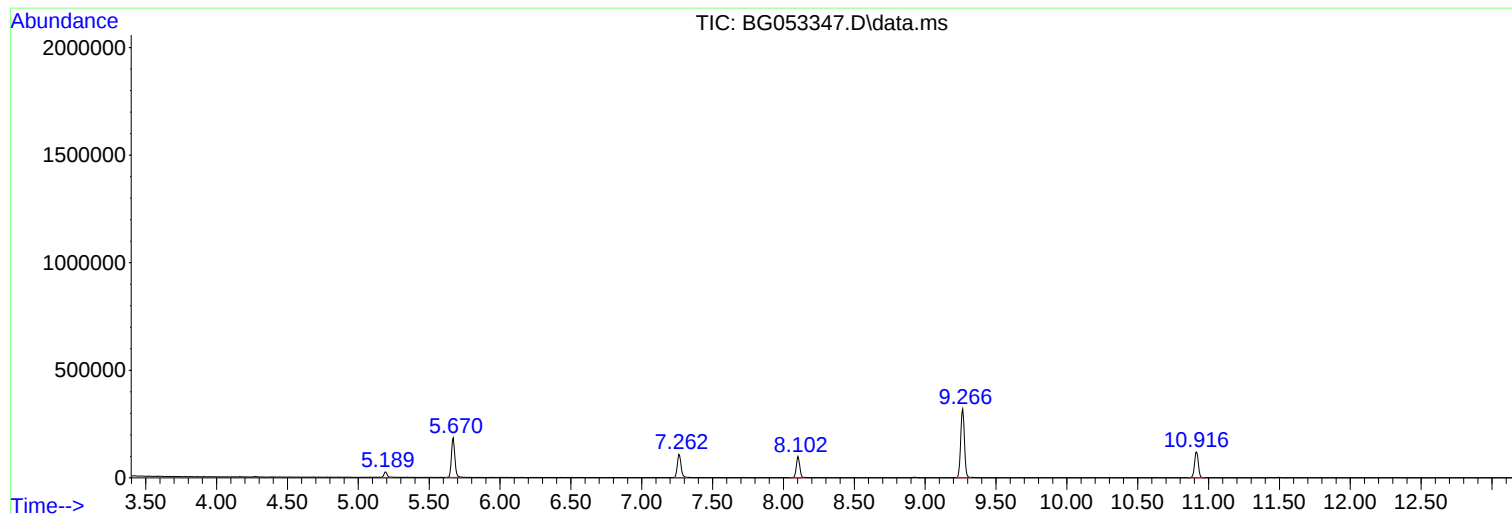

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053347.D
Acq On : 27 Apr 2022 14:53
Operator : CG/JU
Sample : N2521-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.189	4.93 ng	40903	1,4-Dichlorobenzene-d4	8.102

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9		
4	Carbonic acid, hexyl prop-1-en-2...	186	C10H18O3	1000382-54-2	9		
5	1,3-Dioxolane-2-methanol, 2,4-di...	132	C6H12O3	053951-43-2	9		

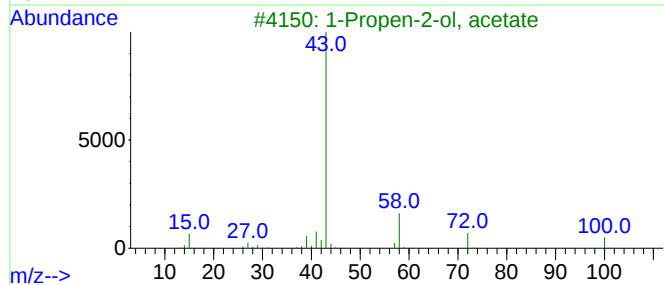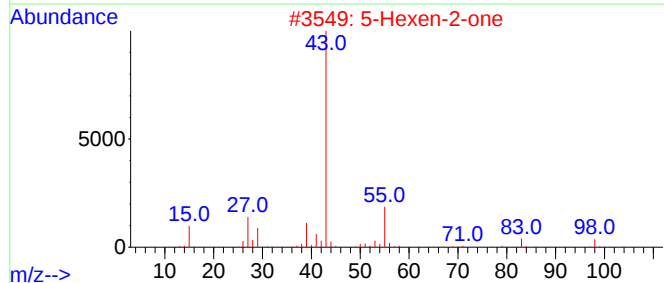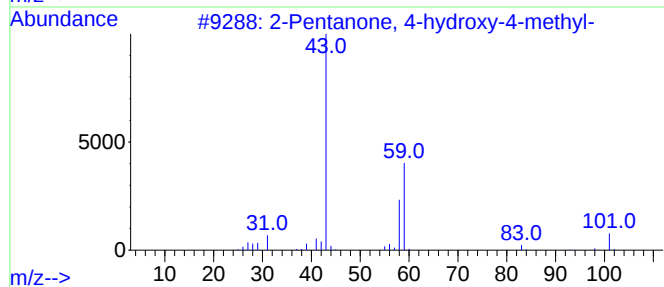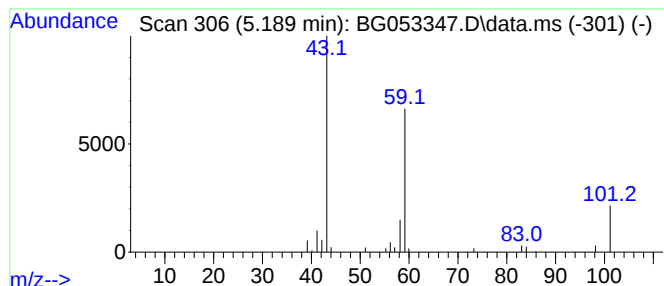

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053347.D
Acq On : 27 Apr 2022 14:53
Operator : CG/JU
Sample : N2521-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.189	4.9	ng	40903	1	8.102	165771	20.0