
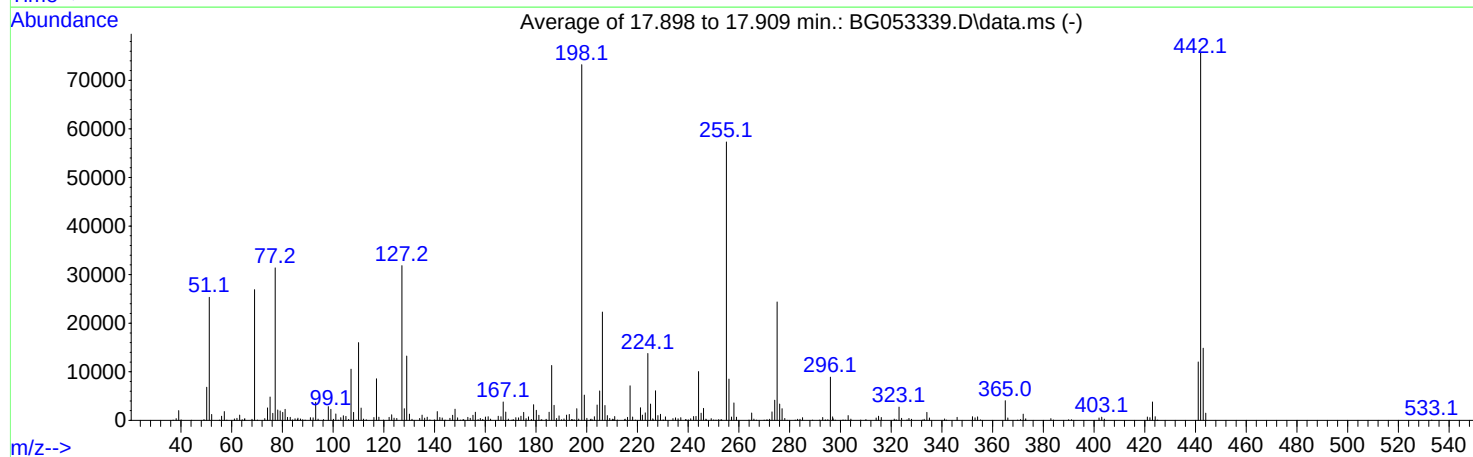


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053339.D
Acq On : 27 Apr 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Apr 24 01:13:30 2022

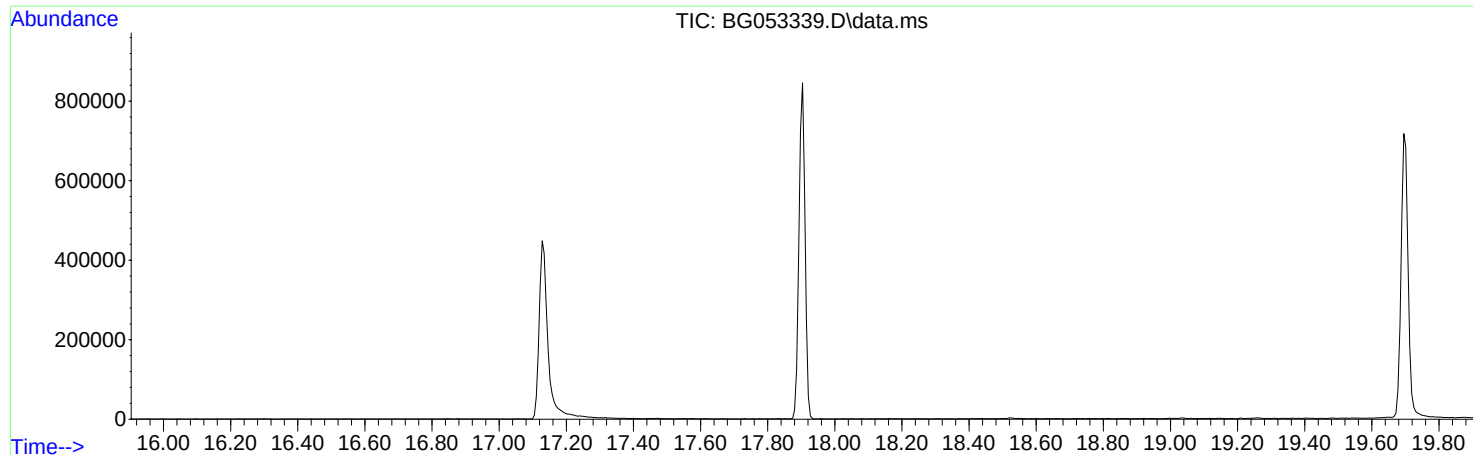




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	25339	PASS
68	69	0.00	2	0.9	229	PASS
69	198	0.00	100	36.8	26923	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	43.5	31848	PASS
197	198	0.00	2	0.4	273	PASS
198	198	100	100	100.0	73219	PASS
199	198	5	9	7.1	5209	PASS
275	198	10	60	33.3	24360	PASS
365	198	1	100	5.5	4055	PASS
441	198	0.01	100	16.4	12036	PASS
442	442	50	100	100.0	75725	PASS
443	442	15	24	19.6	14854	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053339.D
Acq On : 27 Apr 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 13:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

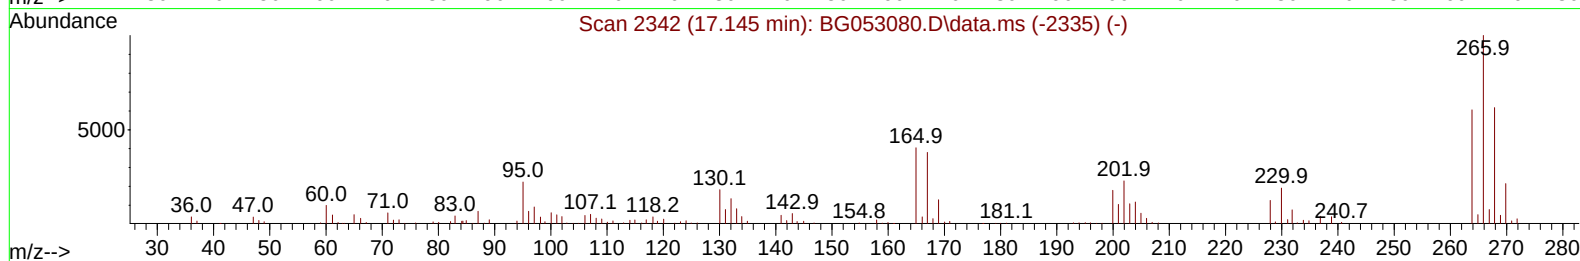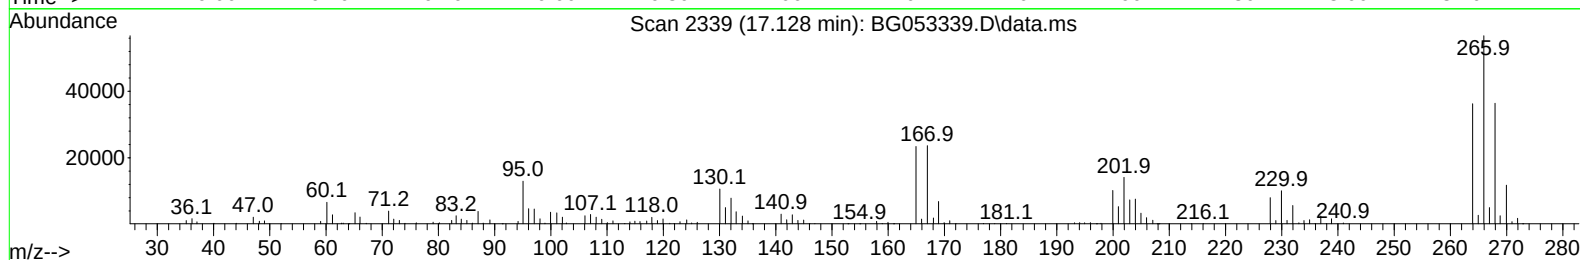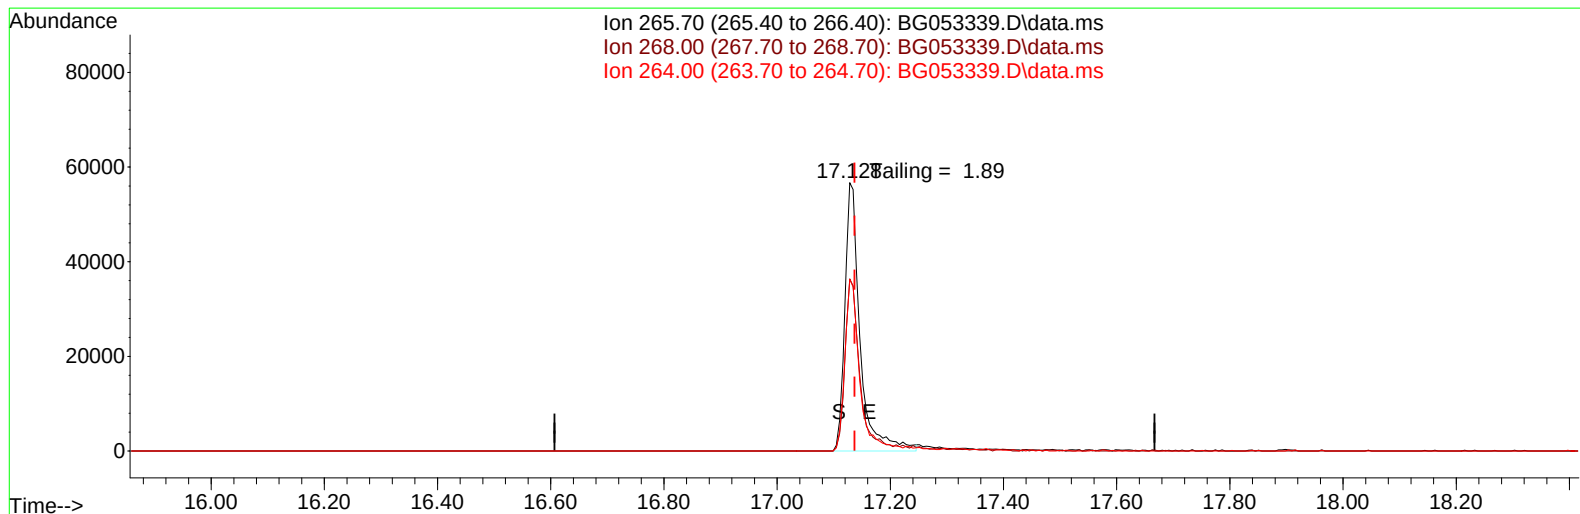

TIC: BG053339.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.008) 25104.35 ng




response 105284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.16
264.00	56.60	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042722\
Data File : BG053339.D
Acq On : 27 Apr 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 13:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

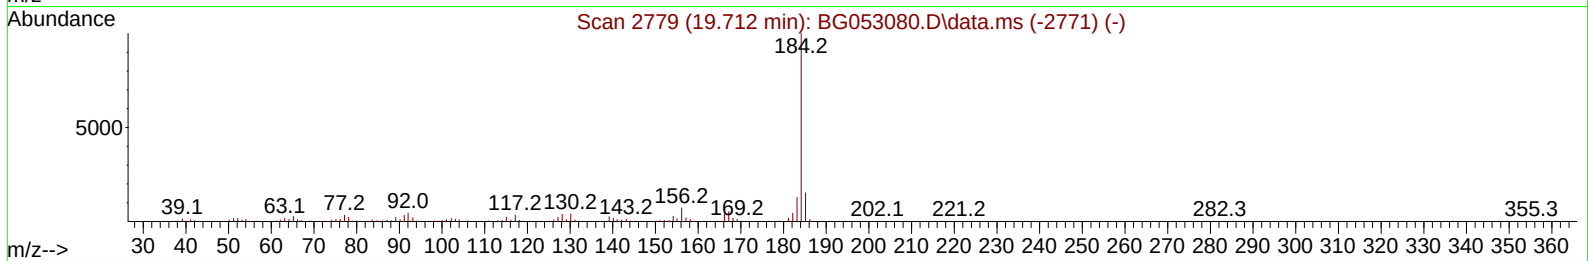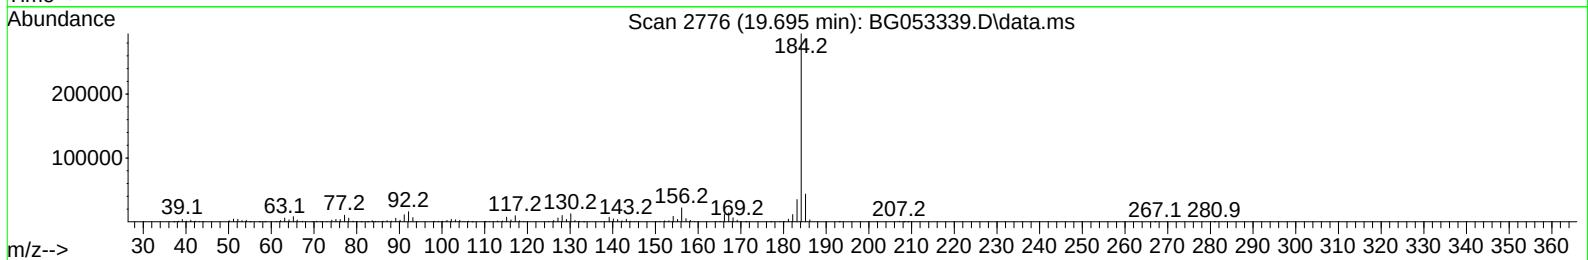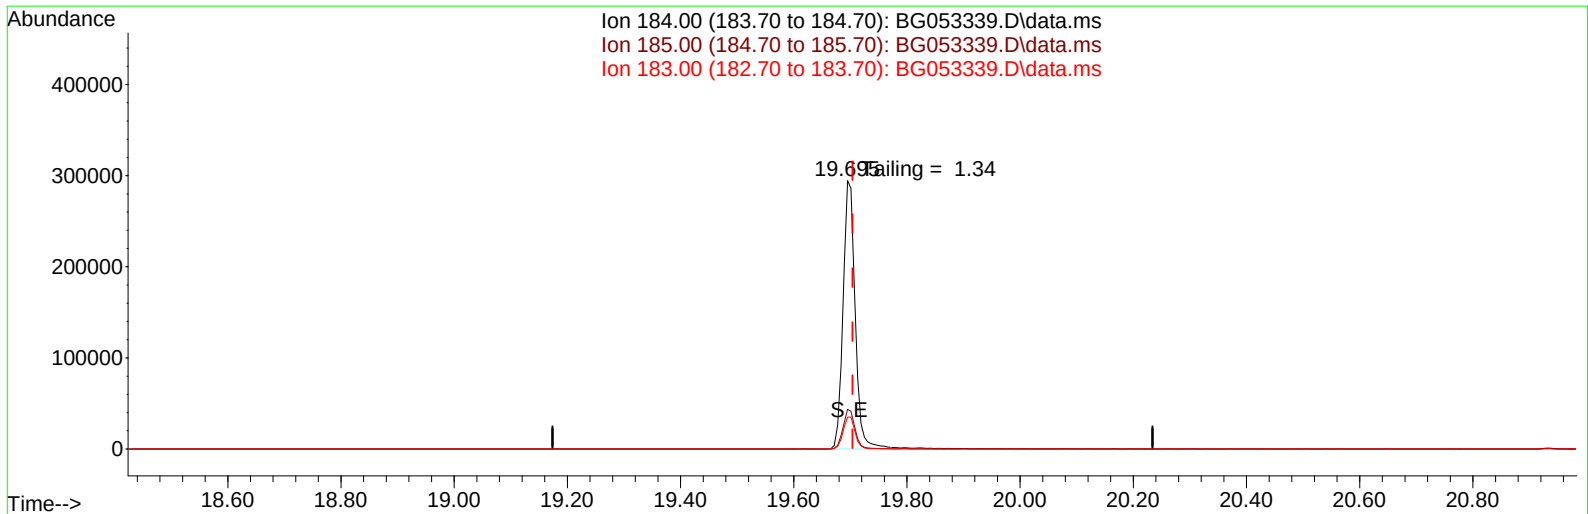

TIC: BG053339.D\data.ms

(77) Benzidine

19.695min (-0.008) 135039.88 ng

response 439231

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.77
183.00	11.80	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2022	BNA_G	<u>BG053339.D</u>
Compound Name	Response	Retention Time
DDT	253070	20.935
DDD	2550	20.541
DDE	172	19.983
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2722	255792	1.06