

Data File : BG026759.D
Acq On : 28 Apr 2017 22:57
Operator : SJ/MA
Sample : I2816-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT41

Quant Time: Apr 29 01:26:58 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 01:26:17 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	179457	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	880701	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	478161	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	886624	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	784116	20.00	ng/ul	0.00
83) Perylene-d12	24.77	264	827519	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	12658	3.18	ng/uL	0.00
5) Phenol-d5	7.19	99	323919	20.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	195588	20.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	260931	19.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	291985	21.97	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	149771	20.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	168293	21.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	260096	20.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	207056	12.16	ng/ul	0.00
43) Dimethylphthalate-d6	14.23	166	1926	0.05	ng/ul	0.21
46) Acenaphthylene-d8	14.31	160	1074741	22.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	123304	17.77	ng/ul	0.00
57) Fluorene-d10	15.60	176	731642	21.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	111801	20.77	ng/ul	0.00
70) Anthracene-d10	17.45	188	1004420	23.34	ng/ul	0.00
76) Pyrene-d10	19.74	212	956920	23.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	887800	22.69	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.07	163	149124	3.96 ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026759.D

Acq On : 28 Apr 2017 22:57

Operator : SJ/MA

Sample : I2816-13

Misc :

ALS Vial : 17 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

JHT41


Quant Time: Apr 29 01:26:58 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Apr 29 01:26:17 2017

Response via : Initial Calibration

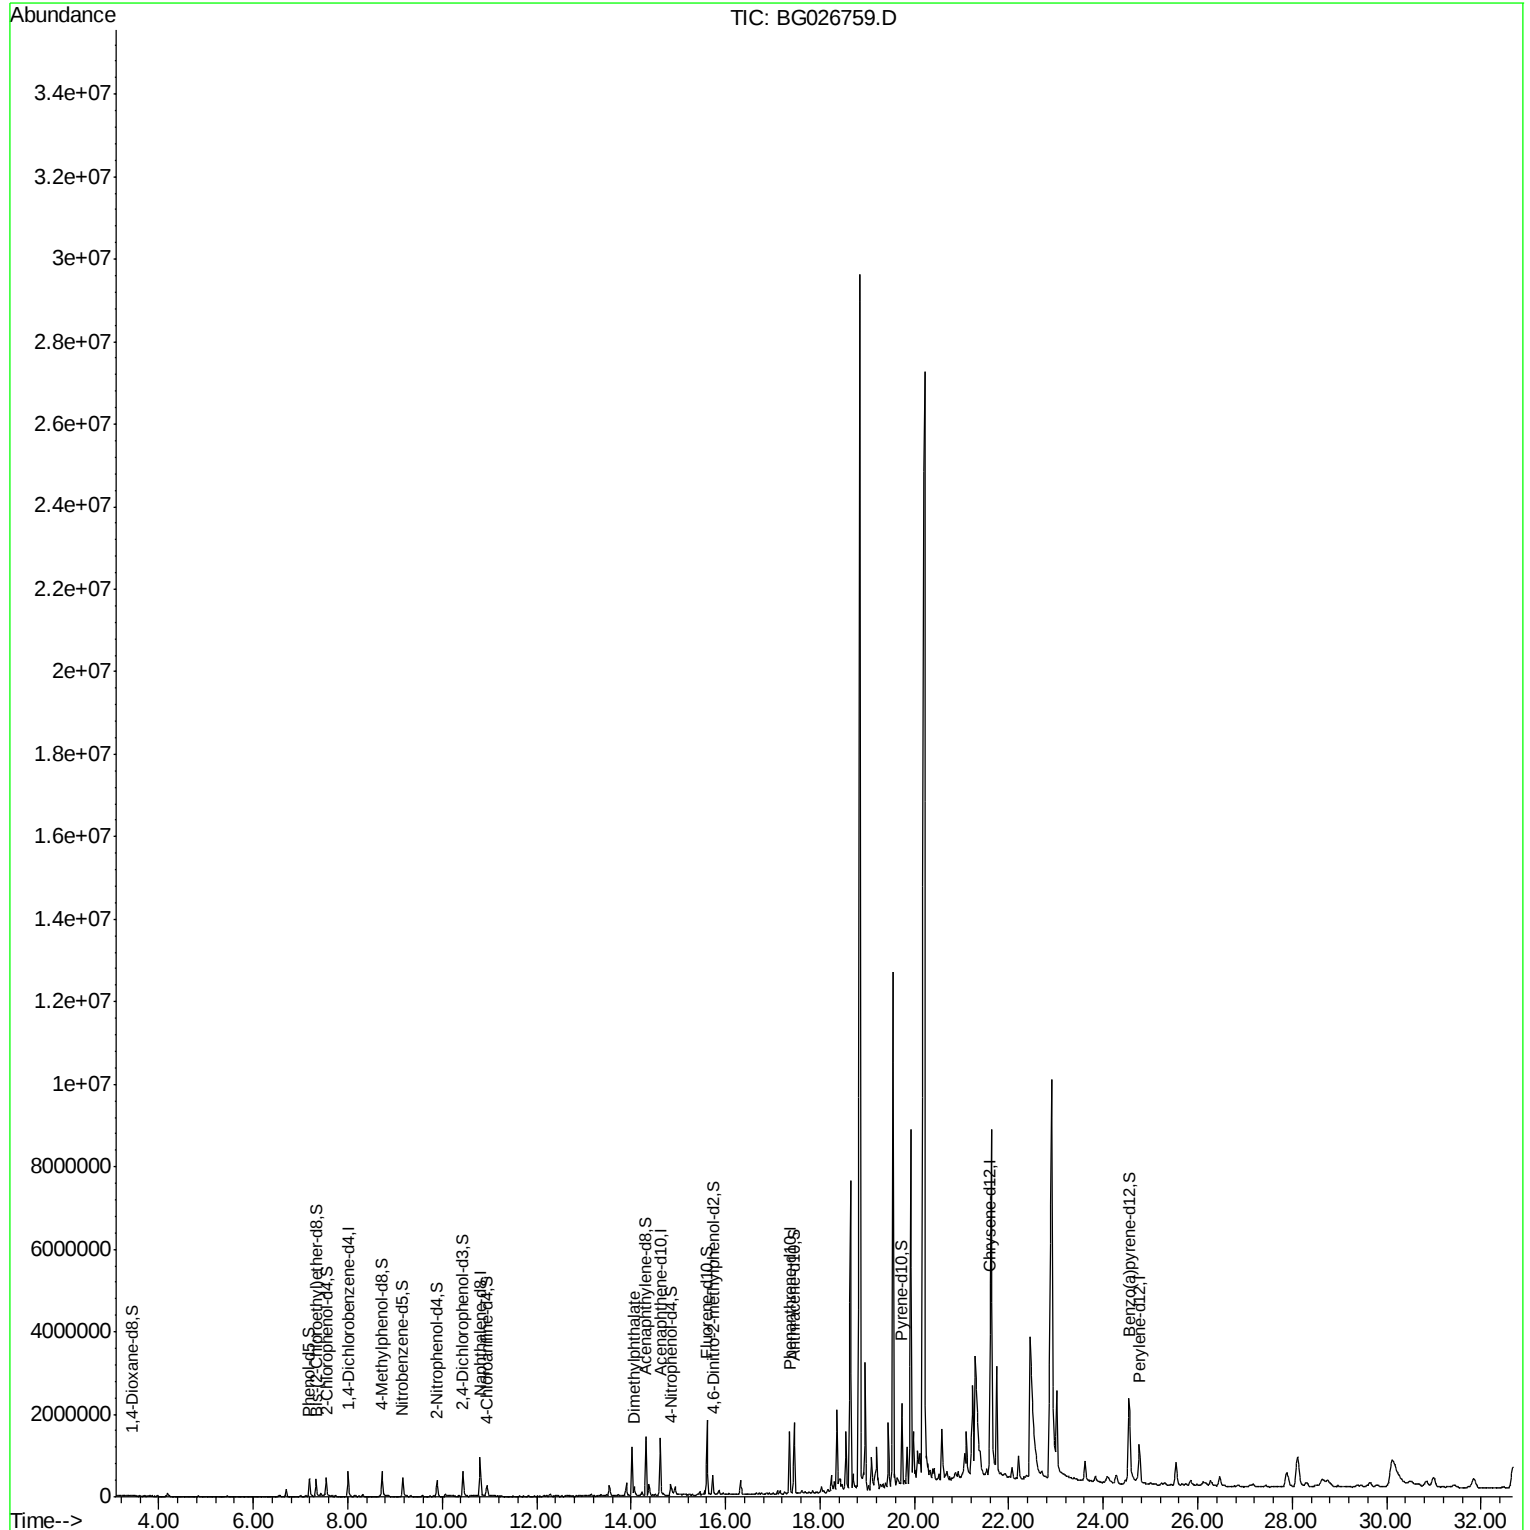

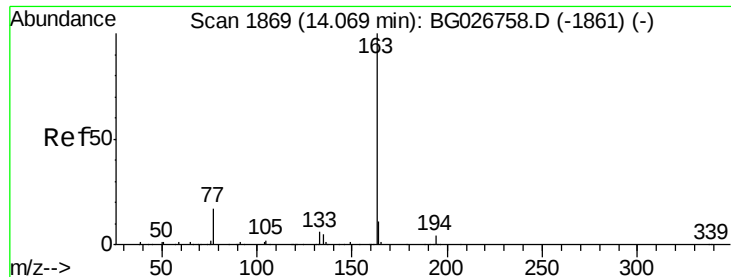

#44

Dimethylphthalate

Concen: 3.96 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BG026759.D

Acq: 28 Apr 2017 22:57

Instrument :

BNA_G

ClientSampleId :

JHT41

Tgt Ion:163 Resp: 149124

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 9.8 9.0 13.4

