

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042817\
 Data File : BG026752.D
 Acq On : 28 Apr 2017 18:24
 Operator : SJ/MA
 Sample : I2816-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT20

Manual Integrations
 APPROVED

mohammad
 5/1/2017 7:23:25 PM

Quant Time: Apr 29 01:06:29 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:39:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	137914	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	702085	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	412677	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	813041	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	731924	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	752480	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	20493	6.69	ng/uL	0.00
5) Phenol-d5	7.19	99	457904	37.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	262242	36.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	366594	35.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	397885	38.95	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	207306	35.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	233774	36.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	366926m	36.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	591691	43.59	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1222555	36.81	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1523634	36.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	198407	33.14	ng/ul	0.00
57) Fluorene-d10	15.61	176	1046801	36.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	153656	31.12	ng/ul	0.00
70) Anthracene-d10	17.45	188	1472408	37.32	ng/ul	0.00
76) Pyrene-d10	19.73	212	1400541	36.25	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1396455	39.25	ng/ul	0.00

Target Compounds						Ovalue
6) Phenol	7.21	94	14113	1.13	ng/ul	89
44) Dimethylphthalate	14.07	163	205582	6.32	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042817\
Data File : BG026752.D
Acq On : 28 Apr 2017 18:24
Operator : SJ/MA
Sample : I2816-08
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHT20

Quant Time: Apr 29 01:06:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:39:01 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/1/2017 7:23:25 PM

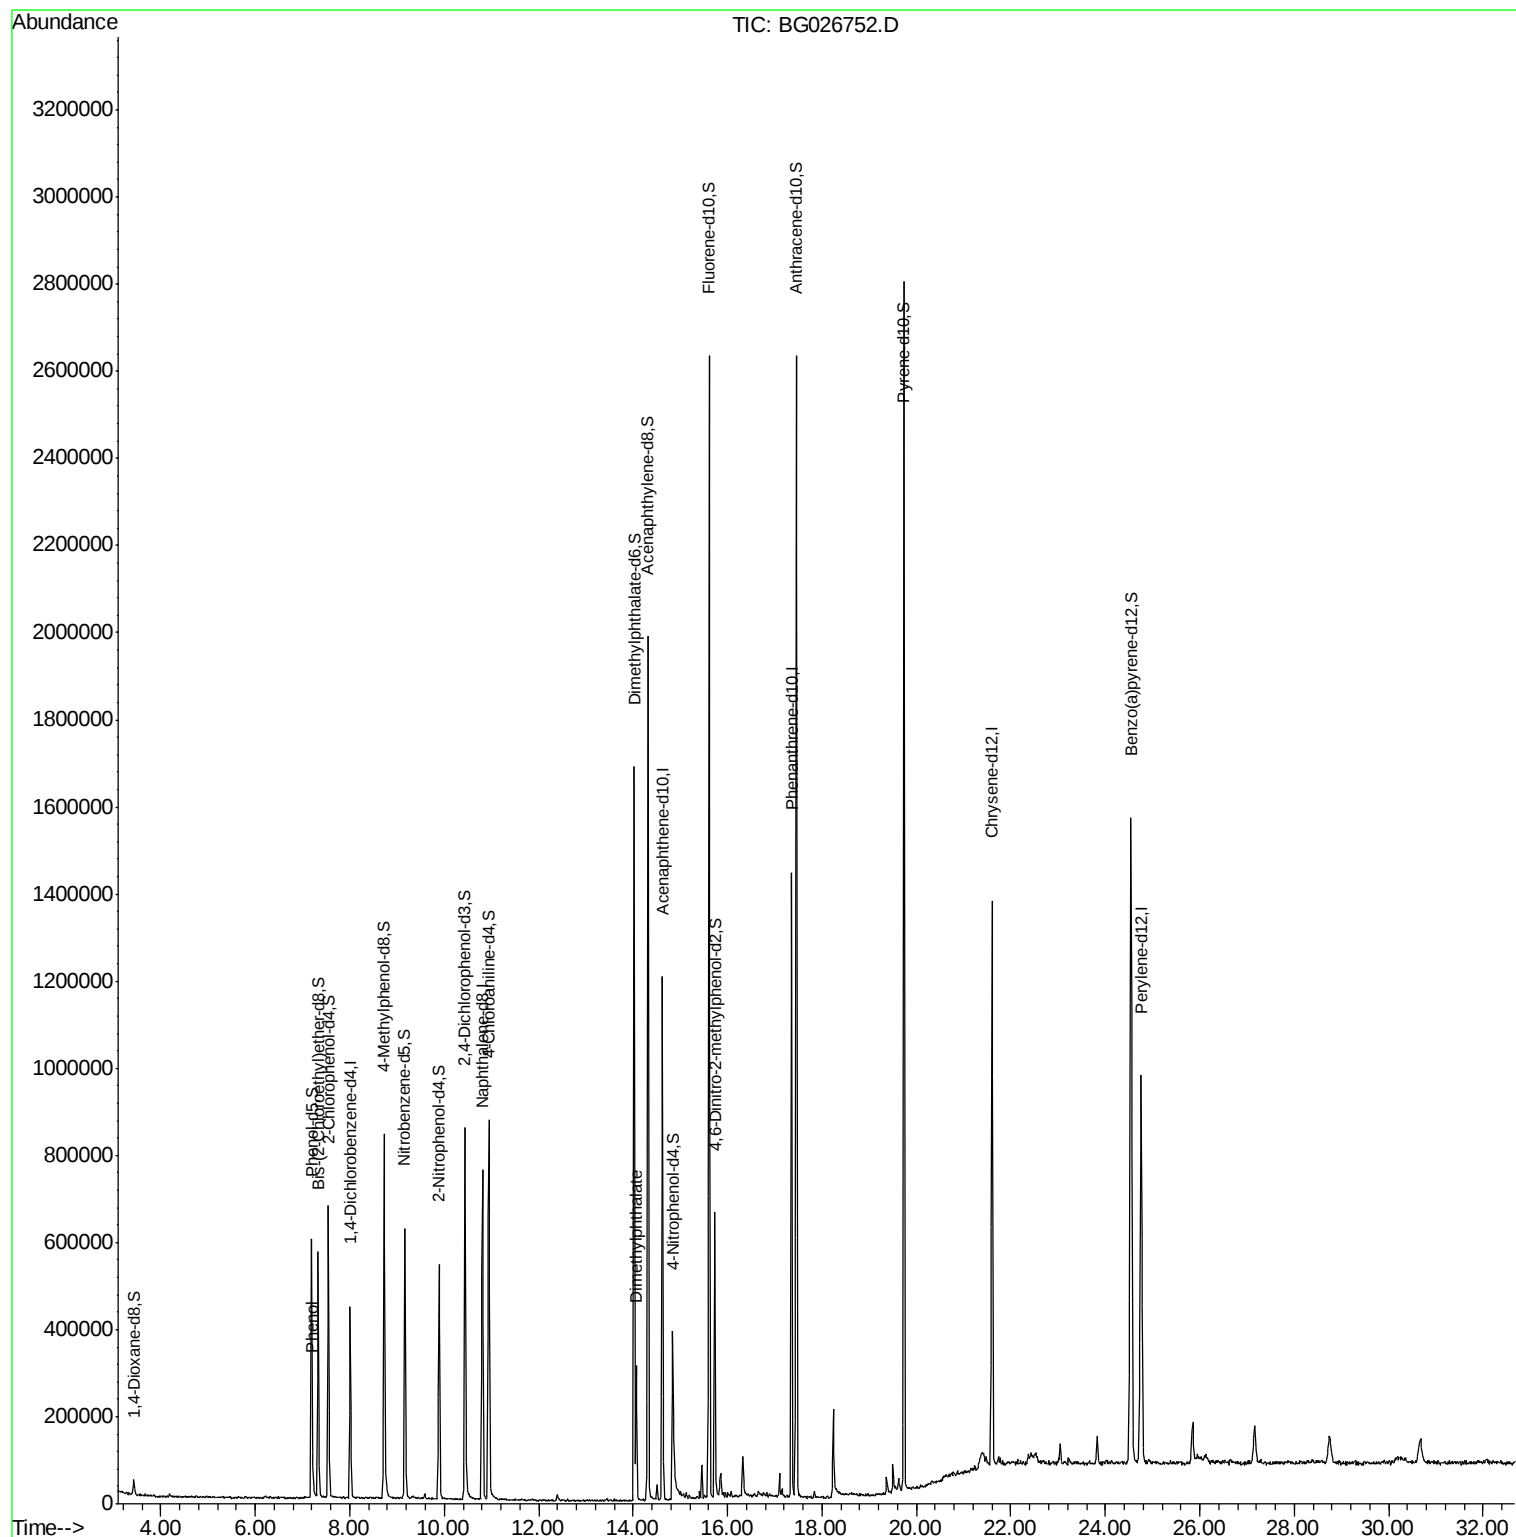

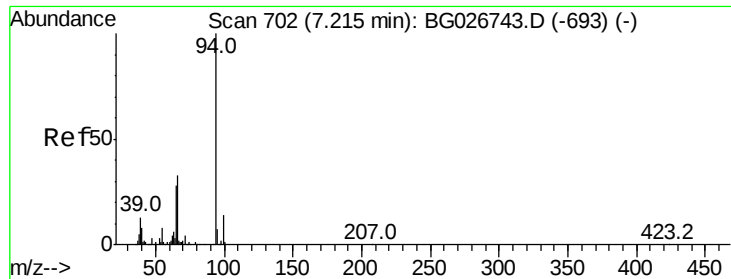

#6

Phenol

Concen: 1.13 ng/ul

RT: 7.21 min Scan# 702

Delta R.T. -0.00 min

Lab File: BG026752.D

Acq: 28 Apr 2017 18:24

Instrument :

BNA_G

ClientSampleId :

JHT20

Tot Ion: 94 Resp: 14113

Ion Ratio Lower Upper

94 100





65 27.9 26.8 40.2

66 47.4 44.4 66.6

Manual Integrations
APPROVED

mohammad

5/1/2017 7:23:25 PM

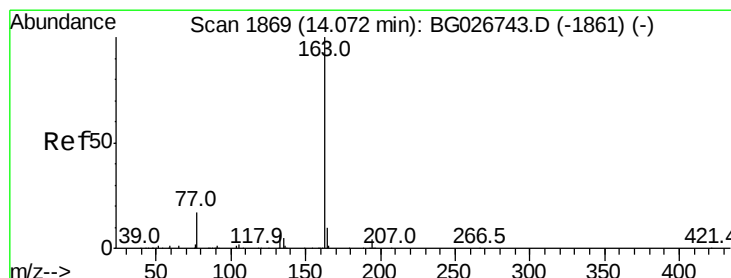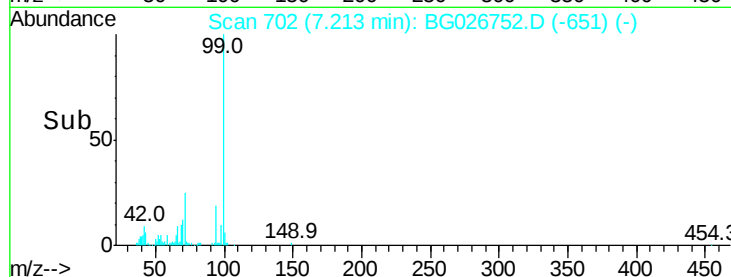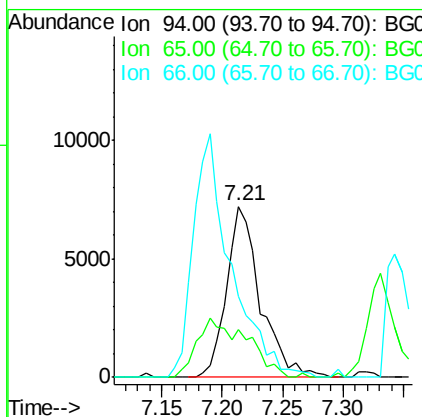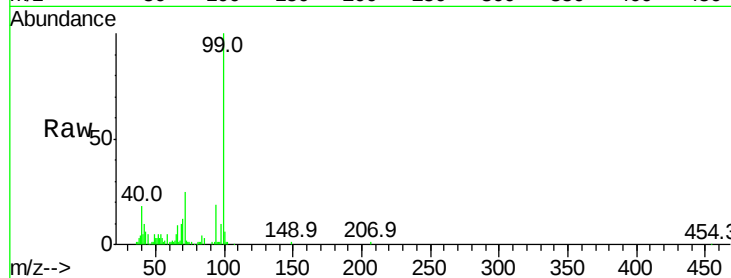

#44

Dimethylphthalate

Concen: 6.32 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG026752.D

Acq: 28 Apr 2017 18:24

Tgt Ion: 163 Resp: 205582

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 10.1 9.0 13.4

