

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057222.D
 Acq On : 28 Apr 2023 17:27
 Operator : CG/JU
 Sample : 02417-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8X9

Quant Time: Apr 29 00:53:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:37:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.375	152	13387	20.000	ng/ul	0.00
20) Naphthalene-d8	11.213	136	57517	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.990	164	46853	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.728	188	122706	20.000	ng/ul	0.00
79) Chrysene-d12	22.033	240	115477	20.000	ng/ul	0.00
88) Perylene-d12	25.546	264	117764	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.652	96	860	2.827	ng/uL	0.00
4) Pyridine-d5	4.099	84	126	0.131	ng/ul	0.00
7) Phenol-d5	7.512	99	19208	15.172	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.682	67	13099	17.591	ng/ul	0.00
11) 2-Chlorophenol-d4	7.900	132	13365	16.019	ng/ul	0.00
15) 4-Methylphenol-d8	9.075	113	15181	15.777	ng/ul	0.00
21) Nitrobenzene-d5	9.550	128	7803	17.036	ng/ul	0.00
24) 2-Nitrophenol-d4	10.285	143	9159	17.134	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.831	165	15851	15.370	ng/ul	0.00
31) 4-Chloroaniline-d4	11.342	131	19578	14.323	ng/ul	0.00
46) Dimethylphthalate-d6	14.373	166	72426	19.509	ng/ul	0.00
49) Acenaphthylene-d8	14.685	160	74508	17.857	ng/ul	0.00
54) 4-Nitrophenol-d4	15.172	143	6888	12.746	ng/ul	0.00
60) Fluorene-d10	15.971	176	64564	18.668	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.089	200	8735	12.015	ng/ul	0.00
73) Anthracene-d10	17.822	188	110008	19.641	ng/ul	0.00
81) Pyrene-d10	20.089	212	141340	20.621	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.300	264	122874	20.480	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.204	105	2500	1.510	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057222.D
Acq On : 28 Apr 2023 17:27
Operator : CG/JU
Sample : 02417-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8X9


Quant Time: Apr 29 00:53:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 23:37:02 2023
Response via : Initial Calibration

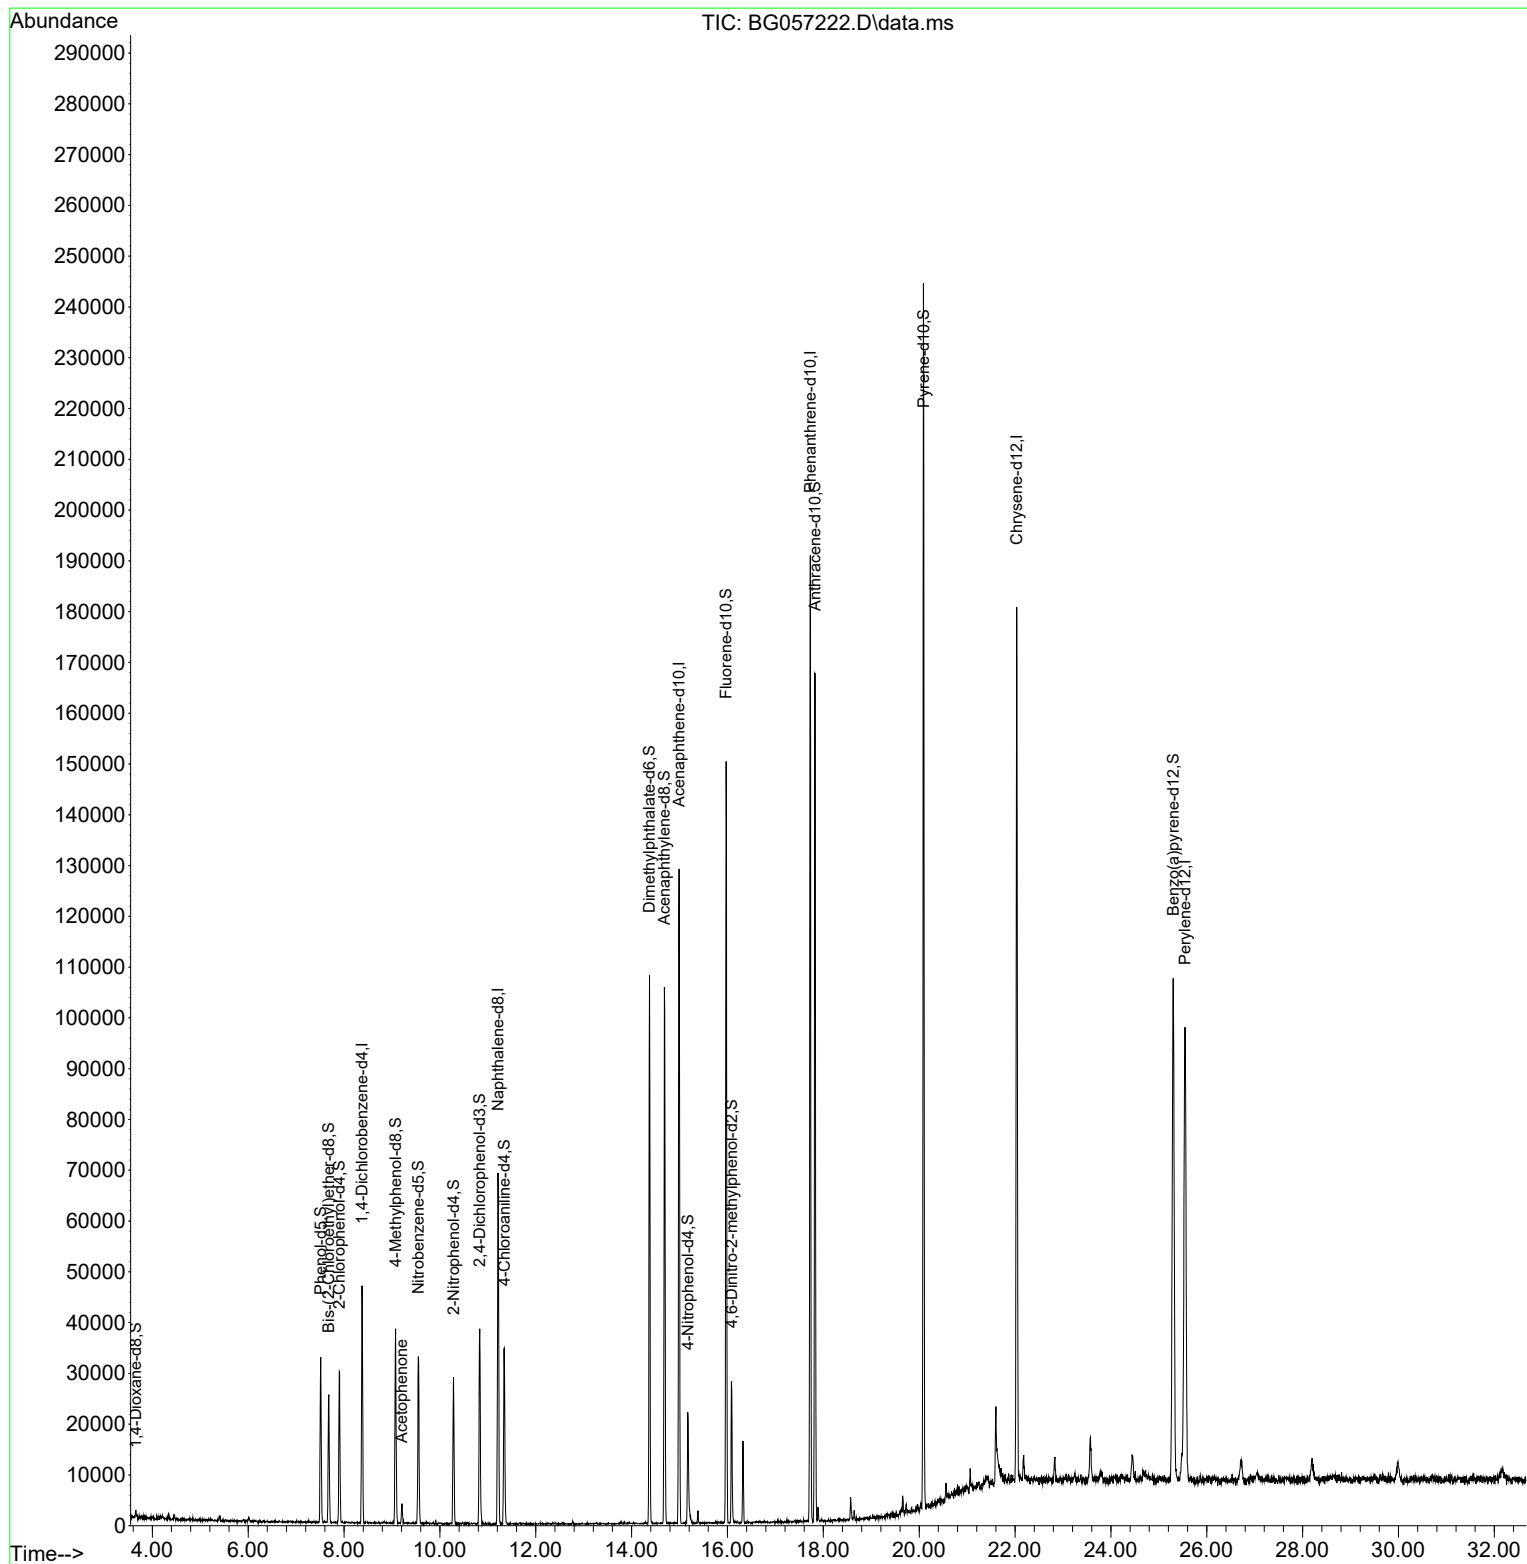

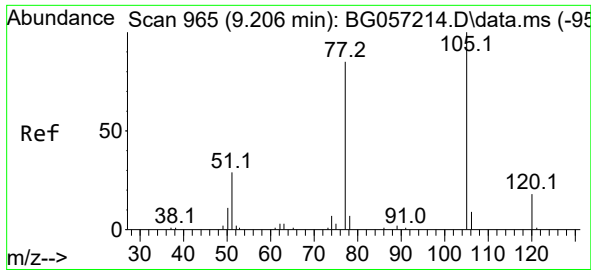

#16
 Acetophenone
 Concen: 1.510 ng/ul
 RT: 9.204 min Scan# 90
 Delta R.T. -0.002 min
 Lab File: BG057222.D
 Acq: 28 Apr 2023 17:27

Instrument :
 BNA_G
 ClientSampleId :
 EW8X9

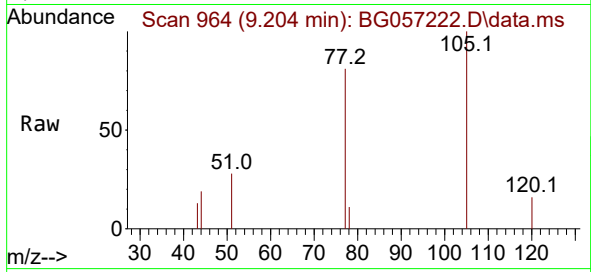

Tgt Ion:	105	Resp:	2500
Ion	Ratio	Lower	Upper
105	100		
77	80.6	70.6	105.8
51	27.7	24.5	36.7

