

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057238.D
 Acq On : 29 Apr 2023 5:50
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020466

Quant Time: May 01 00:28:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:37:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.379	152	14885	20.000	ng/u1	0.00
20) Naphthalene-d8	11.216	136	61981	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.988	164	51054	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.725	188	128768	20.000	ng/u1	0.00
79) Chrysene-d12	22.037	240	118714	20.000	ng/u1	# 0.00
88) Perylene-d12	25.544	264	123924	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.656	96	2512	7.426	ng/uL	0.00
4) Pyridine-d5	4.096	84	19790	18.558	ng/u1	0.00
7) Phenol-d5	7.509	99	28661	20.360	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.680	67	16430	19.844	ng/u1	0.00
11) 2-Chlorophenol-d4	7.903	132	19278	20.781	ng/u1	0.00
15) 4-Methylphenol-d8	9.078	113	22646	21.167	ng/u1	0.00
21) Nitrobenzene-d5	9.554	128	10717	21.712	ng/u1	0.00
24) 2-Nitrophenol-d4	10.288	143	12436	21.589	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.828	165	24693	22.219	ng/u1	0.00
31) 4-Chloroaniline-d4	11.345	131	33208	22.545	ng/u1	0.00
46) Dimethylphthalate-d6	14.377	166	84761	20.953	ng/u1	0.00
49) Acenaphthylene-d8	14.688	160	97472	21.438	ng/u1	0.00
54) 4-Nitrophenol-d4	15.170	143	11670	19.818	ng/u1	0.00
60) Fluorene-d10	15.974	176	81211	21.550	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.086	200	16221	21.261	ng/u1	0.00
73) Anthracene-d10	17.825	188	129044	21.955	ng/u1	0.00
81) Pyrene-d10	20.092	212	151979	21.568	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.297	264	136686	21.649	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.697	88	2841	7.920	ng/uL	86
5) Pyridine	4.120	79	21354	18.996	ng/u1	93
6) Benzaldehyde	7.504	77	8729	20.303	ng/u1#	77
8) Phenol	7.539	94	28740	20.256	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.774	93	21306	20.064	ng/u1	95
12) 2-Chlorophenol	7.938	128	20684	21.228	ng/u1	98
13) 2-Methylphenol	8.814	108	21865	19.885	ng/u1	94
14) 2,2'-oxybis(1-Chloropr...	8.896	45	26855	19.615	ng/u1#	95
16) Acetophenone	9.207	105	37646	20.448	ng/u1	98
17) N-Nitroso-di-n-propyla...	9.178	70	21029	19.877	ng/u1	98
18) 4-Methylphenol	9.143	108	23967	20.137	ng/u1	96
19) Hexachloroethane	9.477	117	9124	22.381	ng/u1	95
22) Nitrobenzene	9.595	77	32283	21.964	ng/u1	96
23) Isophorone	10.118	82	58833	21.038	ng/u1	98
25) 2-Nitrophenol	10.317	139	13079	22.416	ng/u1	93
26) 2,4-Dimethylphenol	10.359	107	28505	21.536	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.594	93	30361	20.886	ng/u1	99
29) 2,4-Dichlorophenol	10.852	162	24339	23.073	ng/u1	97
30) Naphthalene	11.269	128	74527	21.900	ng/u1	97
32) 4-Chloroaniline	11.369	127	34300	22.349	ng/u1	99
33) Hexachlorobutadiene	11.539	225	20854	23.308	ng/u1	96
34) Caprolactam	12.109	113	8026	22.601	ng/u1	90
35) 4-Chloro-3-methylphenol	12.462	107	27572	22.717	ng/u1	99
36) 2-Methylnaphthalene	12.843	142	54979	22.030	ng/u1	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057238.D
 Acq On : 29 Apr 2023 5:50
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020466

Quant Time: May 01 00:28:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:37:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	13.061	142	55890	22.272	ng/ul#	96
39) 1,2,4,5-Tetrachloroben...	13.202	216	41057	22.130	ng/ul	98
40) Hexachlorocyclopentadiene	13.178	237	15553	16.799	ng/ul	99
41) 2,4,6-Trichlorophenol	13.437	196	24752	22.907	ng/ul	91
42) 2,4,5-Trichlorophenol	13.513	196	27007	23.280	ng/ul	94
43) 1,1'-Biphenyl	13.824	154	80688	20.713	ng/ul#	96
44) 2-Chloronaphthalene	13.877	162	64841	21.467	ng/ul	97
45) 2-Nitroaniline	14.071	65	20487	22.467	ng/ul	97
47) Dimethylphthalate	14.424	163	85201	20.973	ng/ul	99
48) 2,6-Dinitrotoluene	14.553	165	17802	21.294	ng/ul	93
50) Acenaphthylene	14.717	152	96883	20.969	ng/ul	99
51) 3-Nitroaniline	14.888	138	12410	20.950	ng/ul	98
52) Acenaphthene	15.052	153	69037	20.971	ng/ul	99
53) 2,4-Dinitrophenol	15.099	184	8536	19.173	ng/ul	88
55) 4-Nitrophenol	15.187	109	14307	21.433	ng/ul	97
56) Dibenzofuran	15.387	168	101720	21.398	ng/ul	98
57) 2,4-Dinitrotoluene	15.340	165	26341	22.009	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.610	232	24500	23.241	ng/ul#	98
59) Diethylphthalate	15.769	149	87404	21.177	ng/ul	99
61) Fluorene	16.027	166	85747	21.331	ng/ul	100
62) 4-Chlorophenyl-phenyle...	16.010	204	50645	21.586	ng/ul	96
63) 4-Nitroaniline	16.045	138	9756	17.391	ng/ul	99
66) 4,6-Dinitro-2-methylph...	16.104	198	16554	21.293	ng/ul	95
67) N-Nitrosodiphenylamine	16.221	169	72499	21.554	ng/ul	99
68) 4-Bromophenyl-phenylether	16.903	248	34371	22.332	ng/ul	96
69) Hexachlorobenzene	17.032	284	36731	22.664	ng/ul	98
70) Atrazine	17.149	200	33004	22.077	ng/ul	100
71) Pentachlorophenol	17.378	266	14617	19.512	ng/ul	99
72) Phenanthrene	17.772	178	142999	21.325	ng/ul	99
74) Anthracene	17.860	178	143749	21.341	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.801	216	42589	21.990	ng/ul	98
76) Pentachlorobenzene	15.305	250	44023	22.331	ng/ul	98
77) Carbazole	18.125	167	119202	21.176	ng/ul	99
78) Di-n-butylphthalate	18.647	149	138644	21.539	ng/ul	100
80) Fluoranthene	19.758	202	176982	21.144	ng/ul	98
82) Pyrene	20.122	202	176974	20.885	ng/ul	98
83) Butylbenzylphthalate	20.974	149	58809	21.672	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.913	252	63479	24.077	ng/ul	95
85) Benzo(a)anthracene	22.013	228	180594	21.509	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.861	149	84050	21.296	ng/ul	97
87) Chrysene	22.084	228	169717	21.425	ng/ul	98
89) Di-n-octyl phthalate	23.159	149	141158	20.627	ng/ul	100
90) Benzo(b)fluoranthene	24.416	252	188485	21.964	ng/ul	98
91) Benzo(k)fluoranthene	24.492	252	177740	21.289	ng/ul	99
93) Benzo(a)pyrene	25.379	252	156451	21.117	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	29.591	276	199822	21.576	ng/ul	97
95) Dibenzo(a,h)anthracene	29.650	278	166206	21.643	ng/ul	95
96) Benzo(g,h,i)perylene	30.866	276	160268	21.383	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 7.920 ng/uL

RT: 3.697 min Scan# 21

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion: 88 Resp: 2841

Ion Ratio Lower Upper

88 100

43 32.5 28.2 42.4

58 63.4 63.3 94.9



#5

Pyridine

Concen: 18.996 ng/uL

RT: 4.120 min Scan# 99

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion: 79 Resp: 21354


Ion Ratio Lower Upper

79 100

52 70.0 62.4 93.6

51 38.4 29.0 43.4









#6
Benzaldehyde
Concen: 20.303 ng/ul
RT: 7.504 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion: 77 Resp: 8729
Ion Ratio Lower Upper
77 100
105 80.3 79.8 119.6
106 72.7 78.7 118.1#



#8
Phenol
Concen: 20.256 ng/ul
RT: 7.539 min Scan# 681
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion: 94 Resp: 28740
Ion Ratio Lower Upper
94 100
65 31.1 25.5 38.3
66 48.0 36.9 55.3









#10
Bis(2-Chloroethyl)ether
Concen: 20.064 ng/ul
RT: 7.774 min Scan# 721
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion: 93 Resp: 21306
Ion Ratio Lower Upper
93 100
63 78.7 67.2 100.8
95 34.8 26.3 39.5



#12
2-Chlorophenol
Concen: 21.228 ng/ul
RT: 7.938 min Scan# 749
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:128 Resp: 20684
Ion Ratio Lower Upper
128 100
64 50.2 41.3 61.9
130 32.1 24.6 37.0



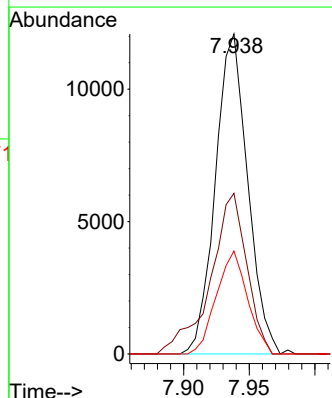





#13
2-Methylphenol
Concen: 19.885 ng/ul
RT: 8.814 min Scan# 898
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:108 Resp: 21865
Ion Ratio Lower Upper
108 100
107 94.0 80.0 120.0

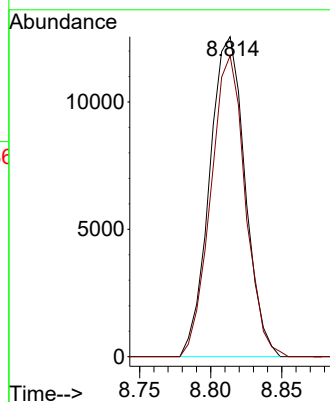

#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.615 ng/ul
RT: 8.896 min Scan# 912
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion: 45 Resp: 26855
Ion Ratio Lower Upper
45 100
77 15.8 12.9 19.3
79 15.4 8.9 13.3#


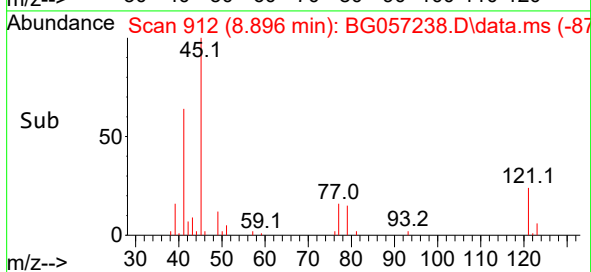
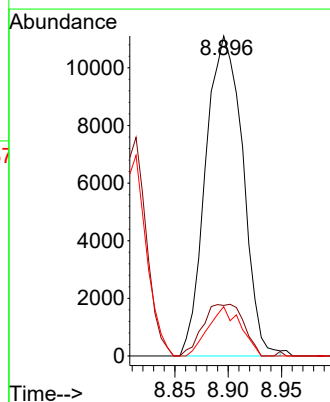
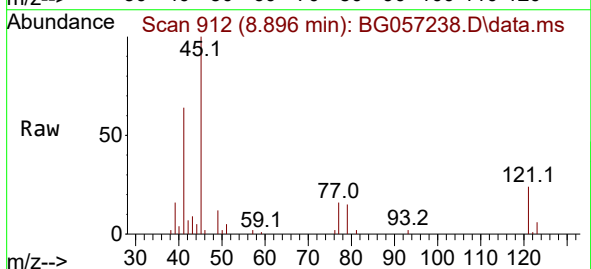




#16
Acetophenone
Concen: 20.448 ng/ul
RT: 9.207 min Scan# 90
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:105 Resp: 37646
Ion Ratio Lower Upper
105 100
77 86.8 70.6 105.8
51 29.2 24.5 36.7

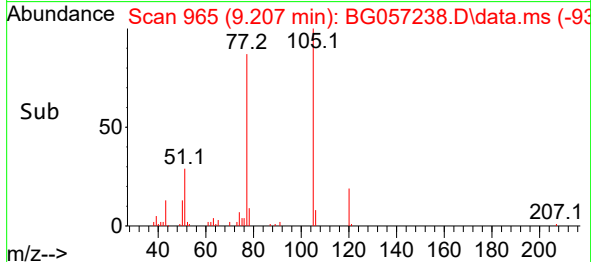

#17
N-Nitroso-di-n-propylamine
Concen: 19.877 ng/ul
RT: 9.178 min Scan# 960
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion: 70 Resp: 21029
Ion Ratio Lower Upper
70 100
42 57.6 45.0 67.4
101 8.7 6.5 9.7
130 18.1 15.9 23.9




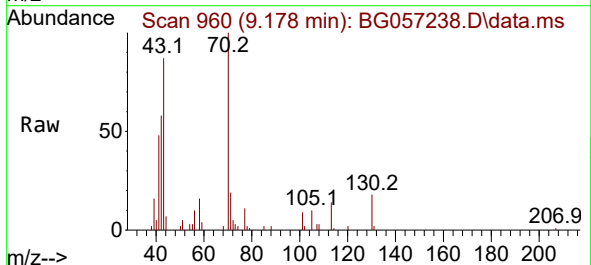




#18
4-Methylphenol
Concen: 20.137 ng/ul
RT: 9.143 min Scan# 91
Delta R.T. 0.007 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:108 Resp: 23967
Ion Ratio Lower Upper
108 100
107 110.4 85.1 127.7



#19
Hexachloroethane
Concen: 22.381 ng/ul
RT: 9.477 min Scan# 1011
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:117 Resp: 9124
Ion Ratio Lower Upper
117 100
201 143.6 109.4 164.2
199 84.9 65.4 98.2









#22
Nitrobenzene
Concen: 21.964 ng/ul
RT: 9.595 min Scan# 1031
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion: 77 Resp: 32283
Ion Ratio Lower Upper
77 100
123 34.4 29.6 44.4
65 15.4 11.4 17.0



#23
Isophorone
Concen: 21.038 ng/ul
RT: 10.118 min Scan# 1120
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion: 82 Resp: 58833
Ion Ratio Lower Upper
82 100
95 9.0 6.8 10.2
138 16.4 12.2 18.2



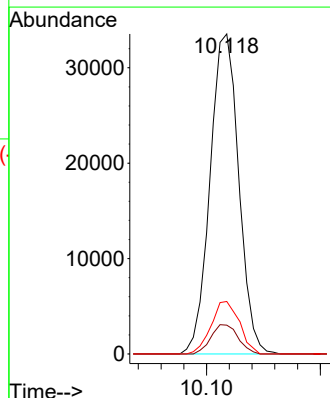





#25
2-Nitrophenol
Concen: 22.416 ng/ul
RT: 10.317 min Scan# 1154
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:139 Resp: 13079
Ion Ratio Lower Upper
139 100
65 65.5 48.7 73.1
109 49.3 35.2 52.8

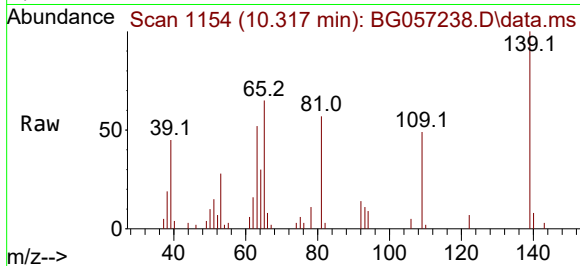

#26
2,4-Dimethylphenol
Concen: 21.536 ng/ul
RT: 10.359 min Scan# 1161
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:107 Resp: 28505
Ion Ratio Lower Upper
107 100
121 43.6 35.4 53.0
122 75.1 57.0 85.4

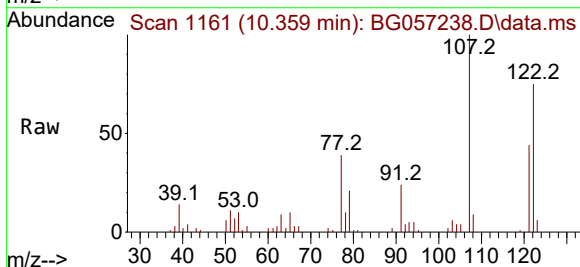



#27

Bis(2-Chloroethoxy)methane

Concen: 20.886 ng/ul

RT: 10.594 min Scan# 1

Delta R.T. 0.007 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion: 93 Resp: 30361

Ion Ratio Lower Upper

93 100

95 30.8 24.8 37.2

123 8.7 8.1 12.1

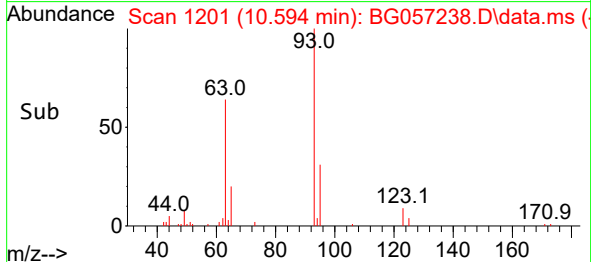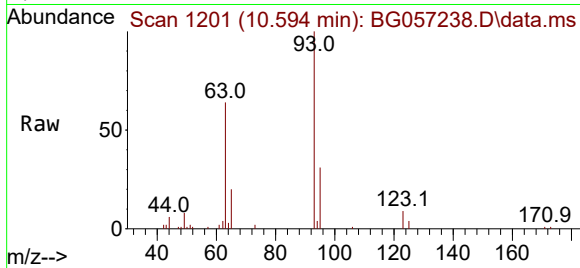

#29

2,4-Dichlorophenol

Concen: 23.073 ng/ul

RT: 10.852 min Scan# 1245

Delta R.T. -0.005 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:162 Resp: 24339


Ion Ratio Lower Upper

162 100

164 60.1 50.5 75.7

98 33.9 27.5 41.3


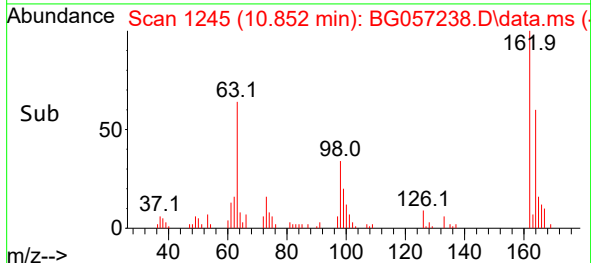
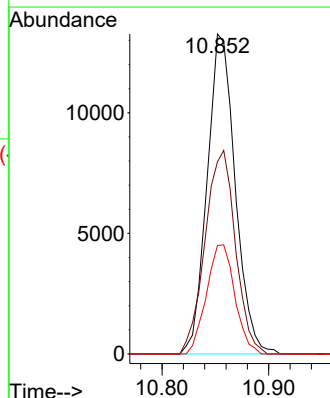
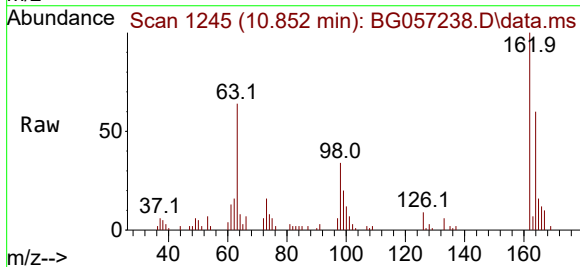




#30
Naphthalene
Concen: 21.900 ng/ul
RT: 11.269 min Scan# 1126
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:128 Resp: 74527
Ion Ratio Lower Upper
128 100
129 10.3 8.5 12.7
127 12.3 11.4 17.0



#32
4-Chloroaniline
Concen: 22.349 ng/ul
RT: 11.369 min Scan# 1333
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:127 Resp: 34300
Ion Ratio Lower Upper
127 100
129 32.2 25.4 38.0









#33
Hexachlorobutadiene
Concen: 23.308 ng/ul
RT: 11.539 min Scan# 11
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:225 Resp: 20854
Ion Ratio Lower Upper
225 100
223 57.5 47.5 71.3
227 65.1 48.4 72.6

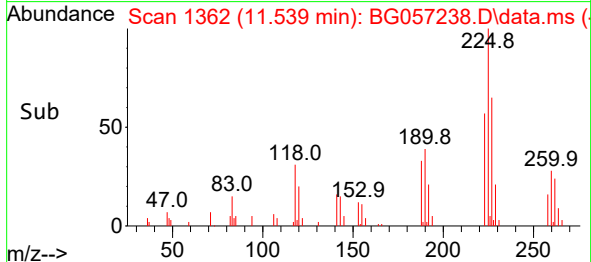

#34
Caprolactam
Concen: 22.601 ng/ul
RT: 12.109 min Scan# 1459
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:113 Resp: 8026
Ion Ratio Lower Upper
113 100
55 169.0 123.1 184.7
56 133.0 98.7 148.1









#35
 4-Chloro-3-methylphenol
 Concen: 22.717 ng/ul
 RT: 12.462 min Scan# 1519
 Delta R.T. 0.001 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020466


Tgt Ion:107 Resp: 27572
 Ion Ratio Lower Upper
 107 100
 144 24.7 18.3 27.5
 142 72.9 58.6 88.0



#36
 2-Methylnaphthalene
 Concen: 22.030 ng/ul
 RT: 12.843 min Scan# 1584
 Delta R.T. 0.001 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50

Tgt Ion:142 Resp: 54979
 Ion Ratio Lower Upper
 142 100
 141 83.3 68.7 103.1

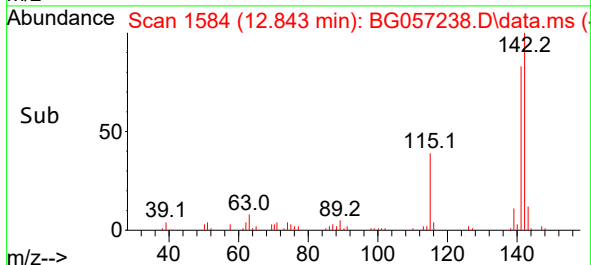



#37

1-Methylnaphthalene

Concen: 22.272 ng/ul

RT: 13.061 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:142 Resp: 55890

Ion Ratio Lower Upper

142 100

141 87.7 72.9 109.3

116 4.8 3.2 4.8#



#39

1,2,4,5-Tetrachlorobenzene

Concen: 22.130 ng/ul

RT: 13.202 min Scan# 1645

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Tgt Ion:216 Resp: 41057




Ion Ratio Lower Upper


216 100

214 80.2 62.9 94.3

179 17.9 15.3 22.9

108 13.9 11.4 17.2



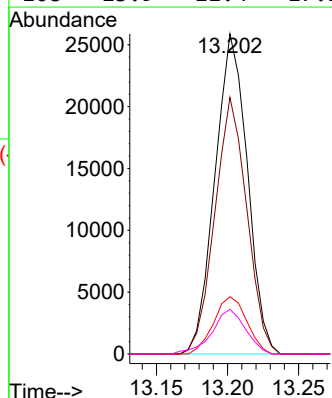





#40
Hexachlorocyclopentadiene
Concen: 16.799 ng/ul
RT: 13.178 min Scan# 1
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:237 Resp: 15553
Ion Ratio Lower Upper
237 100
235 63.2 51.4 77.0
272 12.2 9.4 14.2

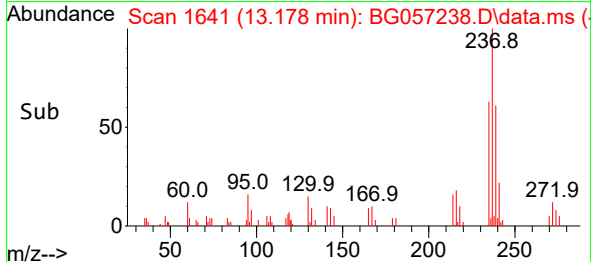

#41
2,4,6-Trichlorophenol
Concen: 22.907 ng/ul
RT: 13.437 min Scan# 1685
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:196 Resp: 24752
Ion Ratio Lower Upper
196 100
198 94.1 83.8 125.8
200 31.0 26.6 40.0





#42

2,4,5-Trichlorophenol

Concen: 23.280 ng/ul

RT: 13.513 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:196 Resp: 27007

Ion Ratio Lower Upper

196 100

198 101.1 85.7 128.5

200 33.9 29.9 44.9

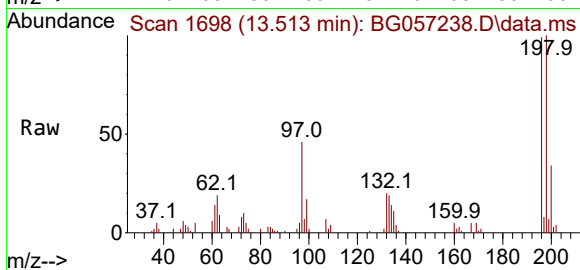

#43

1,1'-Biphenyl

Concen: 20.713 ng/ul

RT: 13.824 min Scan# 1751

Delta R.T. -0.005 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:154 Resp: 80688


Ion Ratio Lower Upper

154 100

153 41.7 31.6 47.4

76 12.1 8.0 12.0#




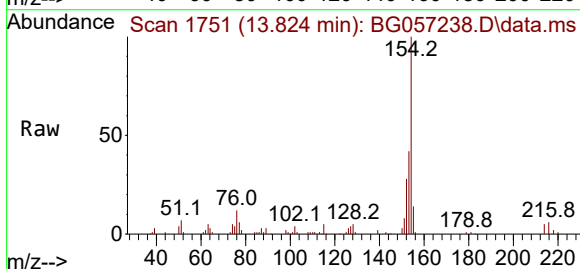




#44
2-Chloronaphthalene
Concen: 21.467 ng/ul
RT: 13.877 min Scan# 1760
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:	162	Resp:	64841
Ion Ratio	Lower	Upper	
162	100		
164	35.1	26.2	39.4
127	35.6	29.4	44.2

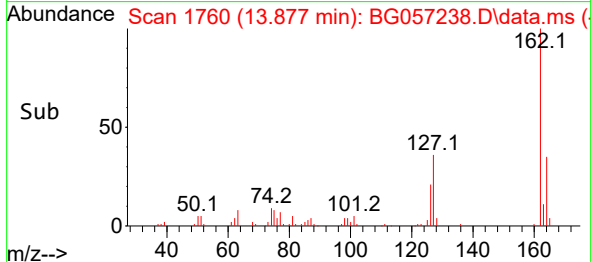

#45
2-Nitroaniline
Concen: 22.467 ng/ul
RT: 14.071 min Scan# 1793
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:	65	Resp:	20487
Ion Ratio	Lower	Upper	
65	100		
92	67.2	51.8	77.6
138	93.0	71.9	107.9

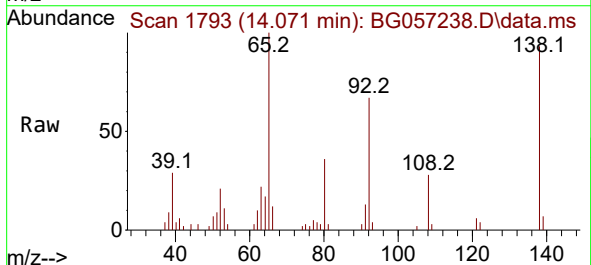



#47

Dimethylphthalate

Concen: 20.973 ng/ul

RT: 14.424 min Scan# 1853

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:163 Resp: 85201

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.2

164 10.3 8.3 12.5

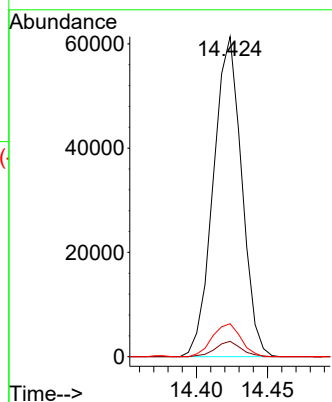

#48

2,6-Dinitrotoluene

Concen: 21.294 ng/ul

RT: 14.553 min Scan# 1875

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:165 Resp: 17802


Ion Ratio Lower Upper

165 100

89 69.9 50.6 76.0

121 18.9 16.8 25.2









#50
Acenaphthylene
Concen: 20.969 ng/ul
RT: 14.717 min Scan# 1903
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:152 Resp: 96883
Ion Ratio Lower Upper
152 100
151 20.9 16.3 24.5
153 12.9 10.1 15.1

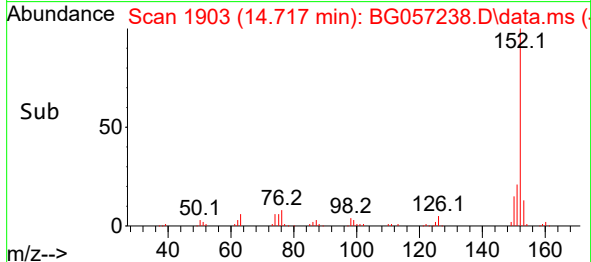

#51
3-Nitroaniline
Concen: 20.950 ng/ul
RT: 14.888 min Scan# 1932
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:138 Resp: 12410
Ion Ratio Lower Upper
138 100
108 9.5 9.2 13.8
92 123.0 99.5 149.3




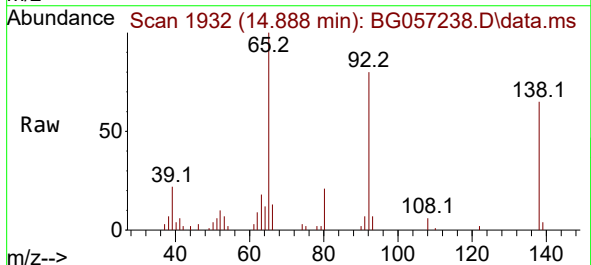




#52
Acenaphthene
Concen: 20.971 ng/ul
RT: 15.052 min Scan# 1960
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:153 Resp: 69037
Ion Ratio Lower Upper
153 100
152 45.6 36.5 54.7
154 87.3 70.6 106.0



#53
2,4-Dinitrophenol
Concen: 19.173 ng/ul
RT: 15.099 min Scan# 1968
Delta R.T. 0.007 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:184 Resp: 8536
Ion Ratio Lower Upper
184 100
63 66.8 48.3 72.5
154 74.2 50.0 75.0









#55
4-Nitrophenol
Concen: 21.433 ng/ul
RT: 15.187 min Scan# 1983
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:109 Resp: 14307
Ion Ratio Lower Upper
109 100
139 85.5 73.8 110.8
65 101.9 81.7 122.5

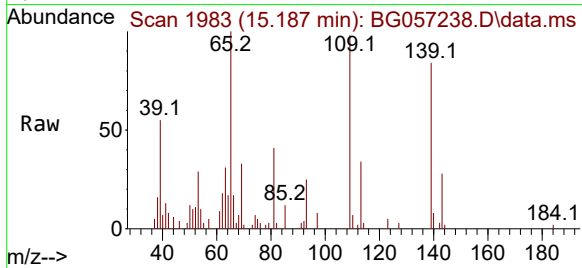

#56
Dibenzofuran
Concen: 21.398 ng/ul
RT: 15.387 min Scan# 2017
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:168 Resp: 101720
Ion Ratio Lower Upper
168 100
139 38.0 29.6 44.4

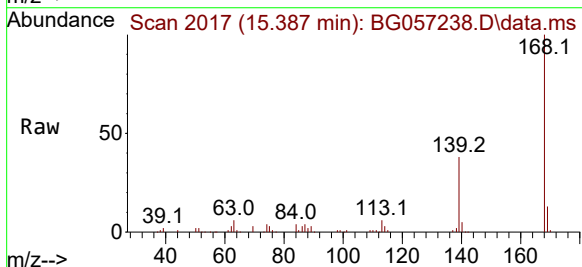



#57

2,4-Dinitrotoluene

Concen: 22.009 ng/ul

RT: 15.340 min Scan# 2009

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:165 Resp: 26341

Ion Ratio Lower Upper

165 100

63 43.3 35.9 53.9

182 2.7 1.9 2.9

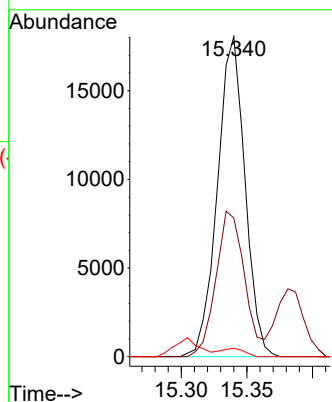

#58

2,3,4,6-Tetrachlorophenol

Concen: 23.241 ng/ul

RT: 15.610 min Scan# 2055

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Tgt Ion:232 Resp: 24500




Ion Ratio Lower Upper


232 100

131 37.9 28.6 43.0

130 2.9 1.8 2.6#

166 27.7 22.2 33.2

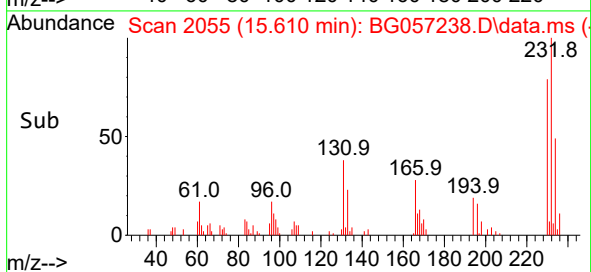

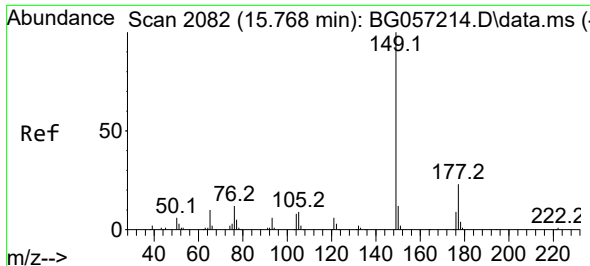


#59
Diethylphthalate
Concen: 21.177 ng/ul
RT: 15.769 min Scan# 2082
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Instrument :




BNA_G

ClientSampleId :

SSTD020466



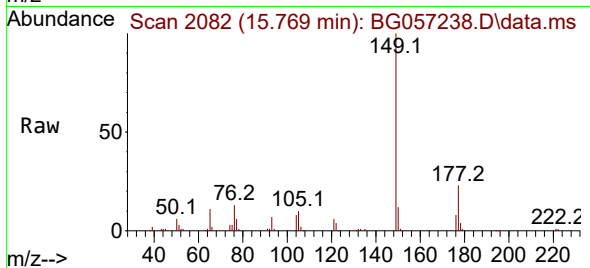



Tgt Ion:149 Resp: 87404
Ion Ratio Lower Upper
149 100
177 23.1 18.6 28.0
150 11.6 9.8 14.8

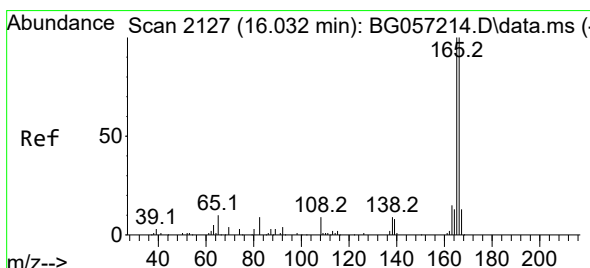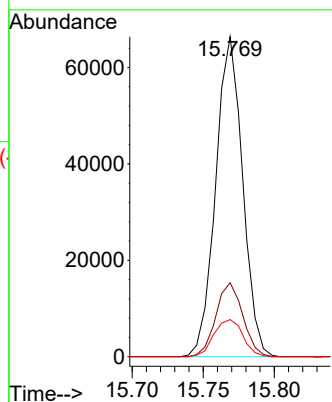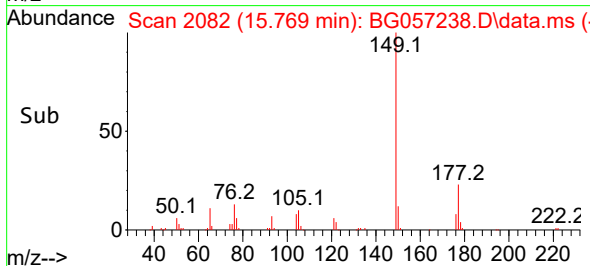

#61
Fluorene
Concen: 21.331 ng/ul
RT: 16.027 min Scan# 2126
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:166 Resp: 85747
Ion Ratio Lower Upper
166 100
165 100.4 80.1 120.1
167 12.7 10.2 15.4

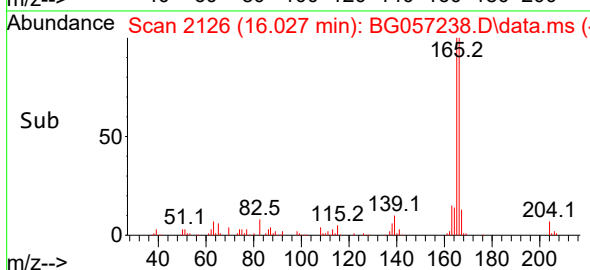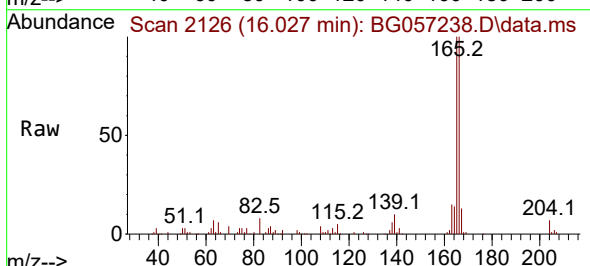



#62

4-Chlorophenyl-phenylether

Concen: 21.586 ng/ul

RT: 16.010 min Scan# 2123

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:204 Resp: 50645

Ion Ratio Lower Upper

204 100

206 32.7 26.5 39.7

141 47.4 41.5 62.3

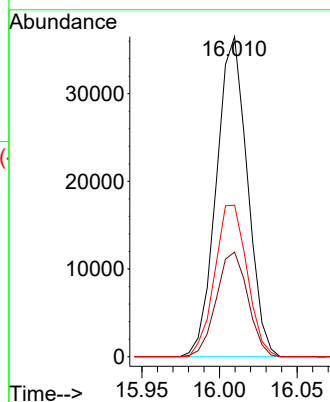

#63

4-Nitroaniline

Concen: 17.391 ng/ul

RT: 16.045 min Scan# 2129

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:138 Resp: 9756


Ion Ratio Lower Upper

138 100

92 50.0 39.9 59.9

108 112.3 89.1 133.7









#66
4,6-Dinitro-2-methylphenol
Concen: 21.293 ng/ul
RT: 16.104 min Scan# 2138
Delta R.T. 0.007 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:198 Resp: 16554
Ion Ratio Lower Upper
198 100
182 3.7 3.0 4.6
77 22.3 20.1 30.1

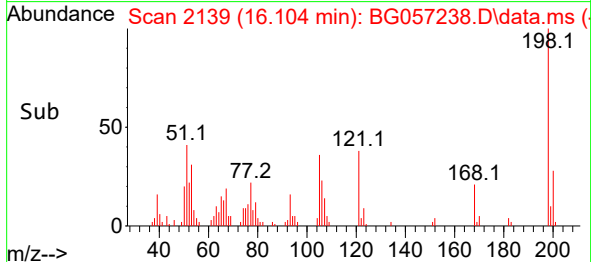

#67
N-Nitrosodiphenylamine
Concen: 21.554 ng/ul
RT: 16.221 min Scan# 2159
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:169 Resp: 72499
Ion Ratio Lower Upper
169 100
168 69.7 55.4 83.2
167 37.9 31.0 46.4


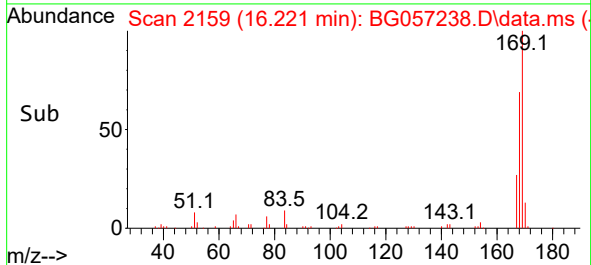






#68
4-Bromophenyl-phenylether
Concen: 22.332 ng/ul
RT: 16.903 min Scan# 21
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:248 Resp: 34371
Ion Ratio Lower Upper
248 100
250 95.6 74.8 112.2
141 65.3 47.8 71.6

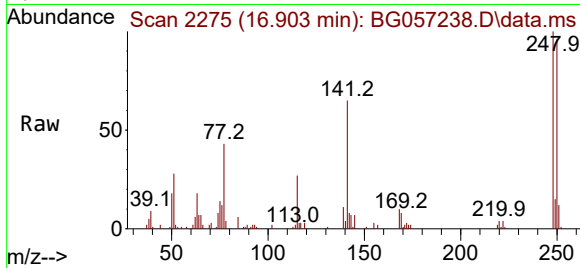

#69
Hexachlorobenzene
Concen: 22.664 ng/ul
RT: 17.032 min Scan# 2297
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:284 Resp: 36731
Ion Ratio Lower Upper
284 100
142 28.1 22.6 33.8
249 34.5 26.2 39.2


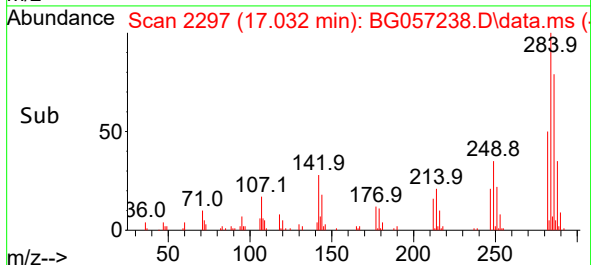
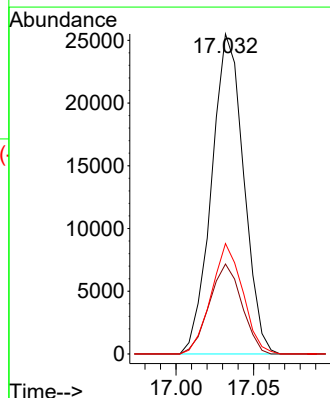
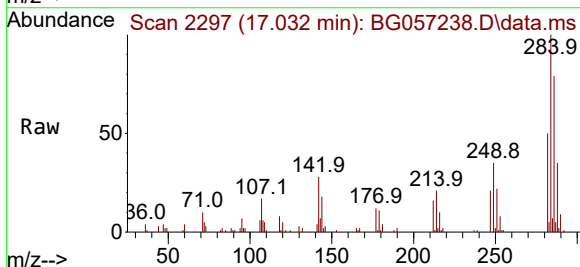




#70
 Atrazine
 Concen: 22.077 ng/ul
 RT: 17.149 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50




Instrument :
 BNA_G
 ClientSampleId :
 SST020466


Tgt Ion:200 Resp: 33004
 Ion Ratio Lower Upper
 200 100
 173 22.3 17.8 26.6
 215 50.0 40.3 60.5



#71
 Pentachlorophenol
 Concen: 19.512 ng/ul
 RT: 17.378 min Scan# 2356
 Delta R.T. 0.001 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50

Tgt Ion:266 Resp: 14617
 Ion Ratio Lower Upper
 266 100
 264 58.8 47.8 71.6
 268 61.5 48.2 72.4



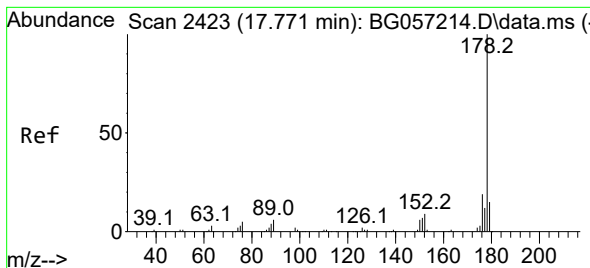

#72

Phenanthrene

Concen: 21.325 ng/ul

RT: 17.772 min Scan# 2423

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:178 Resp: 142999

Ion Ratio Lower Upper

178 100

179 14.5 11.8 17.8

176 18.7 15.4 23.0

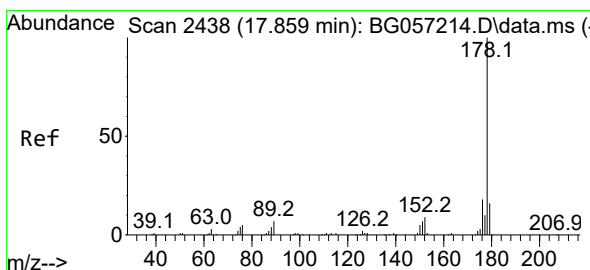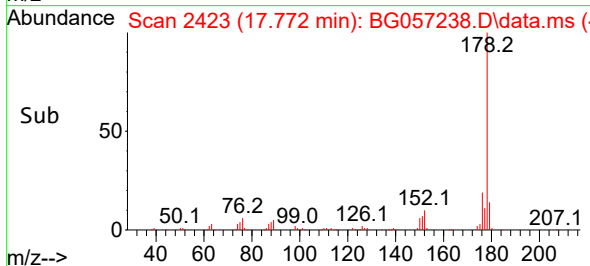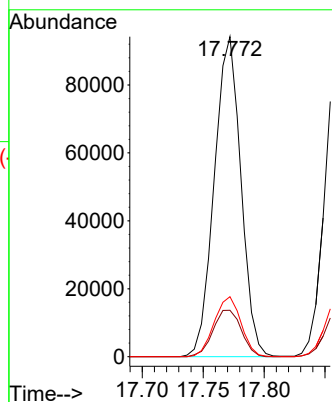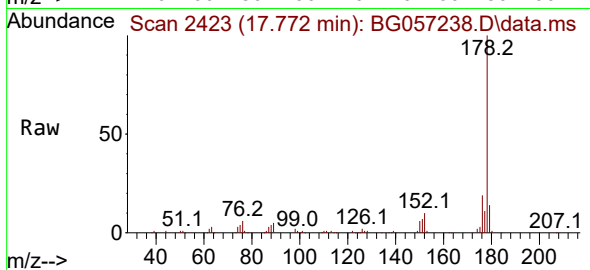

#74

Anthracene

Concen: 21.341 ng/ul

RT: 17.860 min Scan# 2438

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:178 Resp: 143749


Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 18.5 14.7 22.1


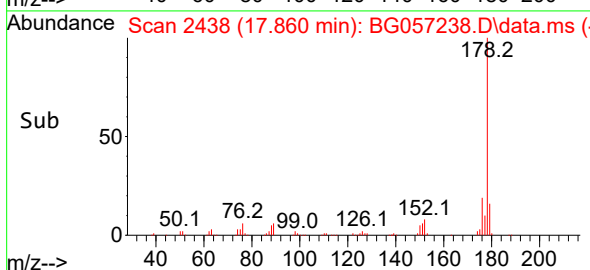

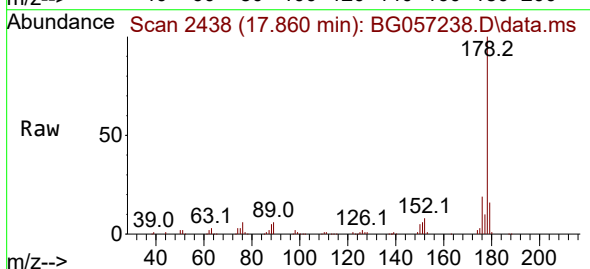




#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.990 ng/uL
RT: 13.801 min Scan# 1
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:216 Resp: 42589
Ion Ratio Lower Upper
216 100
214 78.7 64.3 96.5
218 46.7 38.5 57.7



#76
Pentachlorobenzene
Concen: 22.331 ng/uL
RT: 15.305 min Scan# 2003
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:250 Resp: 44023
Ion Ratio Lower Upper
250 100
248 62.8 52.2 78.2
252 65.4 52.5 78.7







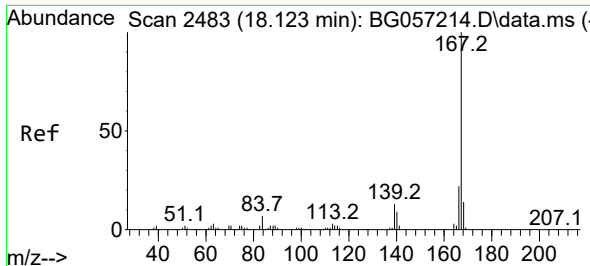

#77
 Carbazole
 Concen: 21.176 ng/ul
 RT: 18.125 min Scan# 2483
 Delta R.T. 0.001 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020466


Tgt Ion:167 Resp: 119202
 Ion Ratio Lower Upper
 167 100
 166 23.1 18.0 27.0
 139 12.2 10.3 15.5

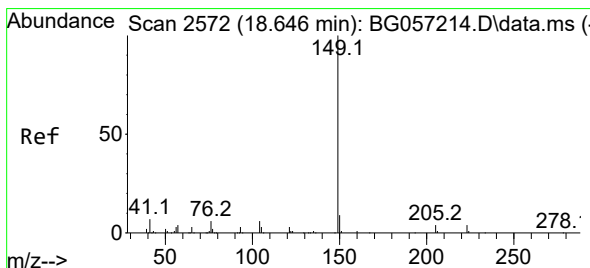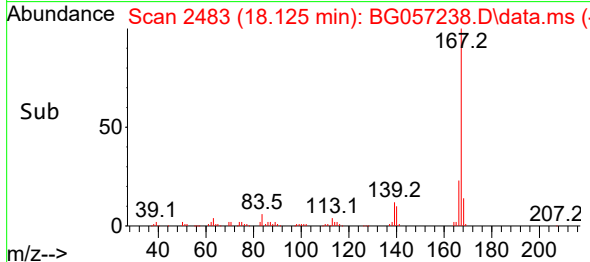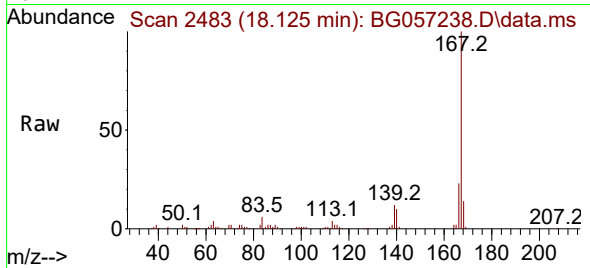

#78
 Di-n-butylphthalate
 Concen: 21.539 ng/ul
 RT: 18.647 min Scan# 2572
 Delta R.T. 0.001 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50

Tgt Ion:149 Resp: 138644
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.3 10.9
 104 6.1 5.0 7.6


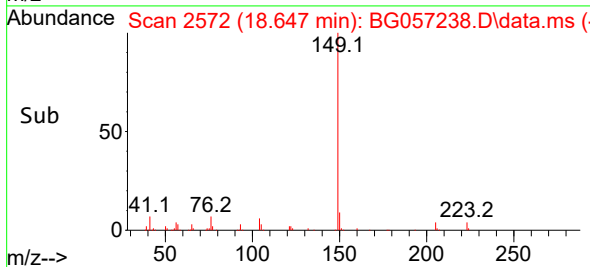

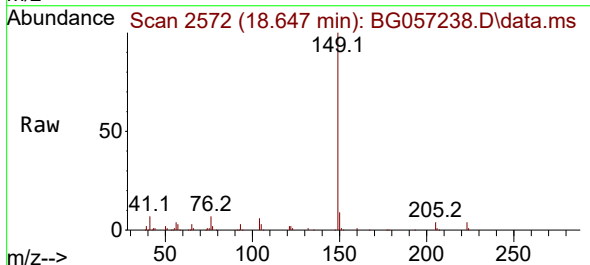


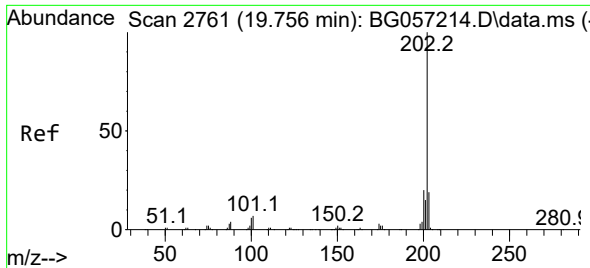

#80
Fluoranthene
Concen: 21.144 ng/ul
RT: 19.758 min Scan# 2761
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:202 Resp: 176982
Ion Ratio Lower Upper
202 100
101 6.2 5.8 8.6
100 5.4 4.6 7.0

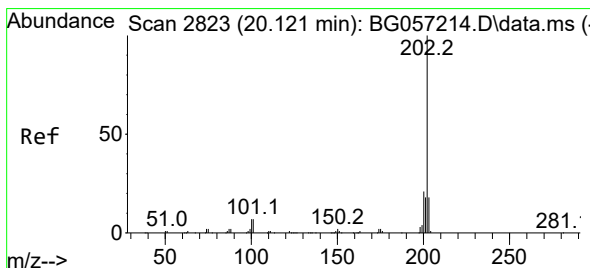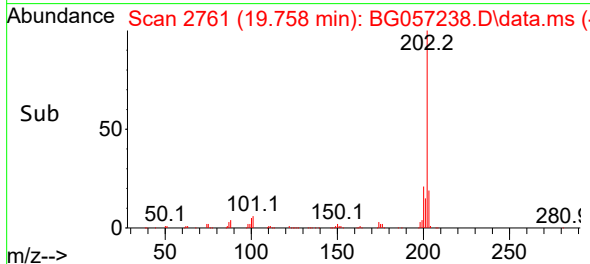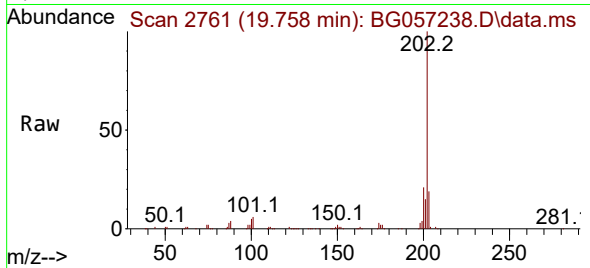

#82
Pyrene
Concen: 20.885 ng/ul
RT: 20.122 min Scan# 2823
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:202 Resp: 176974
Ion Ratio Lower Upper
202 100
101 7.1 5.7 8.5
100 6.3 6.0 9.0

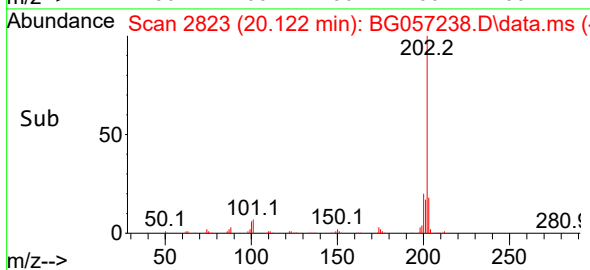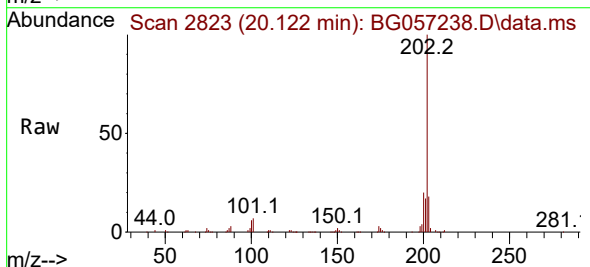



#83

Butylbenzylphthalate

Concen: 21.672 ng/ul

RT: 20.974 min Scan# 2968

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:149 Resp: 58809

Ion Ratio Lower Upper

149 100

91 70.3 58.6 87.8

206 24.9 19.8 29.8



#84

3,3'-Dichlorobenzidine

Concen: 24.077 ng/ul

RT: 21.913 min Scan# 3128

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:252 Resp: 63479


Ion Ratio Lower Upper

252 100

254 63.1 53.7 80.5

126 6.1 5.2 7.8









#85
Benzo(a)anthracene
Concen: 21.509 ng/ul
RT: 22.013 min Scan# 3119
Delta R.T. 0.001 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:228 Resp: 180594
Ion Ratio Lower Upper
228 100
229 19.9 15.8 23.6
226 27.5 21.7 32.5

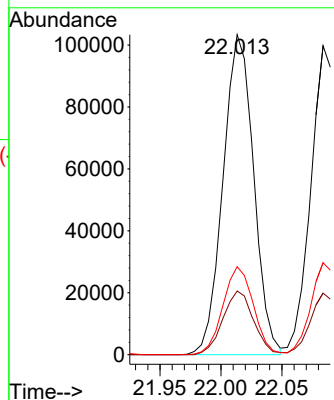

#86
Bis(2-ethylhexyl)phthalate
Concen: 21.296 ng/ul
RT: 21.861 min Scan# 3119
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:149 Resp: 84050
Ion Ratio Lower Upper
149 100
167 26.8 23.0 34.6
279 4.5 3.6 5.4



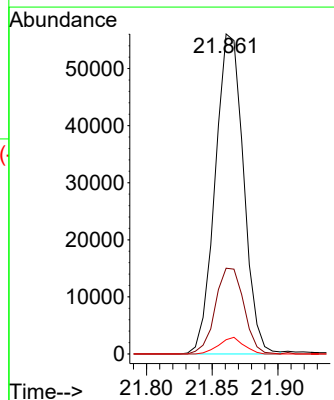





#87
Chrysene
Concen: 21.425 ng/ul
RT: 22.084 min Scan# 3157
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50




Instrument :
BNA_G
ClientSampleId :
SSTD020466


Tgt Ion:228 Resp: 169717
Ion Ratio Lower Upper
228 100
226 29.8 22.8 34.2
229 19.9 15.5 23.3



#89
Di-n-octyl phthalate
Concen: 20.627 ng/ul
RT: 23.159 min Scan# 3340
Delta R.T. -0.005 min
Lab File: BG057238.D
Acq: 29 Apr 2023 5:50

Tgt Ion:149 Resp: 141158





#90

Benzo(b)fluoranthene

Concen: 21.964 ng/ul

RT: 24.416 min Scan# 3554

Delta R.T. -0.005 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:252 Resp: 188485

Ion Ratio Lower Upper

252 100

253 21.4 16.7 25.1

125 4.9 4.8 7.2

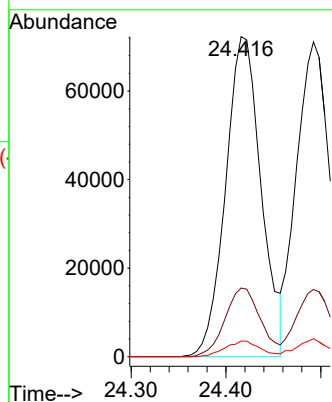

#91

Benzo(k)fluoranthene

Concen: 21.289 ng/ul

RT: 24.492 min Scan# 3567

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:252 Resp: 177740


Ion Ratio Lower Upper

252 100

253 21.3 17.7 26.5

125 5.7 4.5 6.7

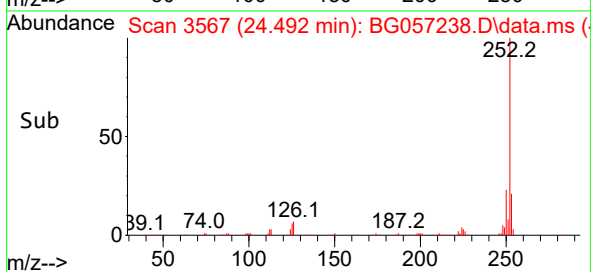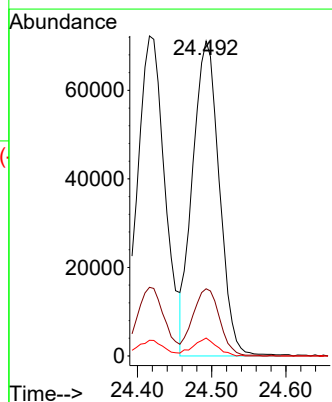



#93

Benzo(a)pyrene

Concen: 21.117 ng/ul

RT: 25.379 min Scan# 3718

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50

Instrument :

BNA_G

ClientSampleId :

SSTD020466





Tgt Ion:252 Resp: 156451

Ion Ratio Lower Upper

252 100

253 22.3 17.2 25.8

125 5.4 5.1 7.7



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.576 ng/ul

RT: 29.591 min Scan# 4435

Delta R.T. 0.001 min

Lab File: BG057238.D

Acq: 29 Apr 2023 5:50




Tgt Ion:276 Resp: 199822


Ion Ratio Lower Upper

276 100

138 10.0 9.4 14.2

277 24.4 18.6 28.0









#95
 Dibenzo(a,h)anthracene
 Concen: 21.643 ng/ul
 RT: 29.650 min Scan# 4445
 Delta R.T. -0.011 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020466

Tgt Ion:278 Resp: 166206
 Ion Ratio Lower Upper
 278 100
 139 8.4 5.8 8.6
 279 25.2 18.3 27.5



#96
 Benzo(g,h,i)perylene
 Concen: 21.383 ng/ul
 RT: 30.866 min Scan# 4652
 Delta R.T. 0.007 min
 Lab File: BG057238.D
 Acq: 29 Apr 2023 5:50

Tgt Ion:276 Resp: 160268
 Ion Ratio Lower Upper
 276 100
 138 9.2 8.7 13.1
 277 21.8 18.4 27.6

