

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057234.D
 Acq On : 29 Apr 2023 2:22
 Operator : CG/JU
 Sample : 02417-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8X4

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/01/2023
 Supervised By : Jagrut Upadhyay 05/01/2023

Quant Time: Apr 29 05:53:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:37:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.378	152	13328	20.000	ng/u1	0.00
20) Naphthalene-d8	11.215	136	55659	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.986	164	46521	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.730	188	115418	20.000	ng/u1	0.00
79) Chrysene-d12	22.036	240	99487	20.000	ng/u1	0.00
88) Perylene-d12	25.543	264	102665	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.655	96	546	1.803	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	0.00
7) Phenol-d5	7.514	99	17803	14.124	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.679	67	11294	15.234	ng/u1	0.00
11) 2-Chlorophenol-d4	7.902	132	12680	15.266	ng/u1	0.00
15) 4-Methylphenol-d8	9.077	113	9186	9.589	ng/u1	0.00
21) Nitrobenzene-d5	9.553	128	7205	16.255	ng/u1	0.00
24) 2-Nitrophenol-d4	10.281	143	8245	15.939	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.827	165	15552	15.583	ng/u1	0.00
31) 4-Chloroaniline-d4	11.338	131	15718	11.883	ng/u1	0.00
46) Dimethylphthalate-d6	14.375	166	61033	16.557	ng/u1	0.00
49) Acenaphthylene-d8	14.687	160	68896	16.629	ng/u1	0.00
54) 4-Nitrophenol-d4	15.174	143	7450	13.885	ng/u1	0.00
60) Fluorene-d10	15.973	176	57801	16.832	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.085	200	9358	13.685	ng/u1	0.00
73) Anthracene-d10	17.824	188	90211	17.123	ng/u1	0.00
81) Pyrene-d10	20.091	212	108687	18.405	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.302	264	95520	18.262	ng/u1	0.00
Target Compounds						
16) Acetophenone	9.206	105	2495	1.514	ng/u1#	89
72) Phenanthrene	17.771	178	9205	1.532	ng/u1	98
80) Fluoranthene	19.756	202	13962	1.990	ng/u1	97
82) Pyrene	20.121	202	11975	1.686	ng/u1	100
87) Chrysene	22.089	228	6691m	1.008	ng/u1	
90) Benzo(b)fluoranthene	24.432	252	8355m	1.175	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057234.D
Acq On : 29 Apr 2023 2:22
Operator : CG/JU
Sample : 02417-08
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EW8X4

Quant Time: Apr 29 05:53:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 23:37:02 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 05/01/2023
Supervised By : Jagrut Upadhyay 05/01/2023

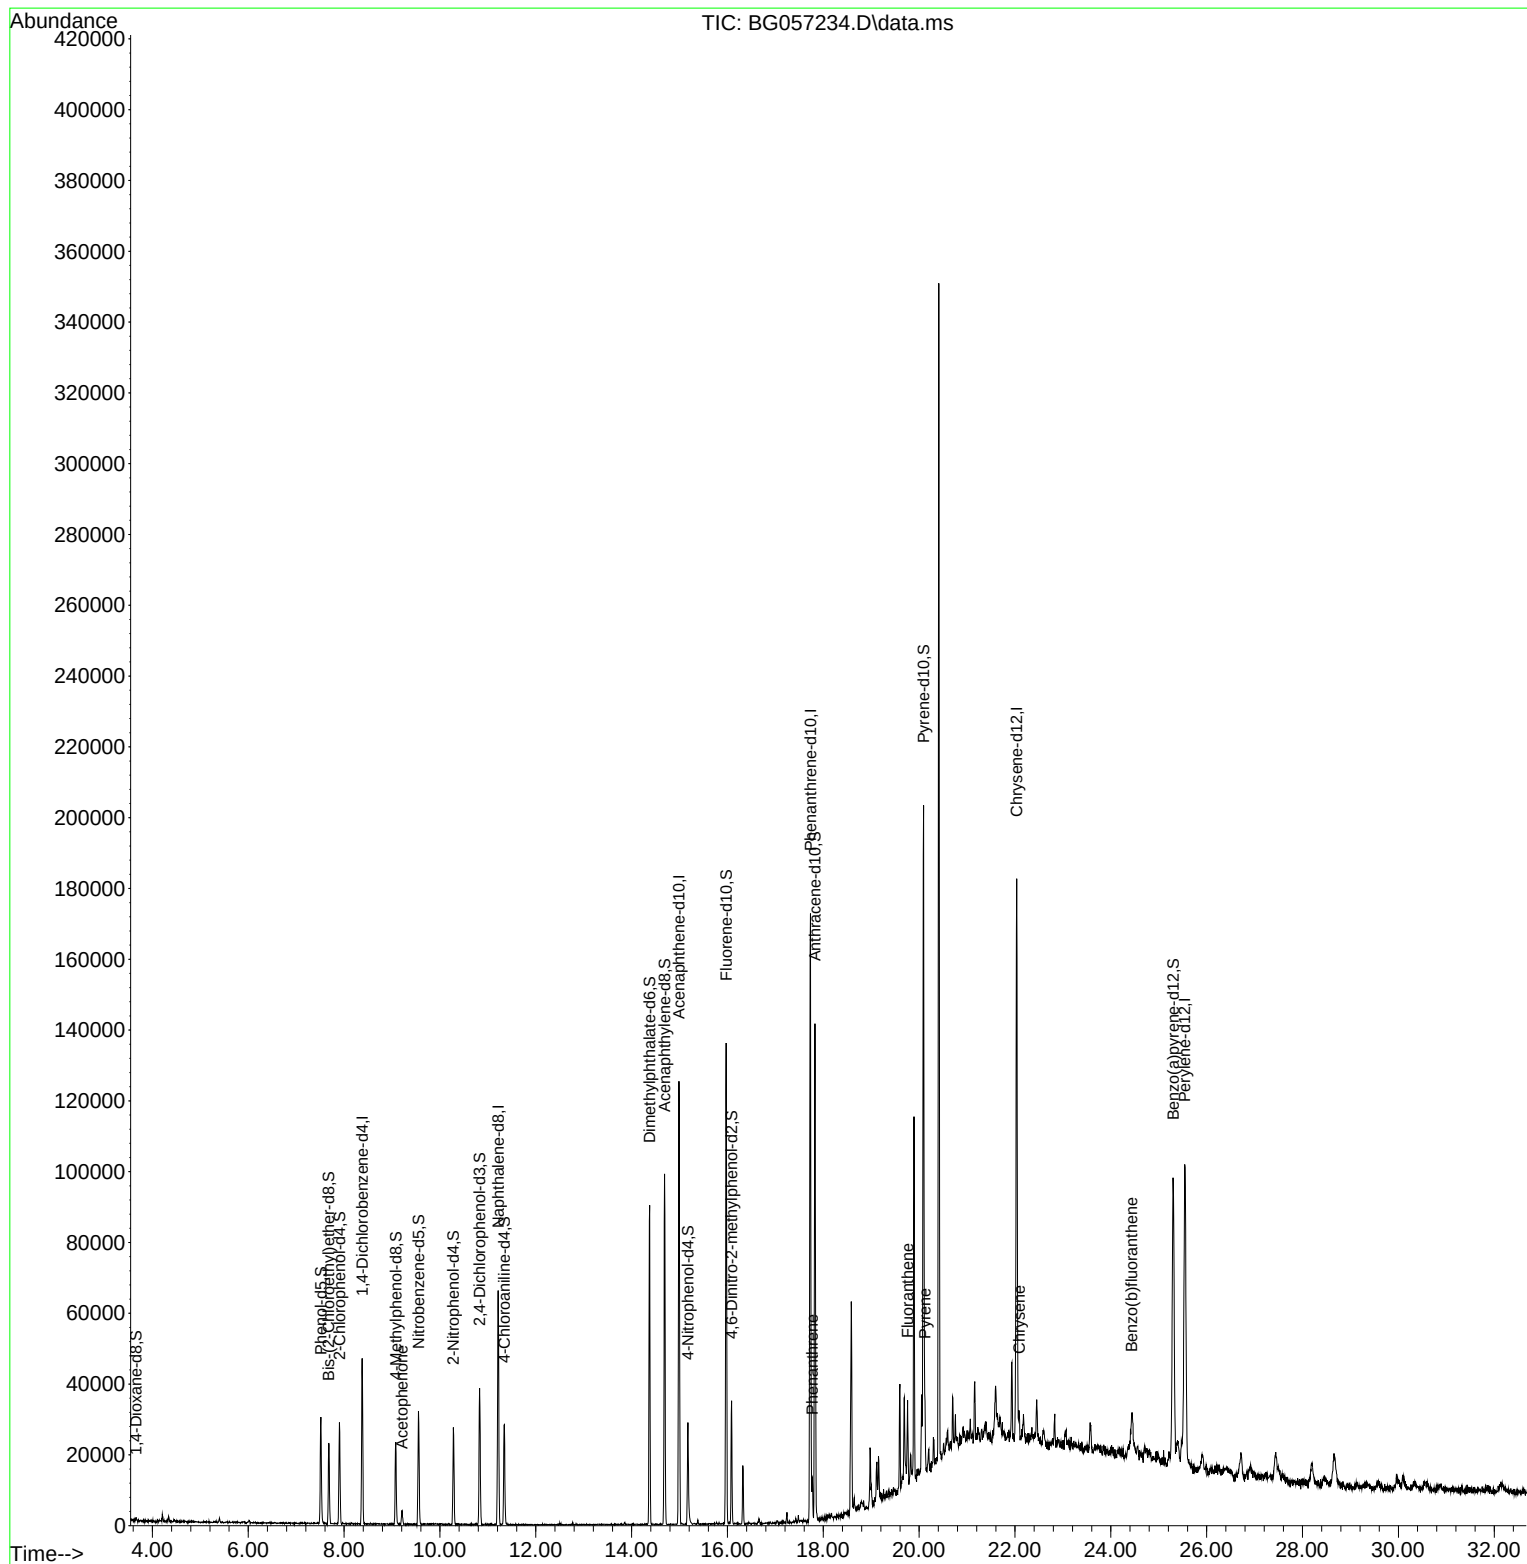

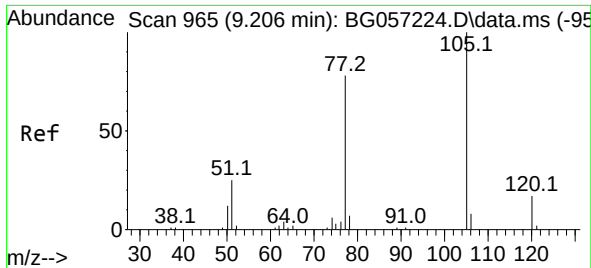

#16
Acetophenone
Concen: 1.514 ng/ul
RT: 9.206 min Scan# 965
Delta R.T. -0.000 min
Lab File: BG057234.D
Acq: 29 Apr 2023 2:22




Instrument :
BNA_G
ClientSampleId :
EW8X4

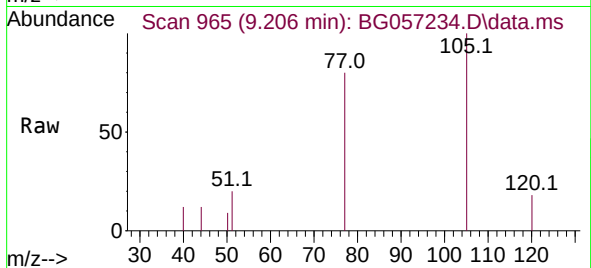

Tgt Ion:	105	Resp:	2495
Ion Ratio	Lower	Upper	
105	100		
77	79.8	70.6	105.8
51	20.5	24.5	36.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/01/2023
Supervised By :Jagrut Upadhyay 05/01/2023

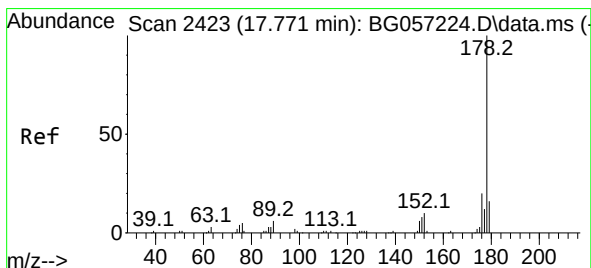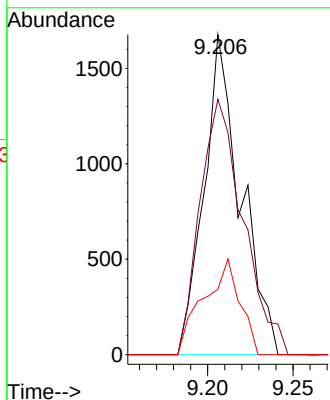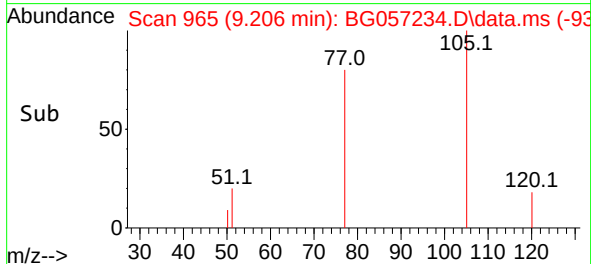

#72
Phenanthrene
Concen: 1.532 ng/ul
RT: 17.771 min Scan# 2423
Delta R.T. -0.000 min
Lab File: BG057234.D
Acq: 29 Apr 2023 2:22


Tgt Ion:	178	Resp:	9205
Ion Ratio	Lower	Upper	
178	100		
179	15.1	11.8	17.8
176	18.1	15.4	23.0

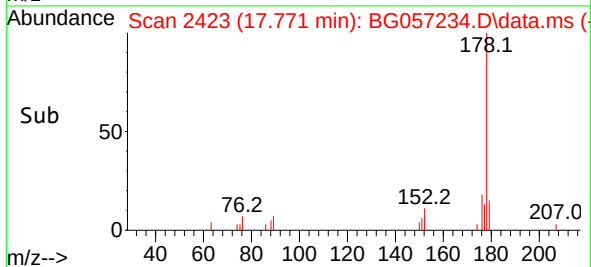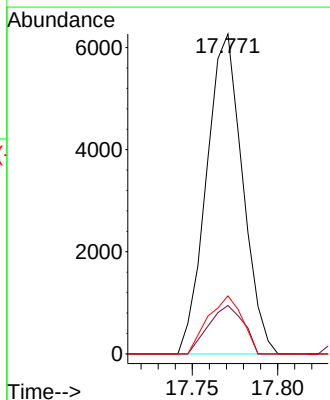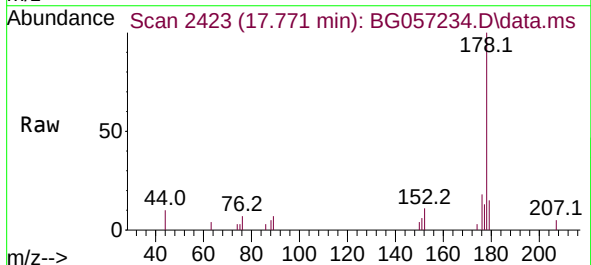

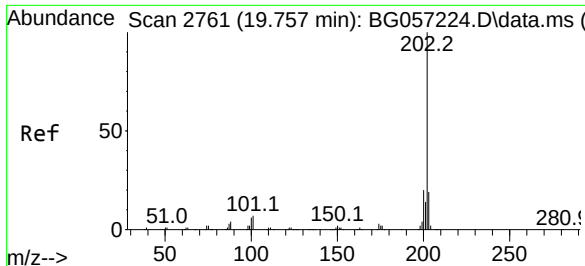

#80
Fluoranthene
Concen: 1.990 ng/u1
RT: 19.756 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG057234.D
Acq: 29 Apr 2023 2:22




Instrument :
BNA_G
ClientSampleId :
EW8X4

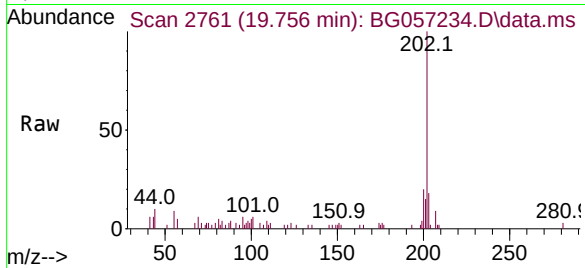

Tgt Ion:202 Resp: 13962
Ion Ratio Lower Upper
202 100
101 6.2 5.8 8.6
100 5.0 4.6 7.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/01/2023
Supervised By :Jagrut Upadhyay 05/01/2023

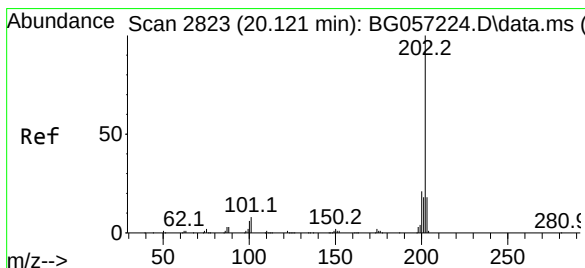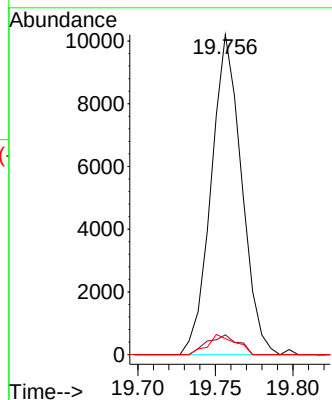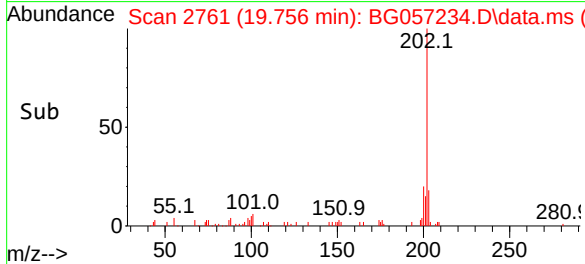

#82
Pyrene
Concen: 1.686 ng/u1
RT: 20.121 min Scan# 2823
Delta R.T. -0.000 min
Lab File: BG057234.D
Acq: 29 Apr 2023 2:22

Tgt Ion:202 Resp: 11975
Ion Ratio Lower Upper
202 100
101 7.4 5.7 8.5
100 7.4 6.0 9.0

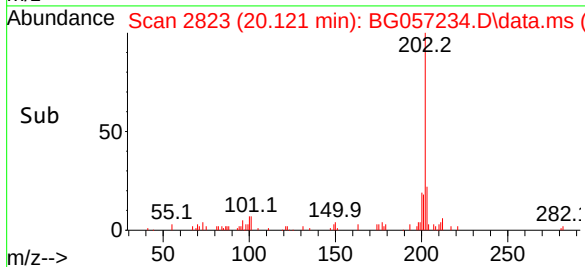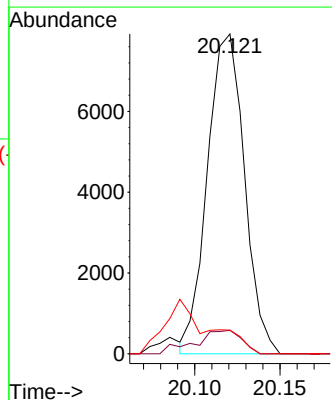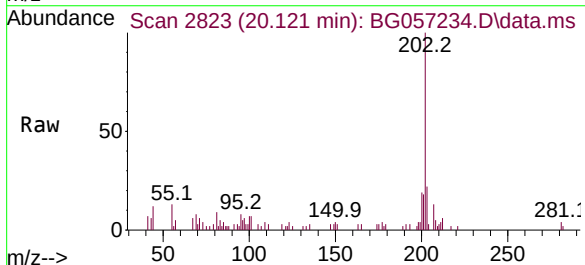

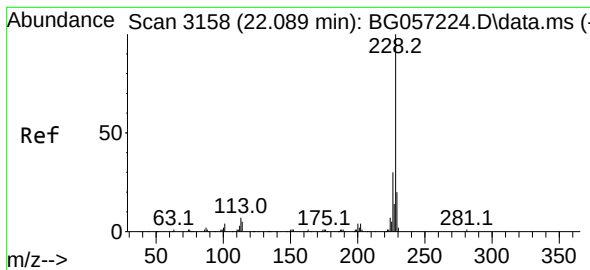

#87

Chrysene

Concen: 1.008 ng/ul m

RT: 22.089 min Scan# 3158

Delta R.T. -0.000 min

Lab File: BG057234.D

Acq: 29 Apr 2023 2:22

Instrument :

BNA_G

ClientSampleId :

EW8X4





Tgt Ion:228	Resp:	6691
Ion Ratio	Lower	Upper
228	100	
226	25.1	22.8 34.2
229	24.8	15.5 23.3

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 05/01/2023

Supervised By :Jagrut Upadhyay 05/01/2023

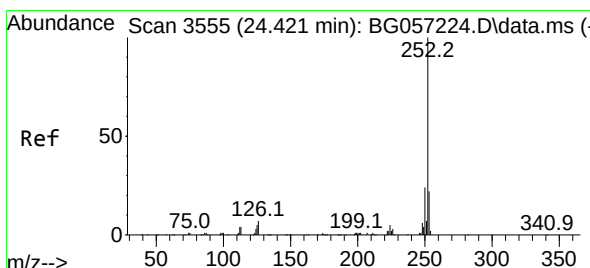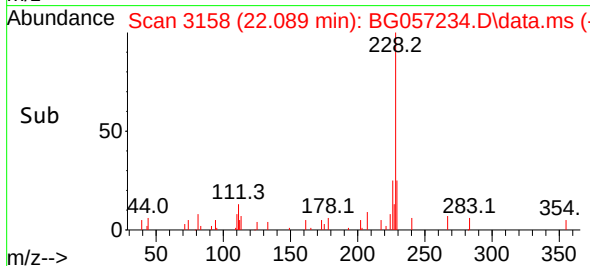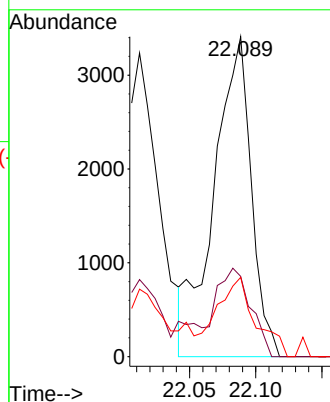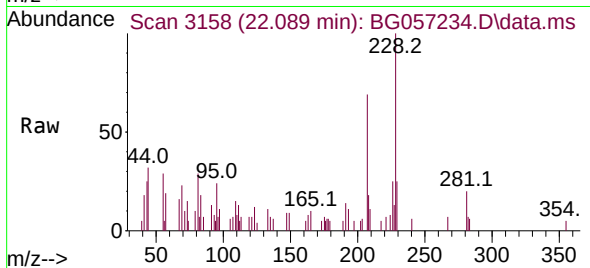

#90

Benzo(b)fluoranthene

Concen: 1.175 ng/ul m

RT: 24.432 min Scan# 3557

Delta R.T. 0.012 min

Lab File: BG057234.D

Acq: 29 Apr 2023 2:22

Tgt Ion:252	Resp:	8355
Ion Ratio	Lower	Upper
252	100	
253	15.8	16.7 25.1#
125	12.0	4.8 7.2#

