

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057219.D
 Acq On : 28 Apr 2023 15:24
 Operator : CG/JU
 Sample : PB152400BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.656	16	20	24	rBV3	3644	5026	0.86%	0.097%
2	3.797	41	44	48	rVB2	726	1102	0.19%	0.021%
3	4.049	84	87	90	rBV2	512	660	0.11%	0.013%
4	4.096	92	95	109	rVV	44410	71091	12.09%	1.365%
5	4.454	152	156	159	rVB3	650	767	0.13%	0.015%
6	4.825	216	219	223	rBV2	509	881	0.15%	0.017%
7	7.509	669	676	688	rBV	60835	109562	18.64%	2.104%
8	7.680	698	705	714	rVB	50598	81147	13.81%	1.558%
9	7.903	736	743	751	rBV2	60420	102549	17.45%	1.969%
10	8.379	817	824	834	rVB	48513	79388	13.51%	1.524%
11	8.514	843	847	848	rBV2	435	603	0.10%	0.012%
12	9.072	936	942	951	rVB2	79367	137401	23.38%	2.638%
13	9.553	1016	1024	1032	rVV	65520	117095	19.92%	2.248%
14	10.282	1140	1148	1155	rBV	57106	99516	16.93%	1.911%
15	10.435	1170	1174	1176	rBV2	402	618	0.11%	0.012%
16	10.828	1234	1241	1251	rVV	77929	137750	23.44%	2.645%
17	10.905	1251	1254	1258	rVB2	463	598	0.10%	0.011%
18	11.210	1299	1306	1318	rVB	70132	124461	21.17%	2.390%
19	11.339	1321	1328	1340	rVB	76596	139104	23.67%	2.671%
20	12.778	1568	1573	1577	rBV2	926	1521	0.26%	0.029%
21	13.853	1752	1756	1759	rVB2	1002	1041	0.18%	0.020%
22	14.376	1838	1845	1851	rBV	198187	288492	49.08%	5.540%
23	14.688	1891	1898	1907	rVB	198466	308435	52.47%	5.923%
24	14.987	1943	1949	1957	rBV	131625	205156	34.90%	3.939%
25	15.169	1974	1980	1999	rBV	64786	113805	19.36%	2.185%
26	15.974	2110	2117	2124	rVB	273581	408133	69.44%	7.837%
27	16.086	2131	2136	2145	rBV	84337	127474	21.69%	2.448%
28	16.215	2155	2158	2162	rVB2	590	899	0.15%	0.017%
29	17.725	2409	2415	2423	rVB	191245	289772	49.30%	5.564%
30	17.825	2425	2432	2439	rBV	322756	484771	82.48%	9.309%
31	18.853	2603	2607	2613	rBV2	549	777	0.13%	0.015%
32	19.399	2697	2700	2701	rBV	695	862	0.15%	0.017%
33	19.440	2705	2707	2709	rVB	1001	621	0.11%	0.012%
34	19.464	2709	2711	2714	rBV3	778	963	0.16%	0.018%
35	19.657	2740	2744	2748	rVV3	4396	5568	0.95%	0.107%
36	19.734	2753	2757	2762	rVB3	3777	5458	0.93%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057219.D
 Acq On : 28 Apr 2023 15:24
 Operator : CG/JU
 Sample : PB152400BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	19.775	2762	2764	2765	rBV	809	674	0.11%	0.013%
38	20.092	2812	2818	2825	rBV	405137	587778	100.00%	11.287%
39	20.351	2861	2862	2865	rBV3	1010	839	0.14%	0.016%
40	20.445	2877	2878	2880	rBV2	1010	790	0.13%	0.015%
41	20.580	2900	2901	2904	rBV3	1358	1094	0.19%	0.021%
42	20.662	2913	2915	2918	rBV4	943	974	0.17%	0.019%
43	20.691	2918	2920	2921	rBV	1130	676	0.12%	0.013%
44	20.744	2927	2929	2932	rBV4	1064	1108	0.19%	0.021%
45	20.909	2955	2957	2958	rBV	1257	708	0.12%	0.014%
46	20.926	2958	2960	2961	rBV2	1122	877	0.15%	0.017%
47	21.238	3012	3013	3014	rBV	2107	1116	0.19%	0.021%
48	21.954	3133	3135	3136	rBV2	1548	709	0.12%	0.014%
49	22.037	3142	3149	3158	rVB2	172293	304723	51.84%	5.851%
50	22.166	3169	3171	3172	rBV2	1531	1296	0.22%	0.025%
51	22.700	3260	3262	3264	rVB3	1504	792	0.13%	0.015%
52	22.812	3280	3281	3282	rBV	2022	1123	0.19%	0.022%
53	23.194	3345	3346	3347	rBV	1658	611	0.10%	0.012%
54	23.523	3400	3402	3403	rVB2	1649	918	0.16%	0.018%
55	23.570	3408	3410	3411	rVV2	1847	1005	0.17%	0.019%
56	24.451	3558	3560	3564	rVB5	3298	3521	0.60%	0.068%
57	24.615	3586	3588	3590	rBV2	1373	1051	0.18%	0.020%
58	24.803	3618	3620	3623	rVB3	1482	959	0.16%	0.018%
59	25.303	3694	3705	3718	rVB2	186525	519537	88.39%	9.976%
60	25.438	3726	3728	3729	rBV	1552	1251	0.21%	0.024%
61	25.473	3731	3734	3735	rVV3	4568	5699	0.97%	0.109%
62	25.544	3736	3746	3760	rVB2	97231	294488	50.10%	5.655%
63	25.931	3810	3812	3813	rBV2	2025	1483	0.25%	0.028%
64	25.967	3816	3818	3822	rBV3	1417	2515	0.43%	0.048%
65	26.924	3979	3981	3983	rBV2	1866	1176	0.20%	0.023%
66	27.811	4130	4132	4133	rBV2	1490	734	0.12%	0.014%
67	27.987	4160	4162	4165	rBV4	1593	1672	0.28%	0.032%
68	29.644	4442	4444	4445	rBV2	1594	1224	0.21%	0.024%
69	29.967	4497	4499	4500	rBV2	1841	1422	0.24%	0.027%
70	30.319	4557	4559	4564	rVB5	2623	2985	0.51%	0.057%
71	30.725	4626	4628	4629	rVB	2110	1126	0.19%	0.022%
72	30.842	4646	4648	4649	rBV	1647	935	0.16%	0.018%
73	30.925	4660	4662	4663	rBV2	1326	817	0.14%	0.016%
74	30.942	4663	4665	4666	rVB2	1720	957	0.16%	0.018%
75	31.024	4676	4679	4681	rBV2	1520	1930	0.33%	0.037%
76	32.317	4897	4899	4902	rBV4	1404	1349	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057219.D
Acq On : 28 Apr 2023 15:24
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 5207709

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057219.D
Acq On : 28 Apr 2023 15:24
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

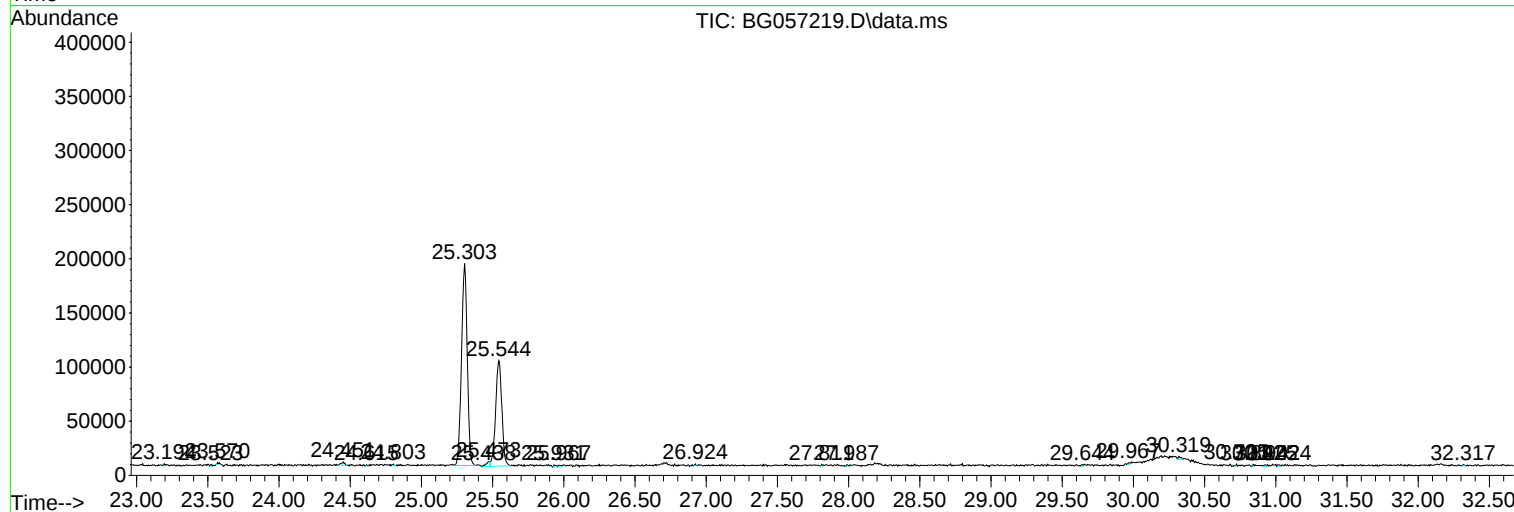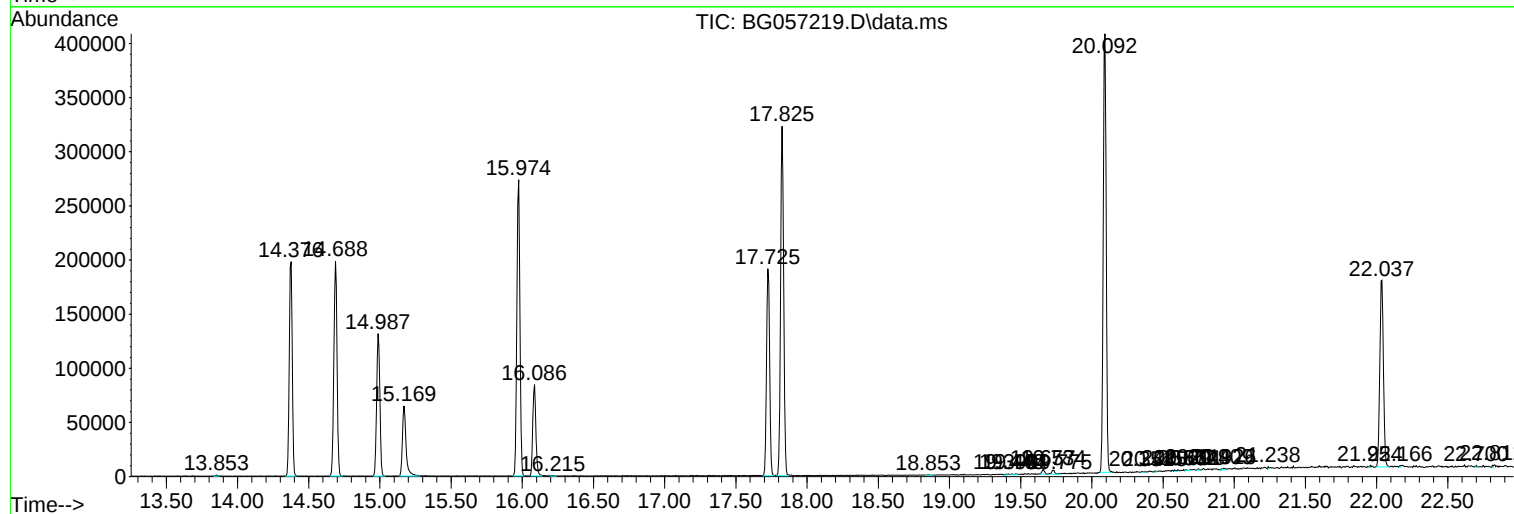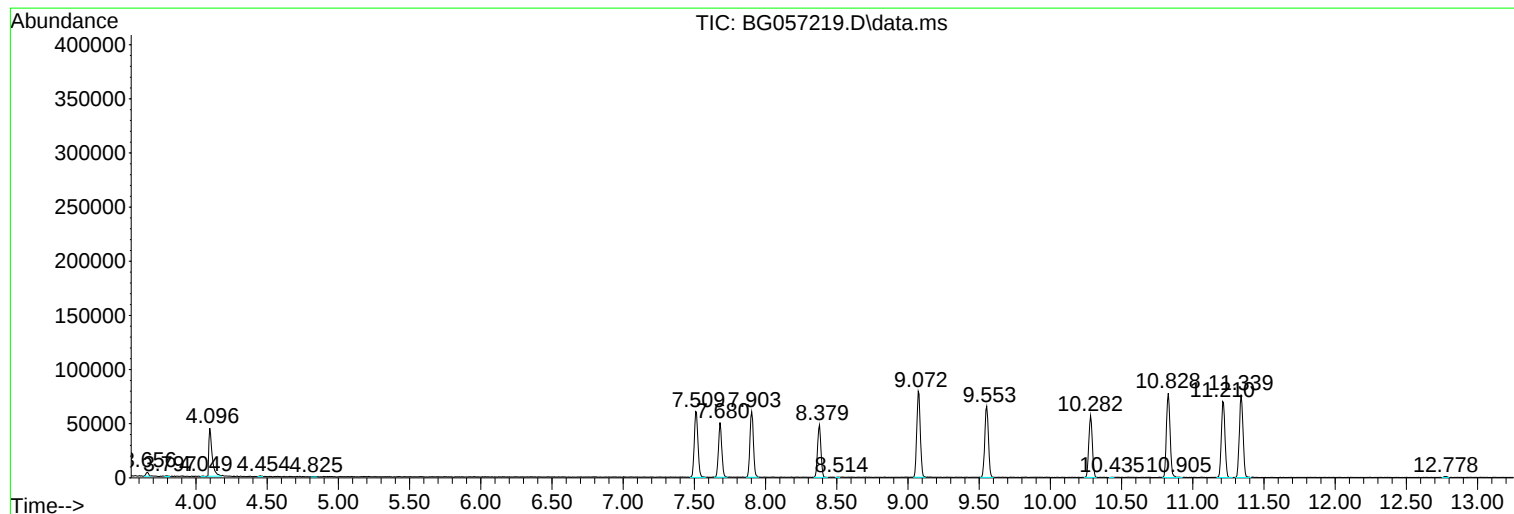

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057219.D
Acq On : 28 Apr 2023 15:24
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057219.D
Acq On : 28 Apr 2023 15:24
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------