

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057239.D
 Acq On : 29 Apr 2023 6:31
 Operator : CG/JU
 Sample : PB152400BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.655	17	20	28	rVV3	2930	4069	0.72%	0.077%
2	4.095	92	95	113	rBV	41846	71061	12.58%	1.353%
3	4.448	154	155	161	rBV3	692	943	0.17%	0.018%
4	4.771	206	210	213	rBV2	584	955	0.17%	0.018%
5	5.006	247	250	251	rBV2	672	656	0.12%	0.012%
6	5.129	270	271	276	rVB2	760	880	0.16%	0.017%
7	5.170	276	278	281	rBV2	674	897	0.16%	0.017%
8	7.514	670	677	686	rBV	65947	114408	20.26%	2.178%
9	7.685	699	706	713	rVB	47388	80670	14.28%	1.536%
10	7.732	713	714	720	rBV2	456	701	0.12%	0.013%
11	7.902	737	743	753	rVB	64347	108032	19.13%	2.056%
12	8.378	818	824	831	rBV	48007	77727	13.76%	1.480%
13	9.071	936	942	952	rVB	82023	144000	25.49%	2.741%
14	9.553	1017	1024	1031	rVB	69577	122550	21.70%	2.333%
15	10.281	1141	1148	1156	rBV	61122	107096	18.96%	2.039%
16	10.827	1234	1241	1249	rBV	88386	154456	27.35%	2.940%
17	11.215	1299	1307	1314	rVB	67947	119849	21.22%	2.281%
18	11.338	1321	1328	1337	rBV	81964	140992	24.96%	2.684%
19	12.766	1566	1571	1576	rBV3	1133	1740	0.31%	0.033%
20	13.853	1753	1756	1760	rVB2	749	902	0.16%	0.017%
21	14.376	1838	1845	1854	rBV	200874	283896	50.26%	5.404%
22	14.687	1891	1898	1907	rBV	211475	324546	57.46%	6.178%
23	14.986	1943	1949	1957	rVB	130631	200932	35.57%	3.825%
24	15.169	1974	1980	1998	rBV	67034	118856	21.04%	2.262%
25	15.973	2110	2117	2125	rBV	284824	420057	74.37%	7.996%
26	16.085	2130	2136	2149	rVB	83958	124076	21.97%	2.362%
27	16.208	2155	2157	2162	rVB2	631	788	0.14%	0.015%
28	17.724	2407	2415	2422	rBV	180763	274914	48.67%	5.233%
29	17.824	2426	2432	2441	rVB	323681	476977	84.45%	9.079%
30	18.347	2518	2521	2524	rBV	521	816	0.14%	0.016%
31	19.592	2731	2733	2736	rBV	722	849	0.15%	0.016%
32	19.657	2739	2744	2748	rBV4	3930	5970	1.06%	0.114%
33	19.727	2751	2756	2763	rBV3	3899	7066	1.25%	0.134%
34	19.915	2786	2788	2792	rBV2	845	1111	0.20%	0.021%
35	19.950	2792	2794	2796	rBV2	1006	947	0.17%	0.018%
36	20.091	2811	2818	2825	rBV	394773	564828	100.00%	10.751%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057239.D
 Acq On : 29 Apr 2023 6:31
 Operator : CG/JU
 Sample : PB152400BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	20.256	2844	2846	2849	rBV2	1162	1268	0.22%	0.024%
38	20.403	2870	2871	2873	rBV2	1068	704	0.12%	0.013%
39	20.790	2934	2937	2938	rBV2	1626	1151	0.20%	0.022%
40	20.855	2946	2948	2951	rBV3	1089	968	0.17%	0.018%

41	20.996	2970	2972	2973	rBV2	1233	879	0.16%	0.017%
42	21.061	2980	2983	2984	rBV2	1246	1152	0.20%	0.022%
43	21.225	3009	3011	3013	rBV3	1112	1354	0.24%	0.026%
44	21.348	3029	3032	3033	rBV3	1436	1301	0.23%	0.025%
45	21.425	3043	3045	3046	rVB	1566	682	0.12%	0.013%

46	21.448	3046	3049	3051	rBV3	1583	1734	0.31%	0.033%
47	21.566	3067	3069	3070	rBV	1163	828	0.15%	0.016%
48	21.660	3081	3085	3087	rBV4	1422	2230	0.39%	0.042%
49	21.701	3090	3092	3095	rBV3	1498	1164	0.21%	0.022%
50	21.724	3095	3096	3100	rBV3	1549	1182	0.21%	0.022%

51	22.036	3142	3149	3156	rVB2	172117	288690	51.11%	5.495%
52	22.376	3205	3207	3208	rBV2	1195	862	0.15%	0.016%
53	22.482	3223	3225	3228	rBV4	1397	1731	0.31%	0.033%
54	22.823	3280	3283	3285	rVB4	2010	1785	0.32%	0.034%
55	23.234	3351	3353	3354	rBV2	1277	839	0.15%	0.016%

56	23.252	3354	3356	3358	rVV2	1229	975	0.17%	0.019%
57	23.375	3375	3377	3381	rVB5	1534	1555	0.28%	0.030%
58	23.569	3407	3410	3416	rVB6	3687	5565	0.99%	0.106%
59	24.057	3491	3493	3494	rBV2	1268	865	0.15%	0.016%
60	24.139	3505	3507	3512	rBV4	1469	2714	0.48%	0.052%

61	24.415	3552	3554	3555	rBV2	2030	1634	0.29%	0.031%
62	24.438	3555	3558	3565	rVB8	4408	9974	1.77%	0.190%
63	24.526	3569	3573	3574	rBV3	1217	1186	0.21%	0.023%
64	24.562	3577	3579	3581	rVB3	1280	953	0.17%	0.018%
65	24.844	3624	3627	3628	rBV3	1474	1501	0.27%	0.029%

66	24.891	3633	3635	3637	rBV2	1175	848	0.15%	0.016%
67	25.302	3692	3705	3717	rBV	182097	518165	91.74%	9.863%
68	25.472	3727	3734	3735	rBV5	5191	9452	1.67%	0.180%
69	25.543	3736	3746	3757	rVB3	88689	275671	48.81%	5.247%
70	25.625	3758	3760	3764	rVB5	1740	1709	0.30%	0.033%

71	26.071	3834	3836	3837	rBV2	1199	821	0.15%	0.016%
72	26.700	3941	3943	3951	rVB6	3760	6970	1.23%	0.133%
73	26.882	3972	3974	3976	rBV3	1120	795	0.14%	0.015%
74	27.816	4131	4133	4136	rVB4	1428	1149	0.20%	0.022%
75	27.846	4136	4138	4140	rBV2	1609	1477	0.26%	0.028%

76	27.963	4156	4158	4160	rVB3	1341	1164	0.21%	0.022%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
 Data File : BG057239.D
 Acq On : 29 Apr 2023 6:31
 Operator : CG/JU
 Sample : PB152400BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	28.186	4189	4196	4199	rBV6	3867	9552	1.69%	0.182%
78	28.791	4297	4299	4300	rBV2	1029	785	0.14%	0.015%
79	28.809	4300	4302	4303	rVV2	1218	718	0.13%	0.014%
80	28.950	4324	4326	4329	rVB4	1398	1205	0.21%	0.023%
81	28.973	4329	4330	4332	rBV2	1532	1242	0.22%	0.024%
82	29.132	4355	4357	4359	rBV2	1176	980	0.17%	0.019%
83	29.338	4391	4392	4394	rBV2	2198	1139	0.20%	0.022%
84	29.479	4414	4416	4418	rBV3	1270	1019	0.18%	0.019%
85	29.790	4467	4469	4471	rBV2	1059	851	0.15%	0.016%
86	29.890	4484	4486	4487	rBV2	1861	1082	0.19%	0.021%
87	29.966	4498	4499	4506	rBV6	1794	2380	0.42%	0.045%
88	30.683	4618	4621	4624	rBV5	2340	3363	0.60%	0.064%
89	31.253	4715	4718	4720	rBV3	1723	1894	0.34%	0.036%
90	31.464	4752	4754	4755	rBV2	1062	694	0.12%	0.013%
91	31.511	4760	4762	4766	rVB5	1450	1821	0.32%	0.035%
92	31.552	4766	4769	4771	rBV4	1399	1285	0.23%	0.024%
93	31.793	4808	4810	4812	rBV2	1146	1048	0.19%	0.020%
94	31.834	4816	4817	4820	rVB2	1702	1047	0.19%	0.020%
95	31.858	4820	4821	4825	rBV4	1799	1374	0.24%	0.026%
96	31.958	4836	4838	4841	rBV4	1346	1237	0.22%	0.024%
97	32.034	4849	4851	4852	rBV	1150	761	0.13%	0.014%
98	32.263	4888	4890	4891	rVB2	1357	698	0.12%	0.013%
99	32.281	4891	4893	4897	rBV4	1343	1678	0.30%	0.032%
100	32.381	4908	4910	4911	rBV2	1230	866	0.15%	0.016%




Sum of corrected areas: 5253579

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057239.D
Acq On : 29 Apr 2023 6:31
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

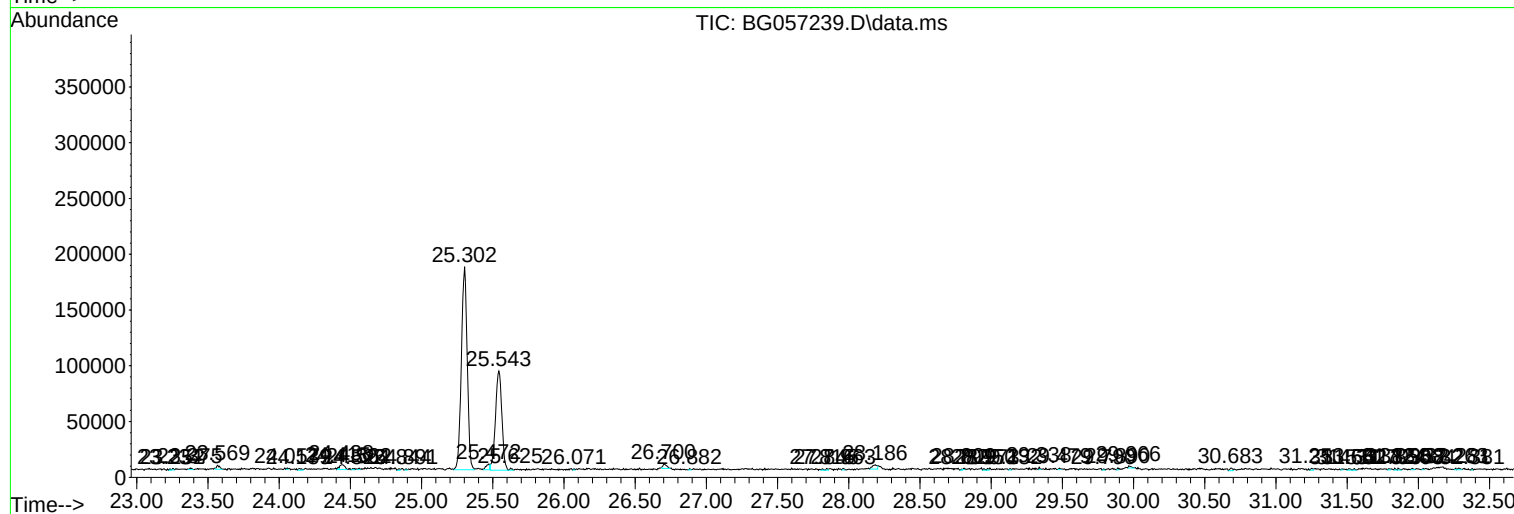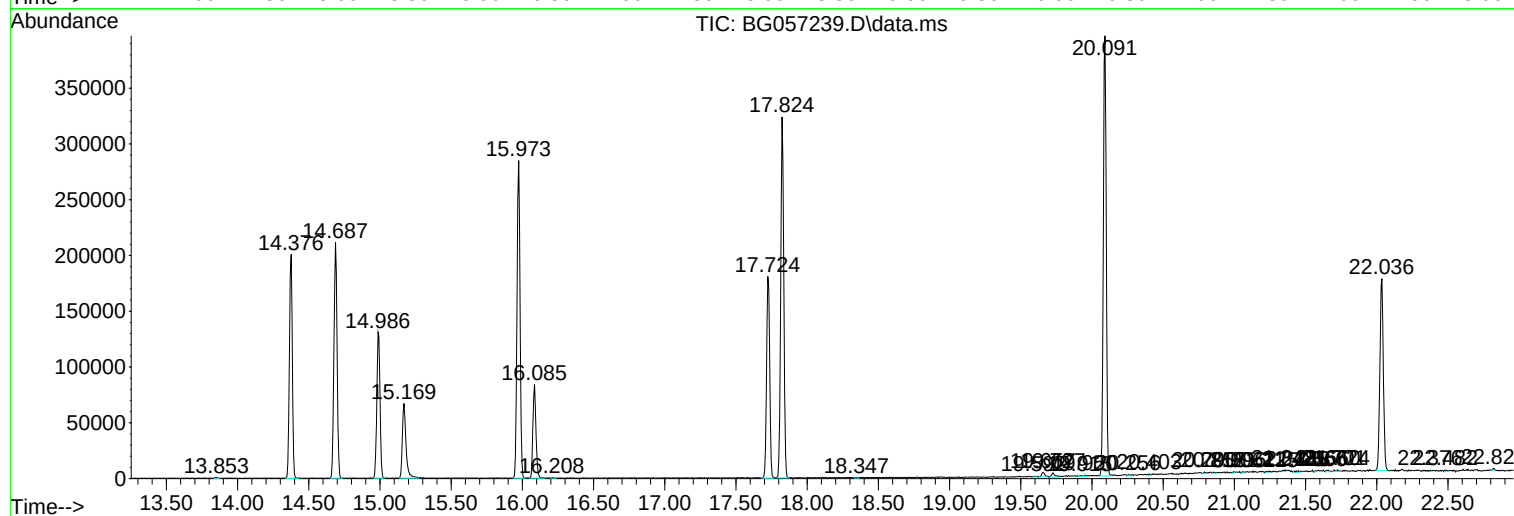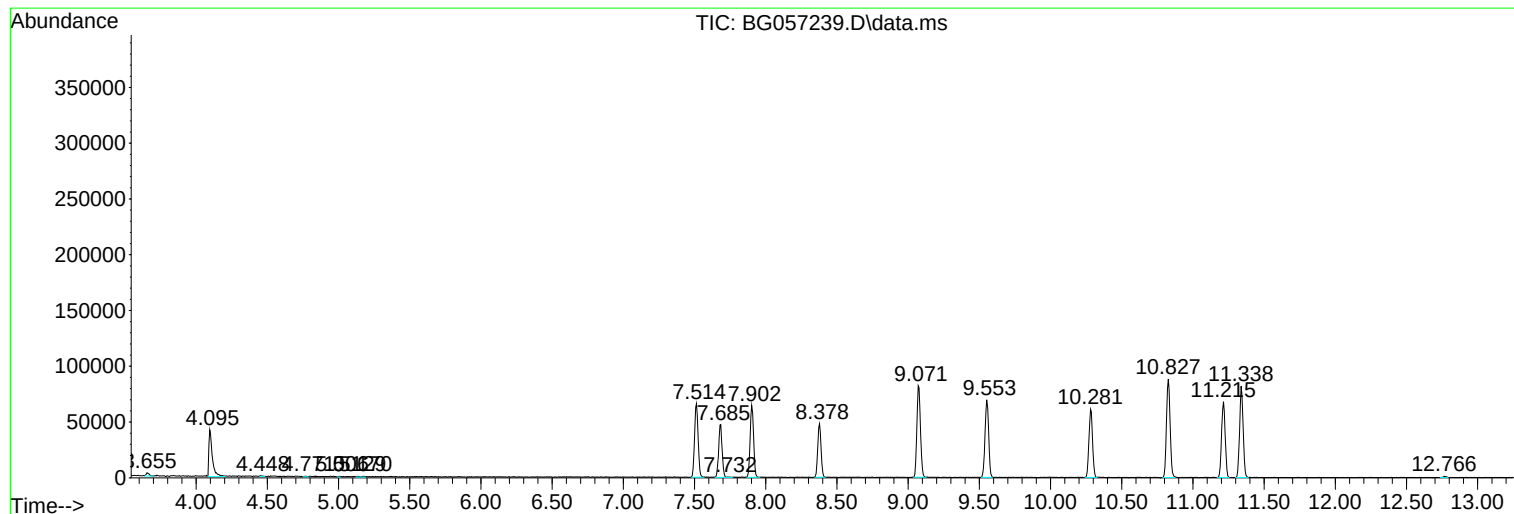

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057239.D
Acq On : 29 Apr 2023 6:31
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042823\
Data File : BG057239.D
Acq On : 29 Apr 2023 6:31
Operator : CG/JU
Sample : PB152400BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc