


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042915\
 Data File : BG016811.D
 Acq On : 29 Apr 2015 23:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 02:01:08 2015

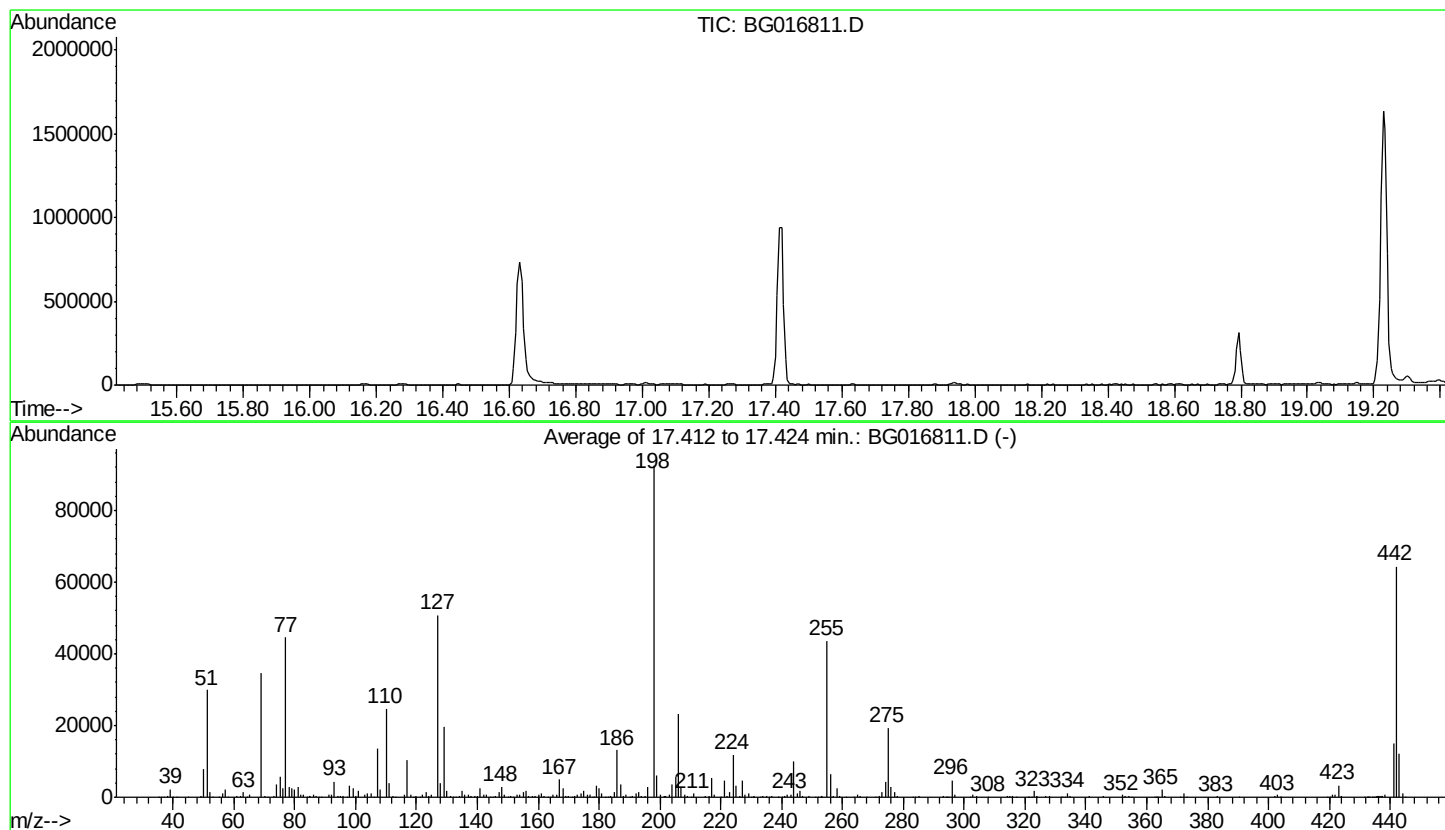

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	29895	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.4	34602	PASS
70	69	0.00	2	0.6	214	PASS
127	198	10	80	54.8	50712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92477	PASS
199	198	5	9	6.8	6248	PASS
275	198	10	60	21.1	19467	PASS
365	198	1	100	2.3	2129	PASS
441	442	0.01	24	23.4	15081	PASS
442	198	50	100	69.7	64445	PASS
443	442	15	24	18.7	12064	PASS