
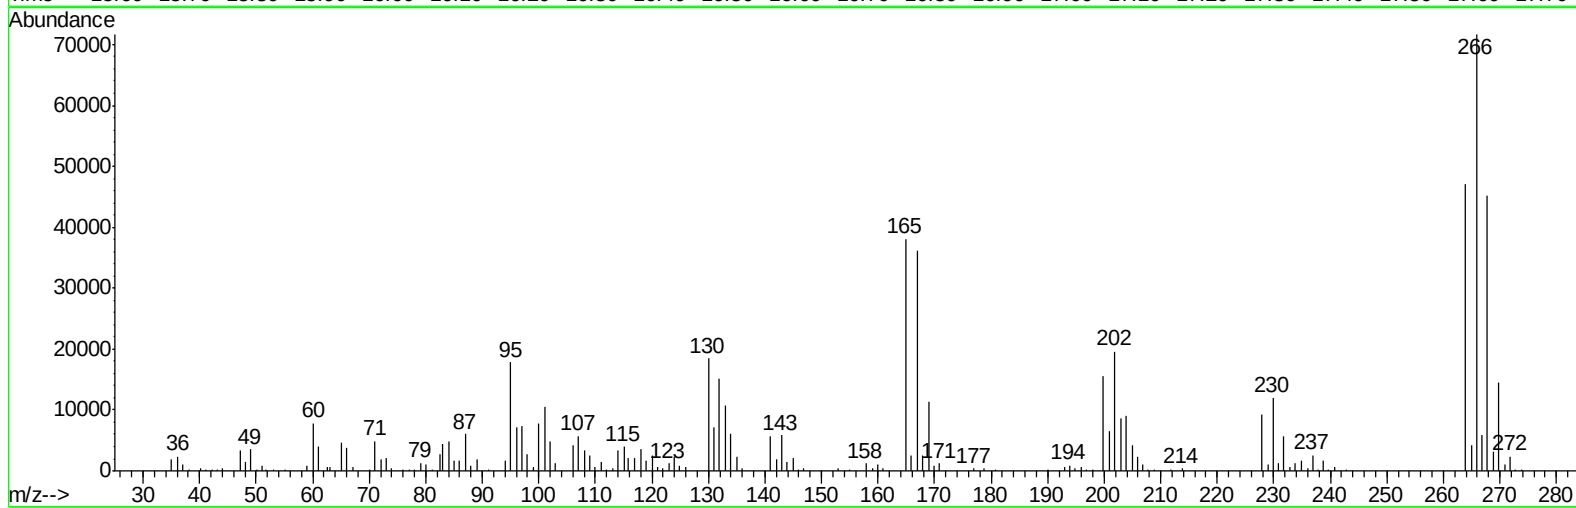


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042915\
Data File : BG016792.D
Acq On : 29 Apr 2015 11:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:39:26 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 02:30:36 2015
Response via : Initial Calibration

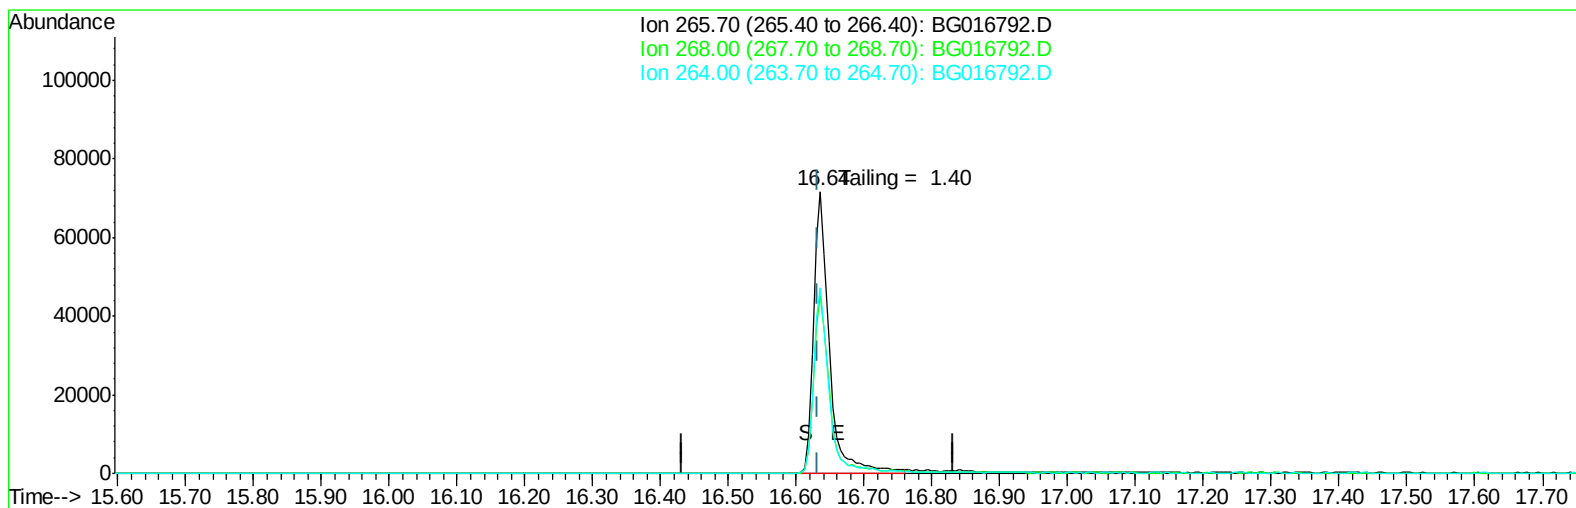

TIC: BG016792.D

(69) Pentachlorophenol (C)



16.636min (+0.003) 1994.15ng

response 114138

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.99
264.00	61.40	65.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042915\
Data File : BG016792.D
Acq On : 29 Apr 2015 11:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:39:26 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 02:30:36 2015
Response via : Initial Calibration

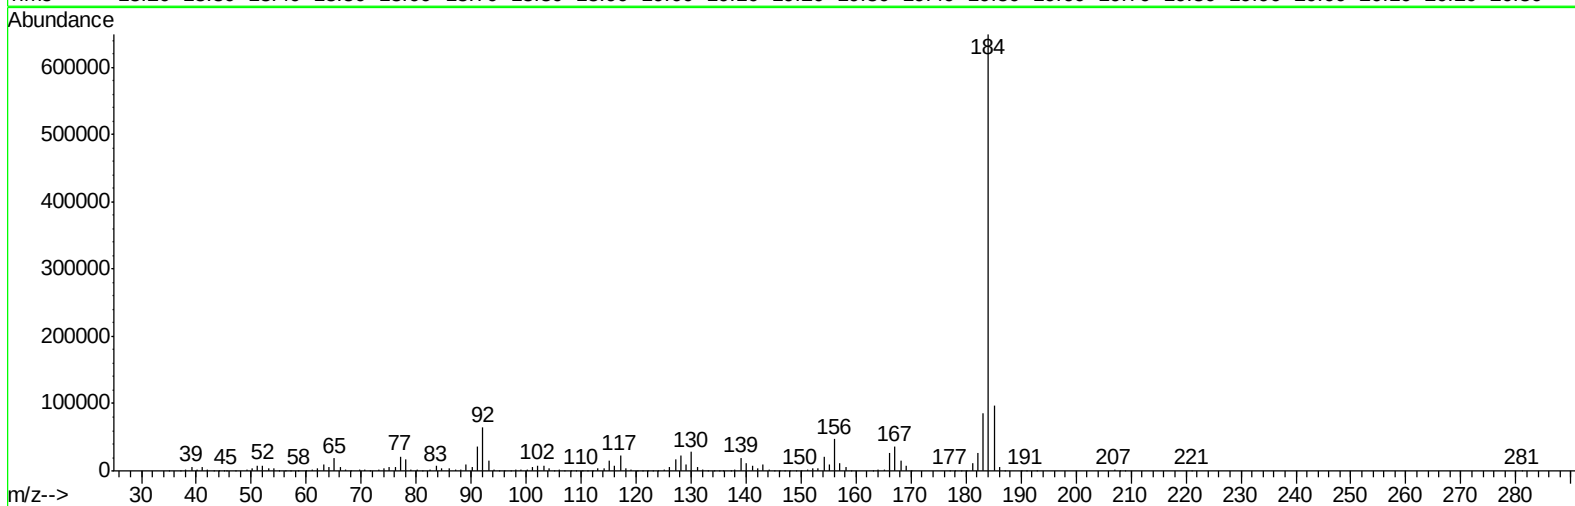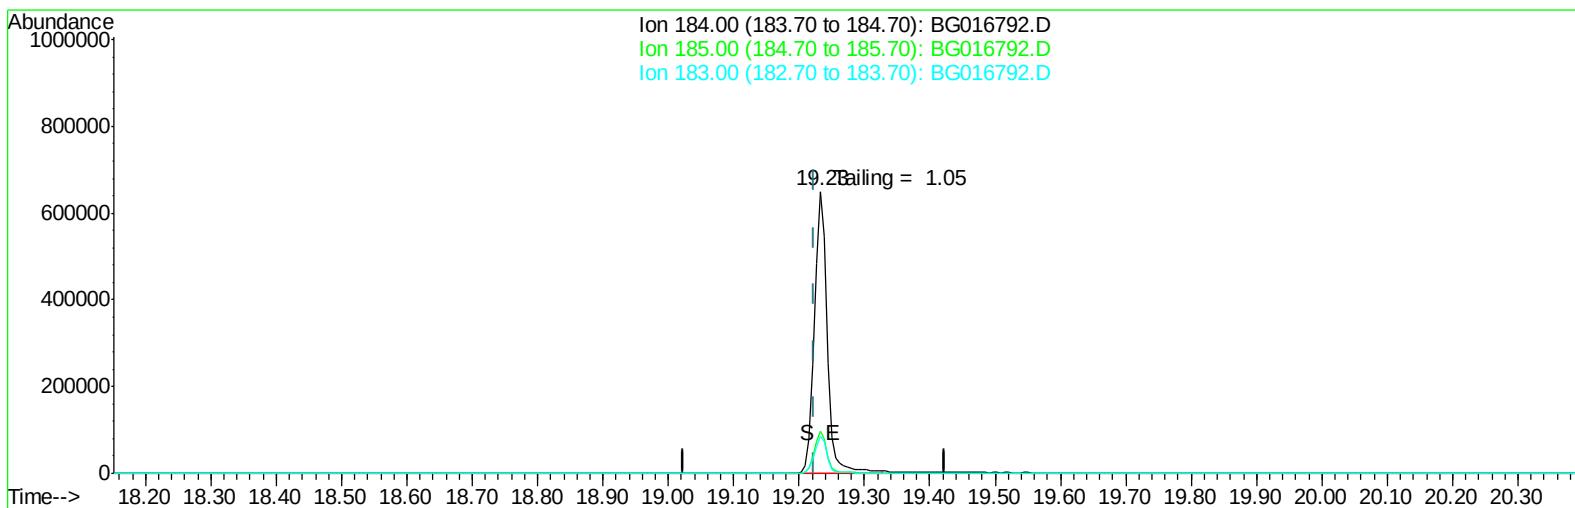

TIC: BG016792.D

(76) Benzidine

19.233min (+0.009) 13166.98ng

response 903916

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	14.88
183.00	13.10	13.18
0.00	0.00	0.00