
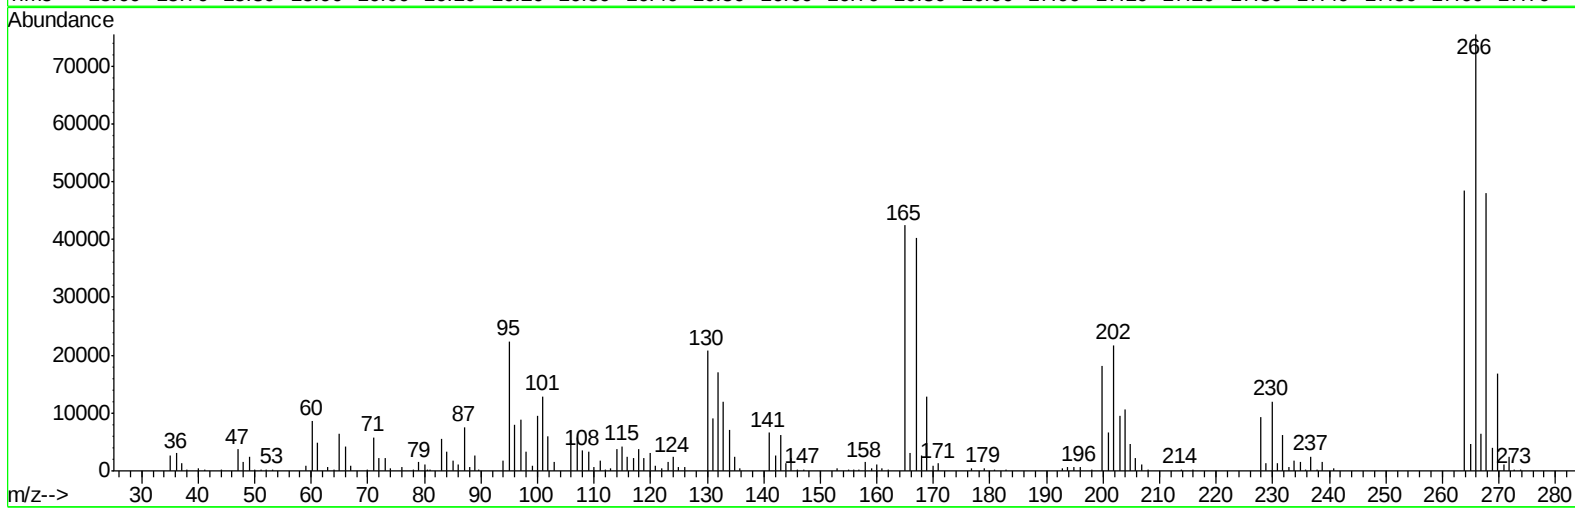


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042915\
Data File : BG016811.D
Acq On : 29 Apr 2015 23:43
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:40:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 02:30:36 2015
Response via : Initial Calibration

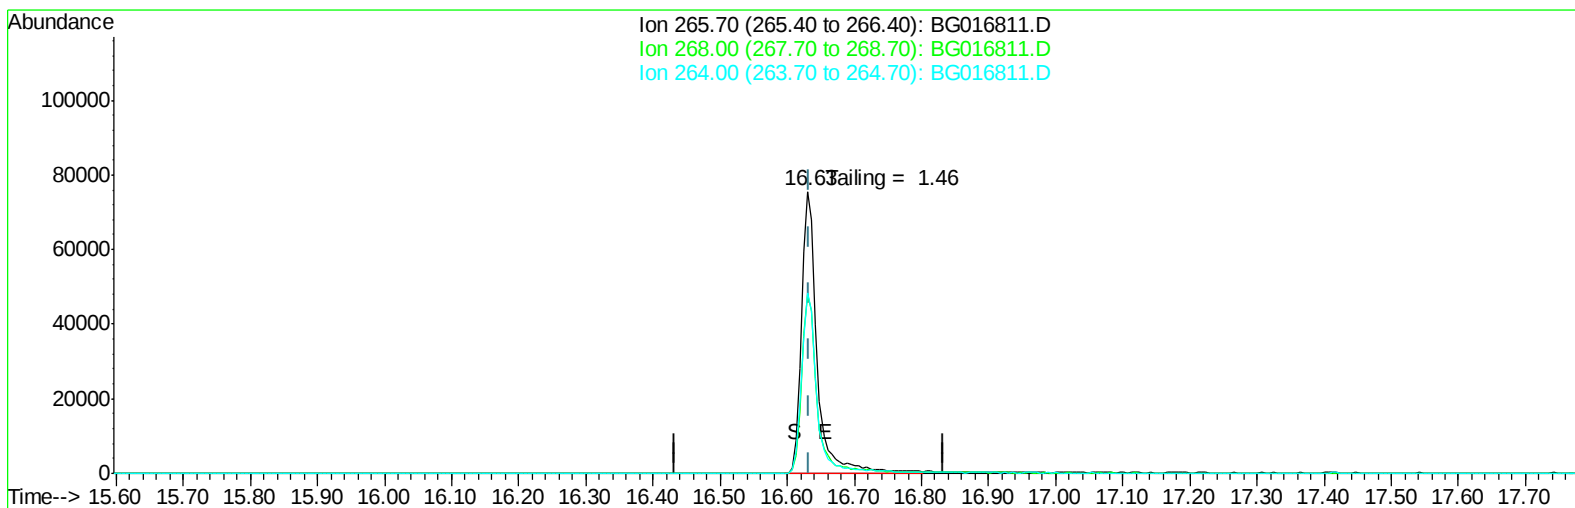

TIC: BG016811.D

(69) Pentachlorophenol (C)



16.631min (-0.002) 1991.90ng

response 123987

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.55
264.00	61.40	64.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042915\
Data File : BG016811.D
Acq On : 29 Apr 2015 23:43
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:40:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 02:30:36 2015
Response via : Initial Calibration

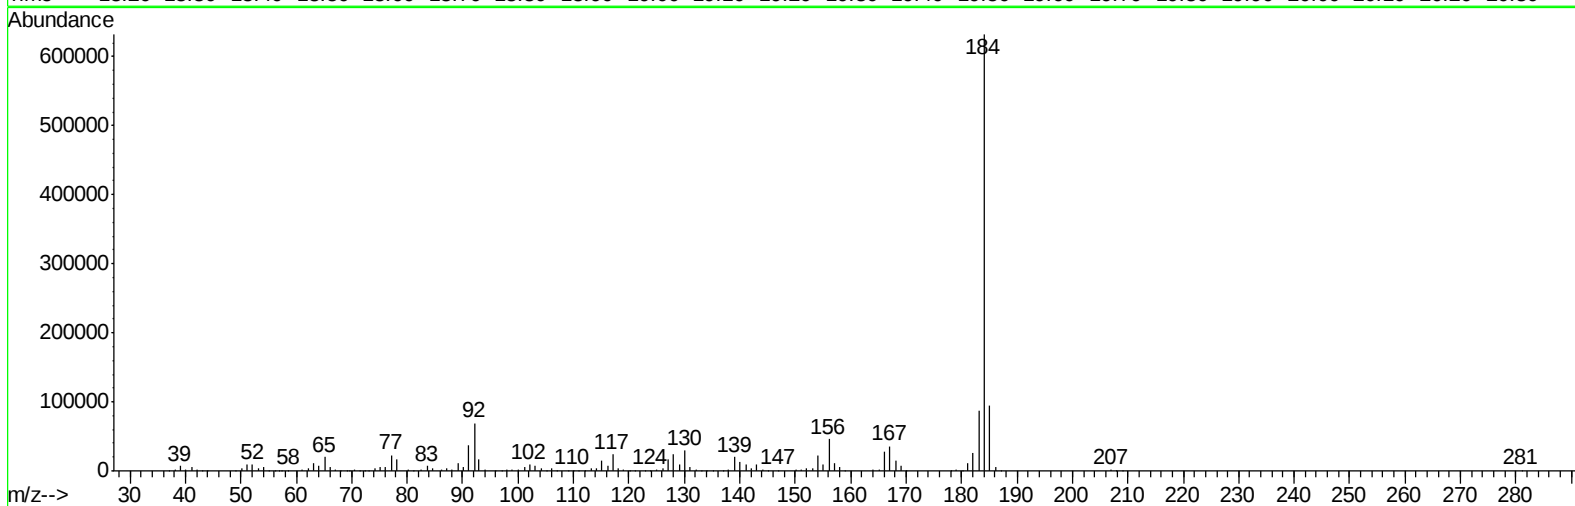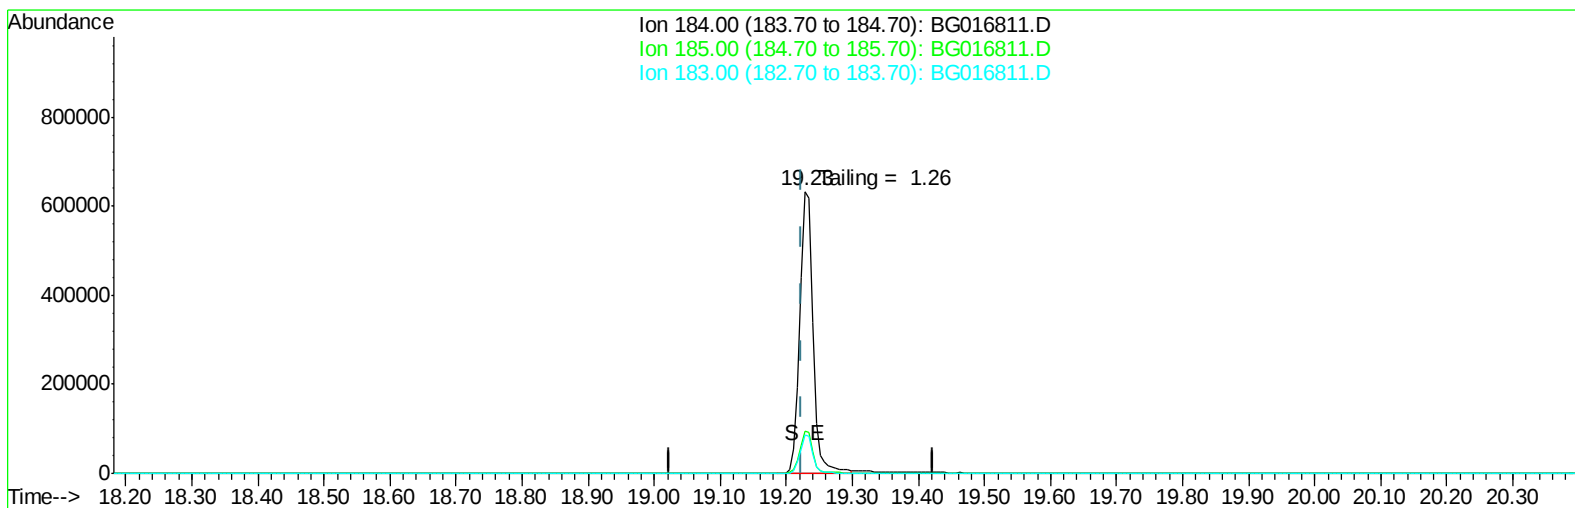

TIC: BG016811.D

(76) Benzidine

19.228min (+0.004) 7286.93ng

response 917824

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	15.11
183.00	13.10	13.70
0.00	0.00	0.00