
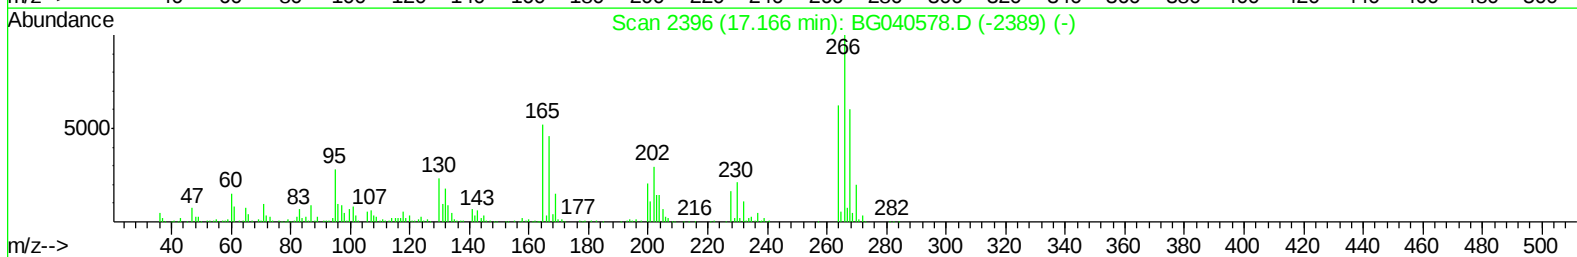
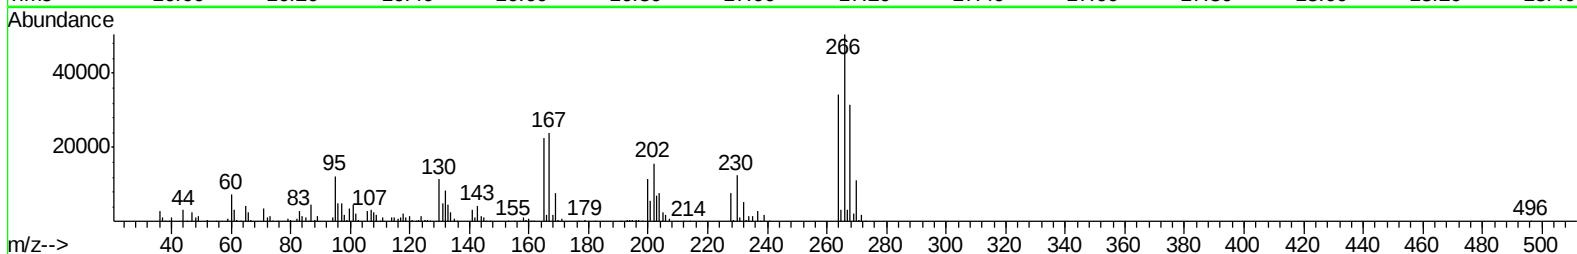


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042919\
Data File : BG040654.D
Acq On : 29 Apr 2019 10:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:36:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

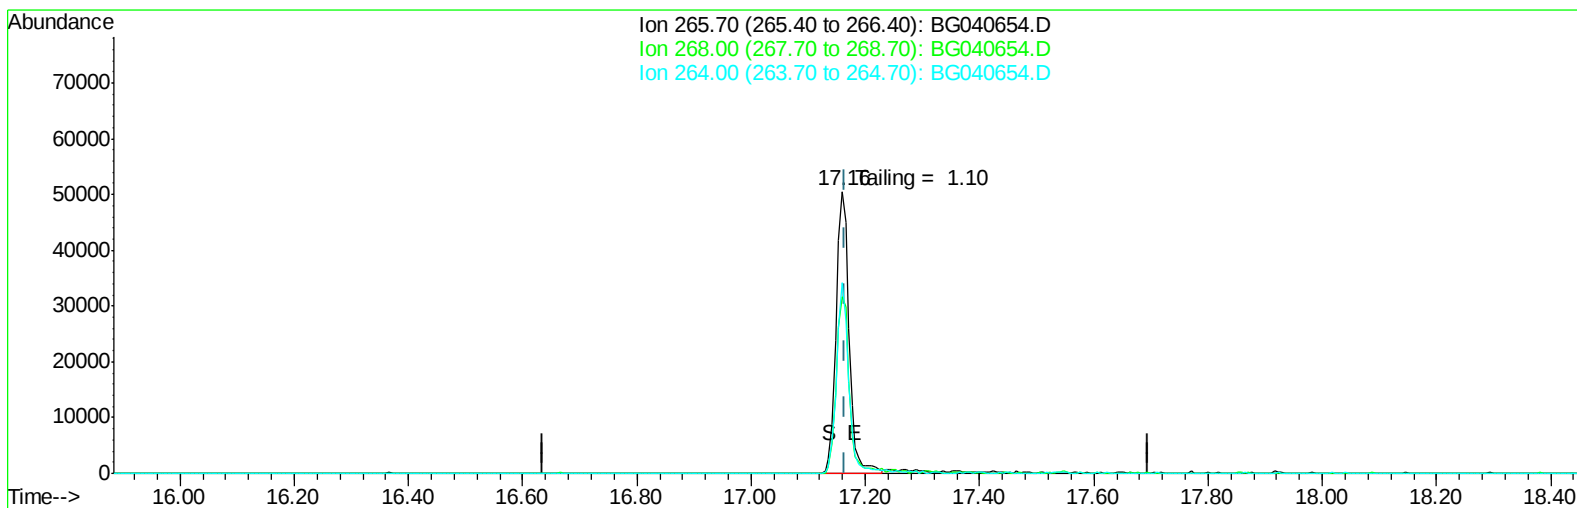

TIC: BG040654.D

(70) Pentachlorophenol (C)




17.159min (-0.007) 173444.73ng

response 79756

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	62.56
264.00	62.50	67.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042919\
Data File : BG040654.D
Acq On : 29 Apr 2019 10:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:36:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

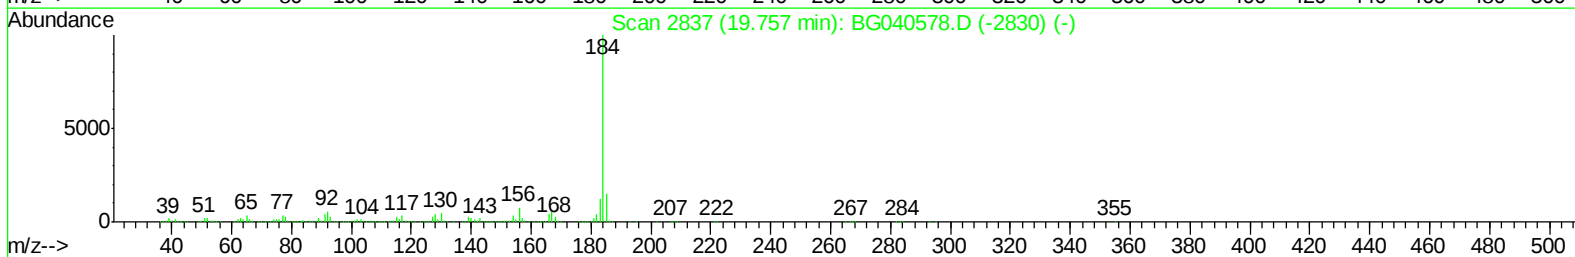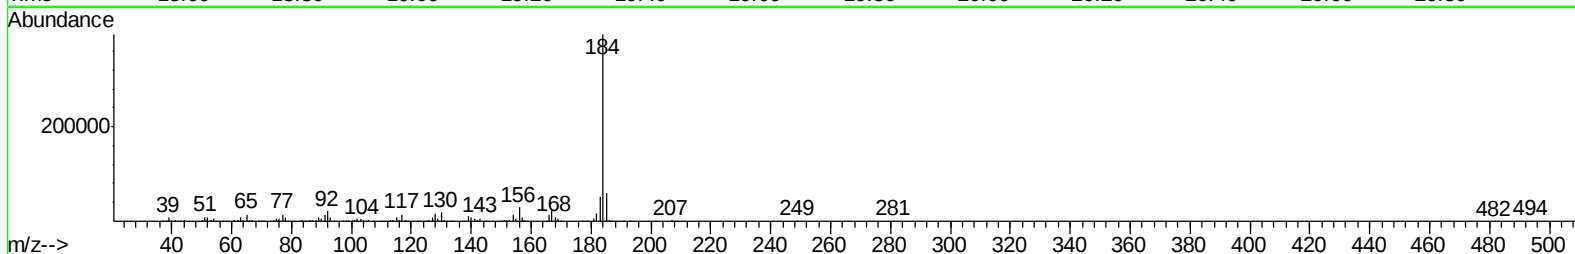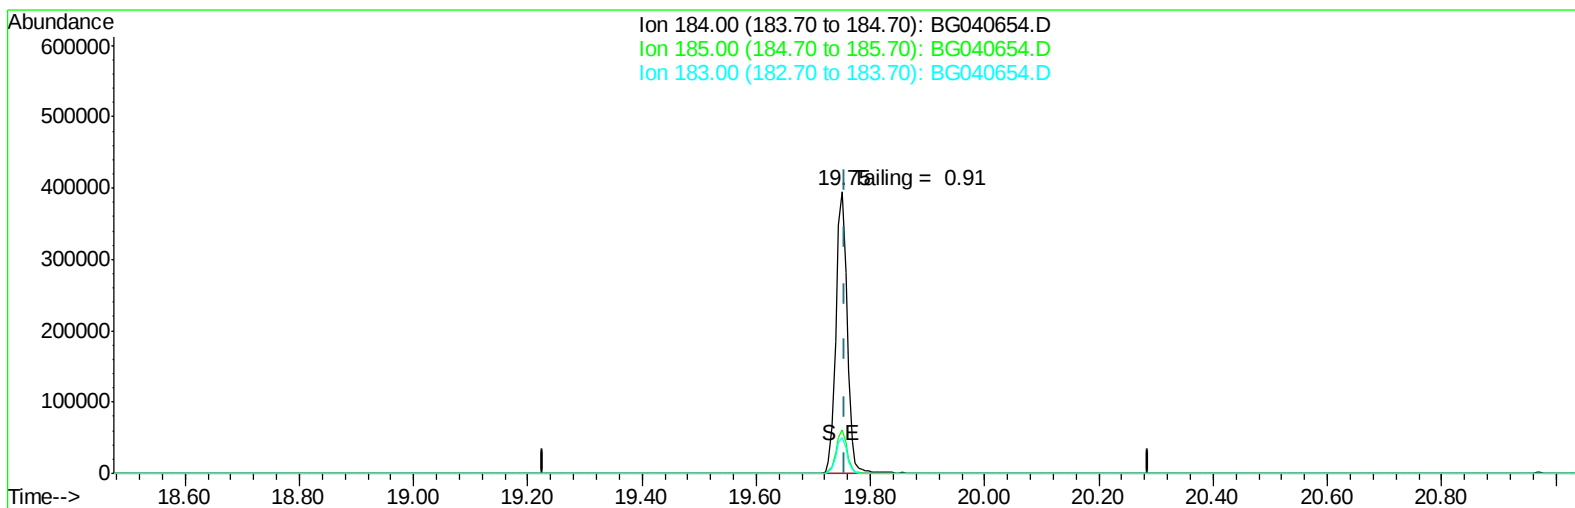

TIC: BG040654.D

(77) Benzidine

19.750min (-0.007) 0.00ng

response 540124

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.37
183.00	12.70	12.75
0.00	0.00	0.00