


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042919\
 Data File : BG040654.D
 Acq On : 29 Apr 2019 10:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

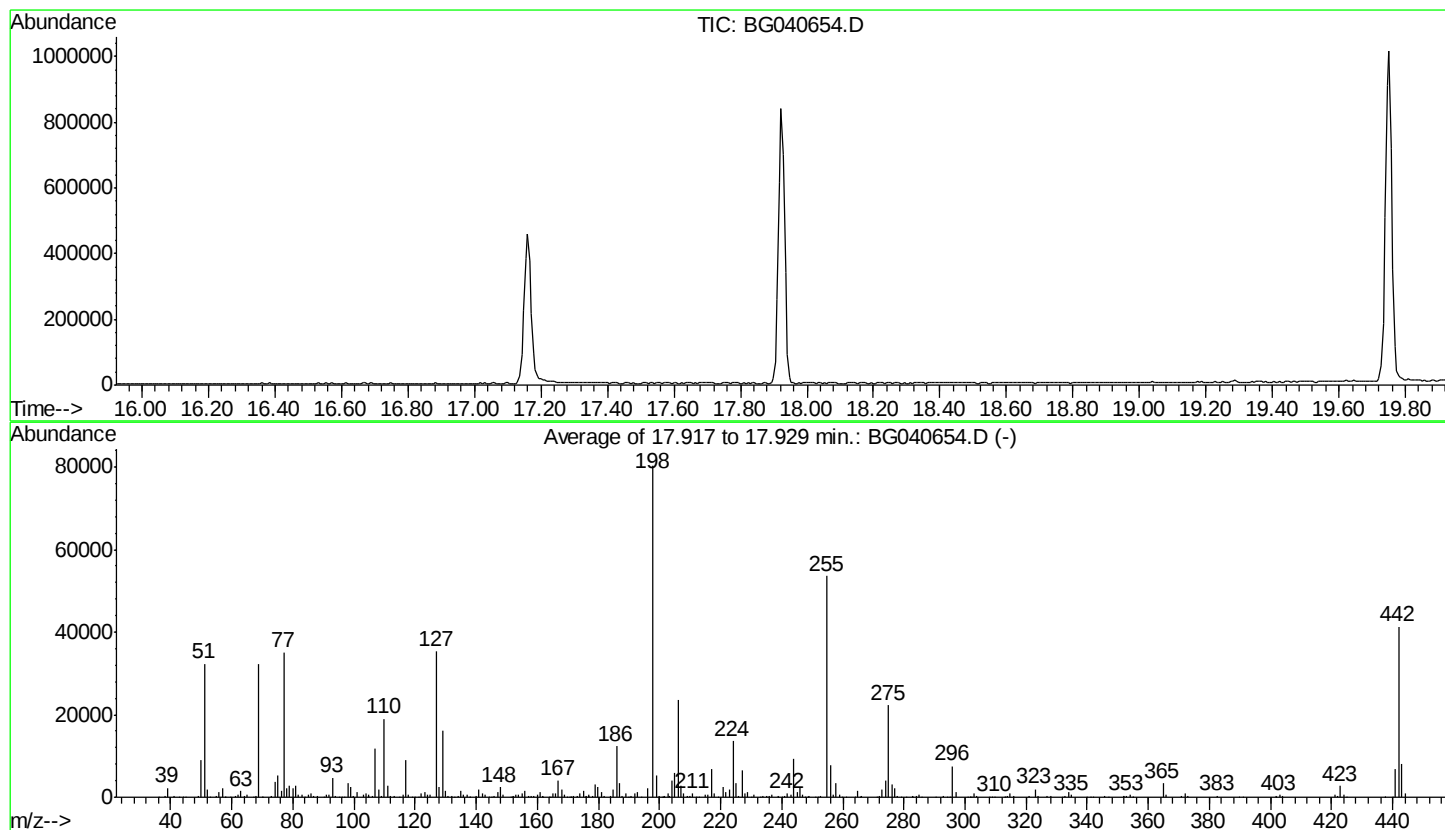

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	32368	PASS
68	69	0.00	2	0.7	226	PASS
69	198	0.00	100	40.3	32397	PASS
70	69	0.00	2	0.3	99	PASS
127	198	10	80	43.8	35221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80346	PASS
199	198	5	9	6.5	5215	PASS
275	198	10	60	27.8	22330	PASS
365	198	1	100	4.2	3364	PASS
441	198	0.01	100	8.4	6724	PASS
442	198	50	100	51.4	41261	PASS
443	442	15	24	19.6	8095	PASS