
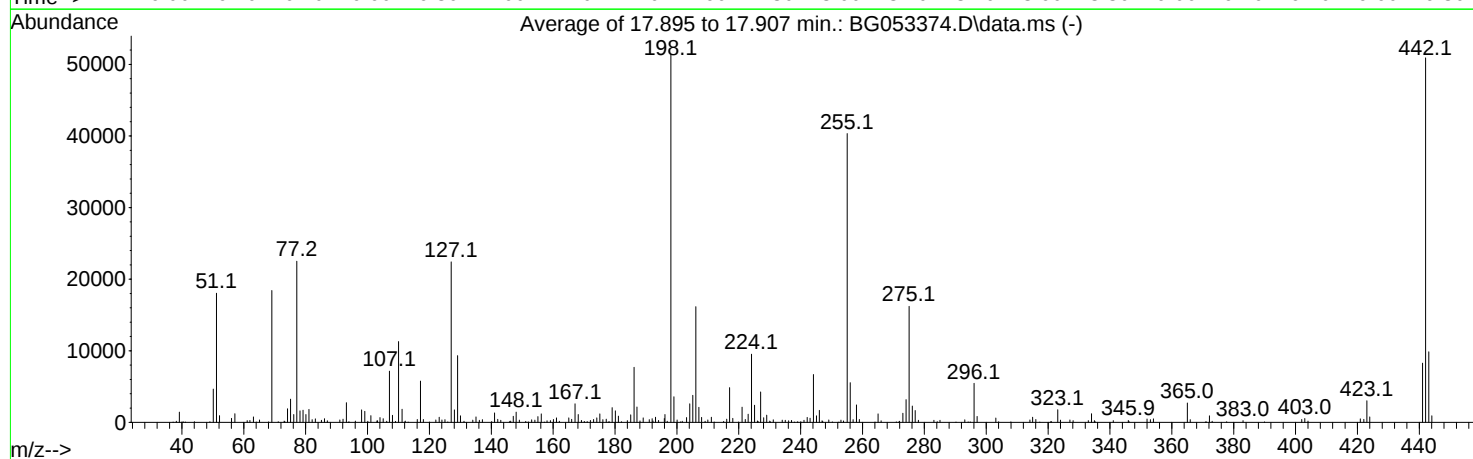


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042922\
 Data File : BG053374.D
 Acq On : 29 Apr 2022 12:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

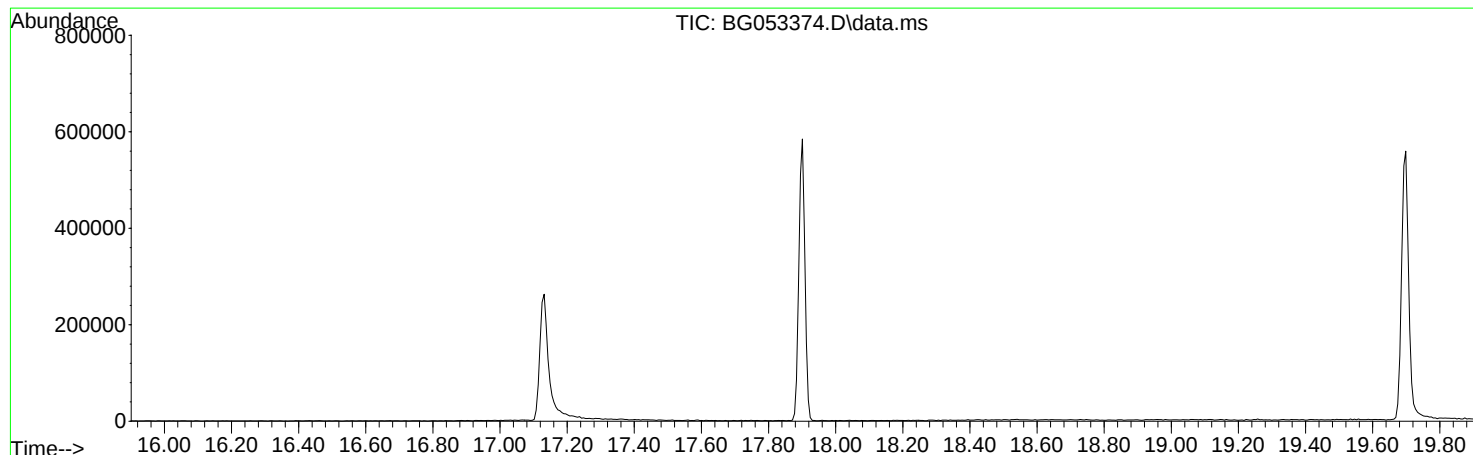

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	18032	PASS
68	69	0.00	2	0.3	64	PASS
69	198	0.00	100	35.8	18412	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	22422	PASS
197	198	0.00	2	0.3	161	PASS
198	198	100	100	100.0	51379	PASS
199	198	5	9	7.0	3579	PASS
275	198	10	60	31.5	16205	PASS
365	198	1	100	5.2	2696	PASS
441	198	0.01	100	16.1	8265	PASS
442	442	50	100	100.0	50904	PASS
443	442	15	24	19.4	9864	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/29/2022	BNA_G	<u>BG053374.D</u>
Compound Name	Response	Retention Time
DDT	203796	20.932
DDD	2583	20.533
DDE	56	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2639	206435	1.28

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042922\
Data File : BG053374.D
Acq On : 29 Apr 2022 12:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 02 03:09:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

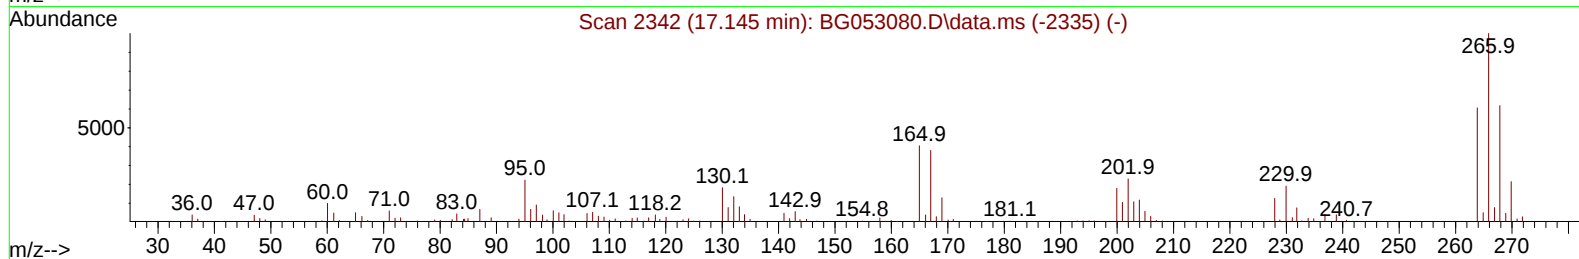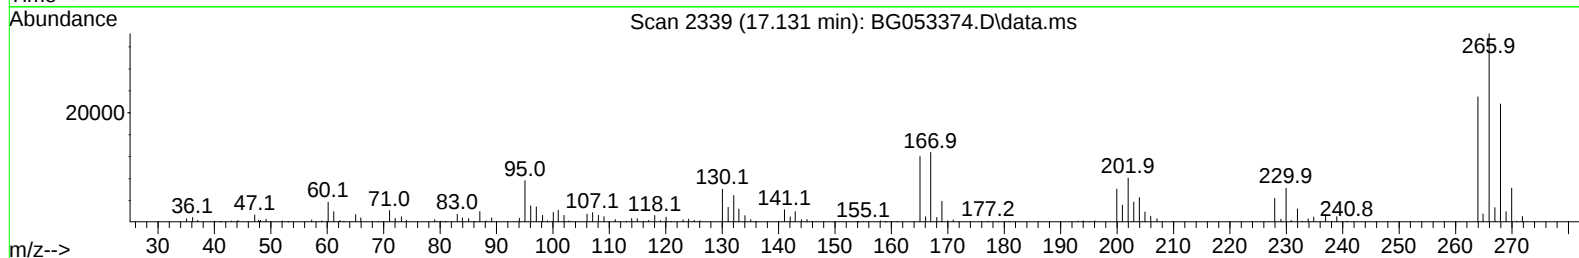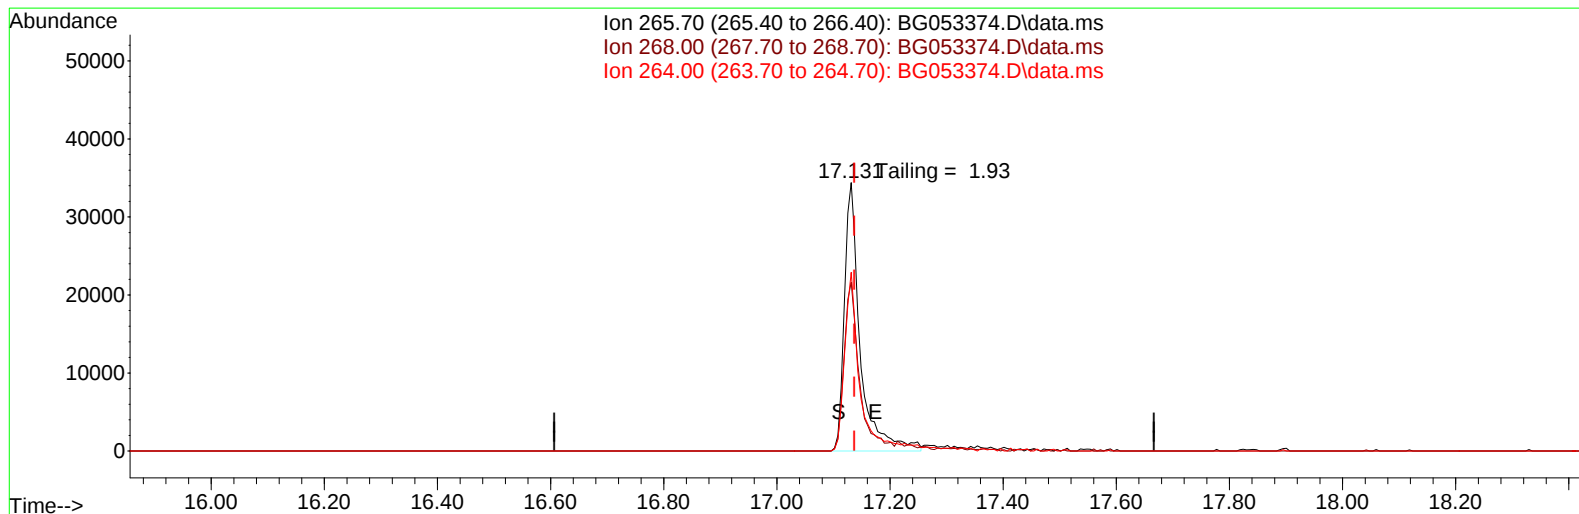

TIC: BG053374.D\data.ms

(70) Pentachlorophenol (C)

17.131min (-0.005) 39753.86 ng




response 65724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.84
264.00	56.60	66.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042922\
Data File : BG053374.D
Acq On : 29 Apr 2022 12:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 02 03:09:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

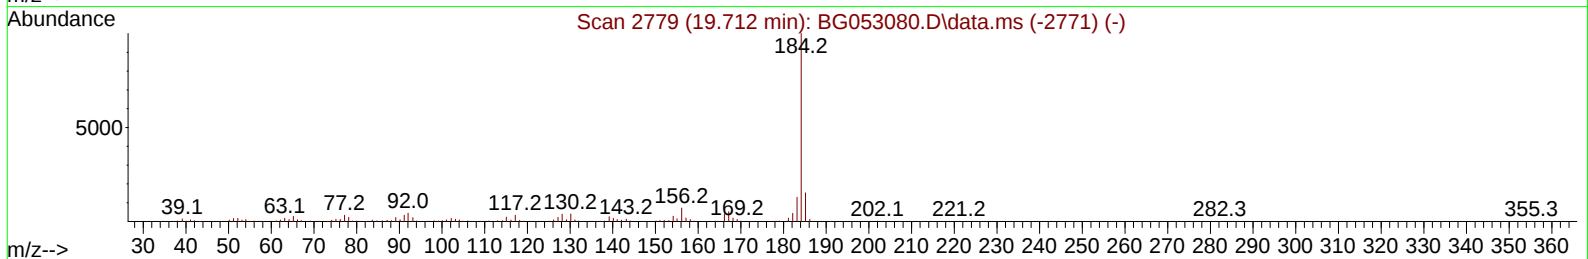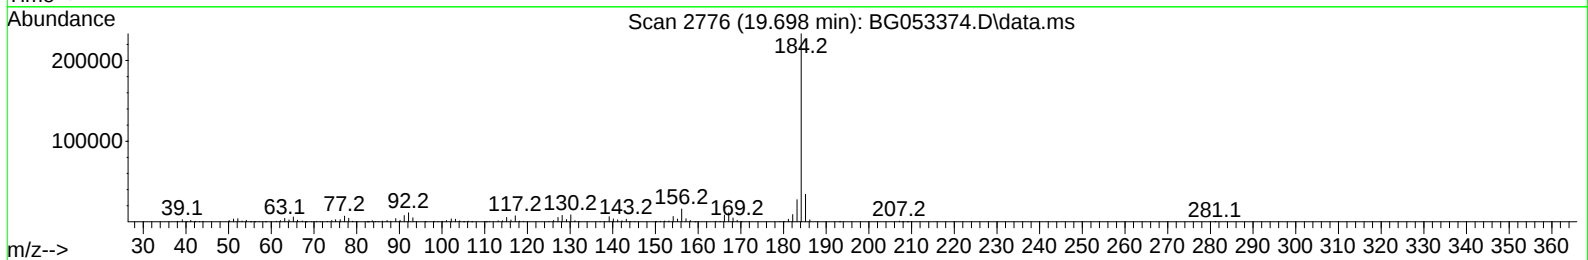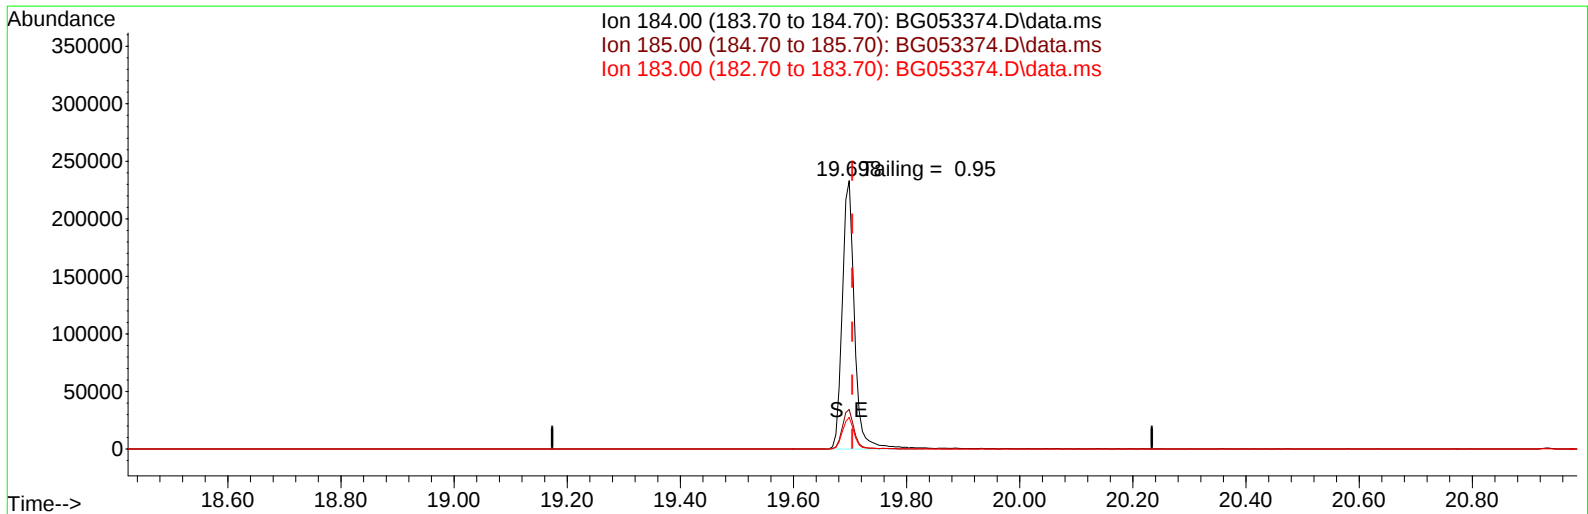

TIC: BG053374.D\data.ms

(77) Benzidine

19.698min (-0.005) 0.00 ng

response 352311

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.71
183.00	11.80	11.79
0.00	0.00	0.00