
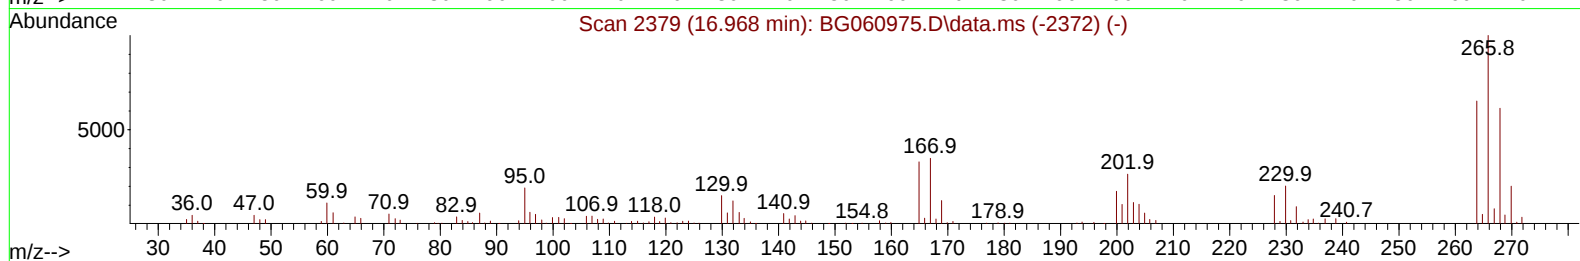
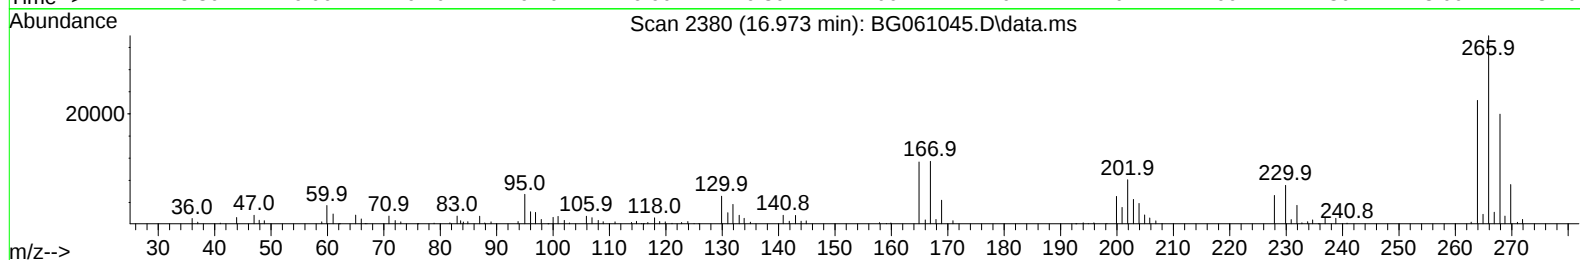


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042924\
Data File : BG061045.D
Acq On : 29 Apr 2024 9:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 09:58:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

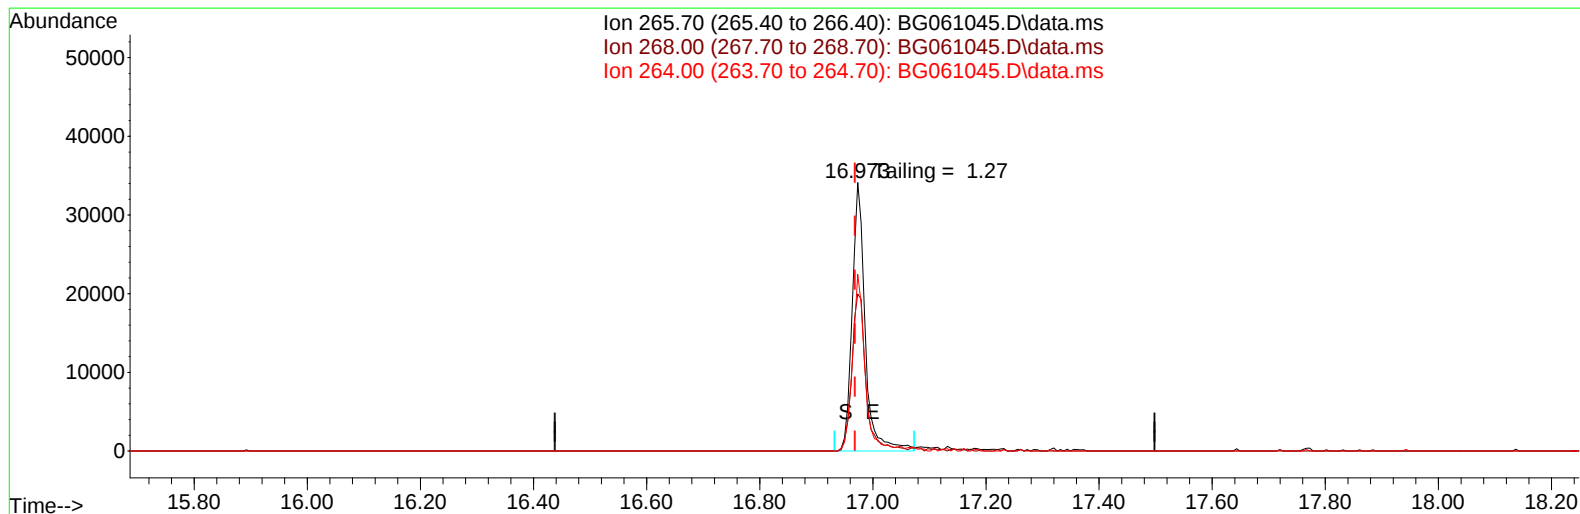

TIC: BG061045.D\data.ms

(70) Pentachlorophenol (C)




16.973min (+ 0.005) 9719.34 ng

response 54722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	58.49
264.00	65.20	65.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042924\
Data File : BG061045.D
Acq On : 29 Apr 2024 9:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 09:58:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

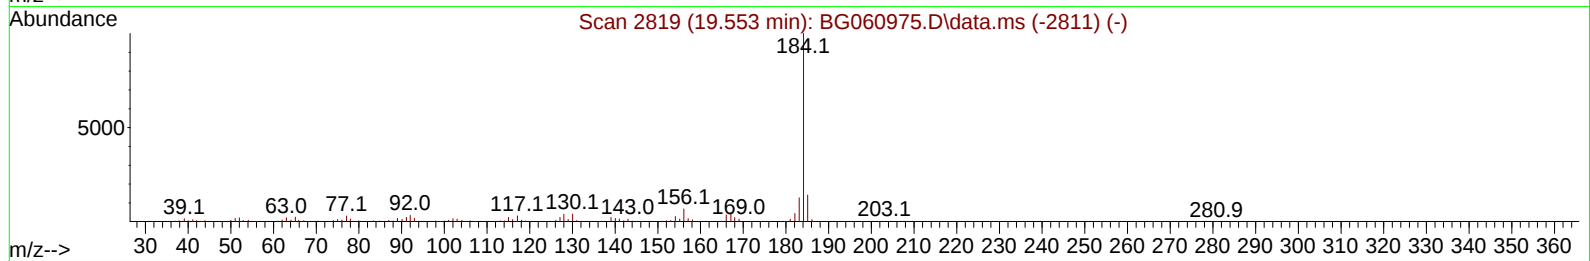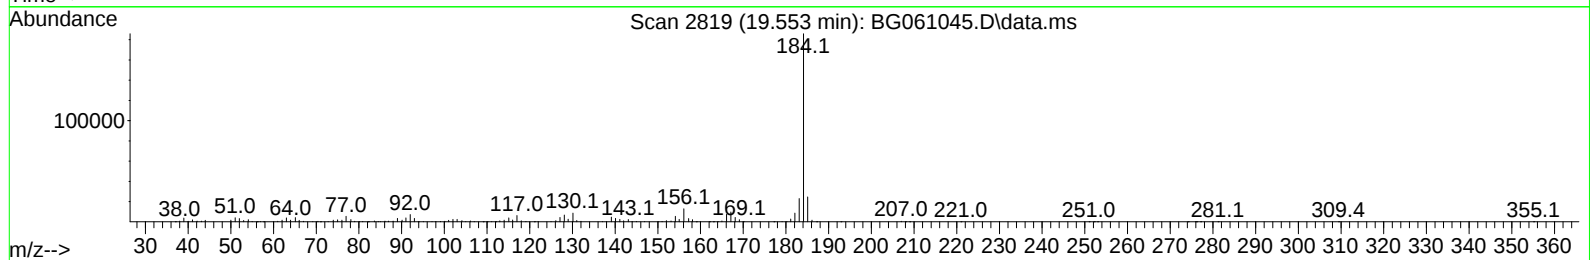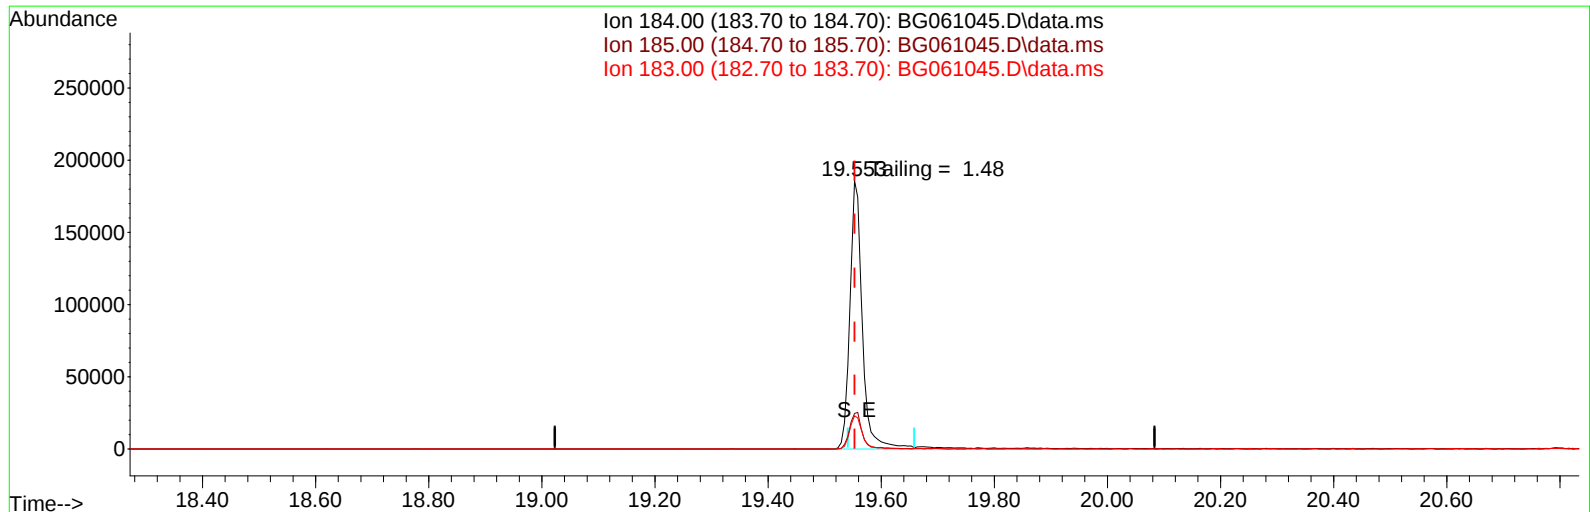

TIC: BG061045.D\data.ms

(77) Benzidine**19.553min (-0.000) 84721.61 ng****response 248028**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.26
183.00	12.70	12.45
0.00	0.00	0.00