


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042924\
Data File : BG061045.D
Acq On : 29 Apr 2024 9:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 22 04:22:00 2024

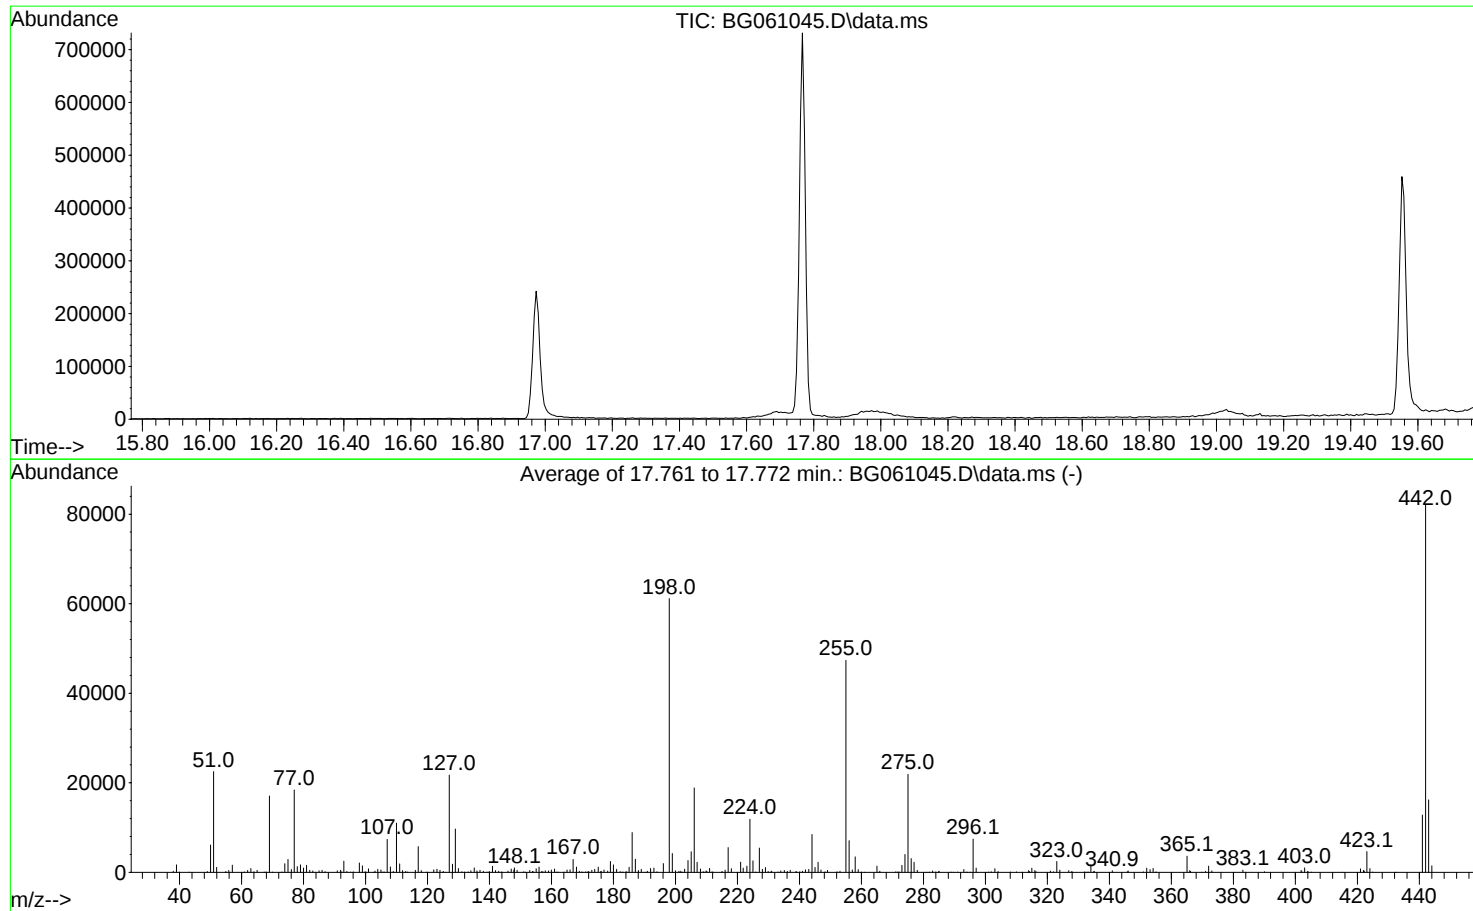




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	22530	PASS
68	69	0.00	2	0.7	112	PASS
69	198	0.00	100	27.9	17041	PASS
70	69	0.00	2	0.4	61	PASS
127	198	10	80	35.6	21744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61152	PASS
199	198	5	9	6.9	4222	PASS
275	198	10	60	35.8	21899	PASS
365	198	1	100	5.9	3598	PASS
441	198	0.01	100	20.9	12790	PASS
442	442	50	100	100.0	82165	PASS
443	442	15	24	19.7	16178	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042924\
Data File : BG061045.D
Acq On : 29 Apr 2024 9:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 29 09:58:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

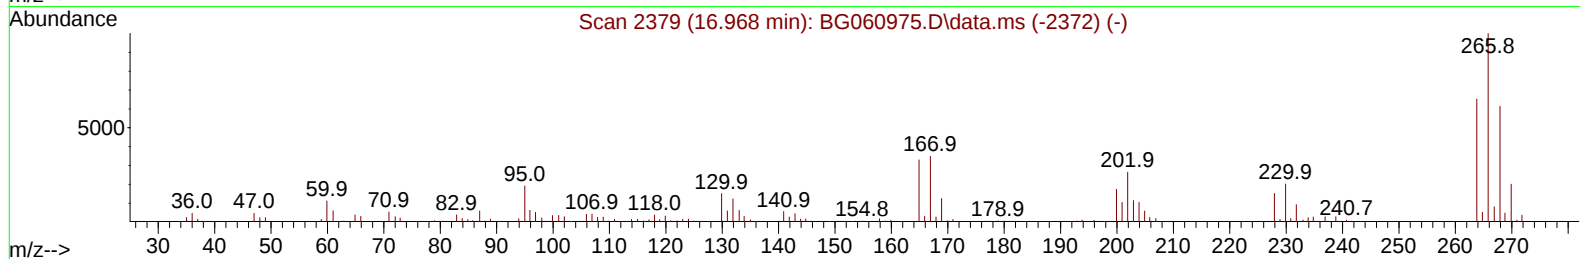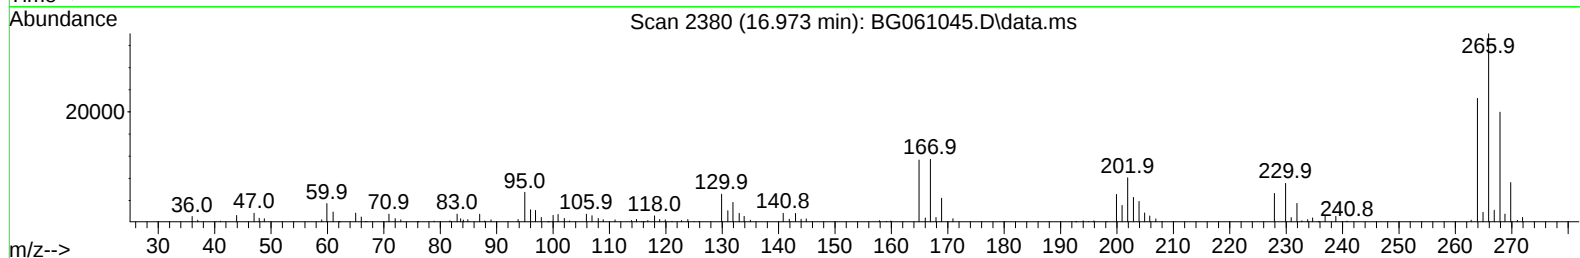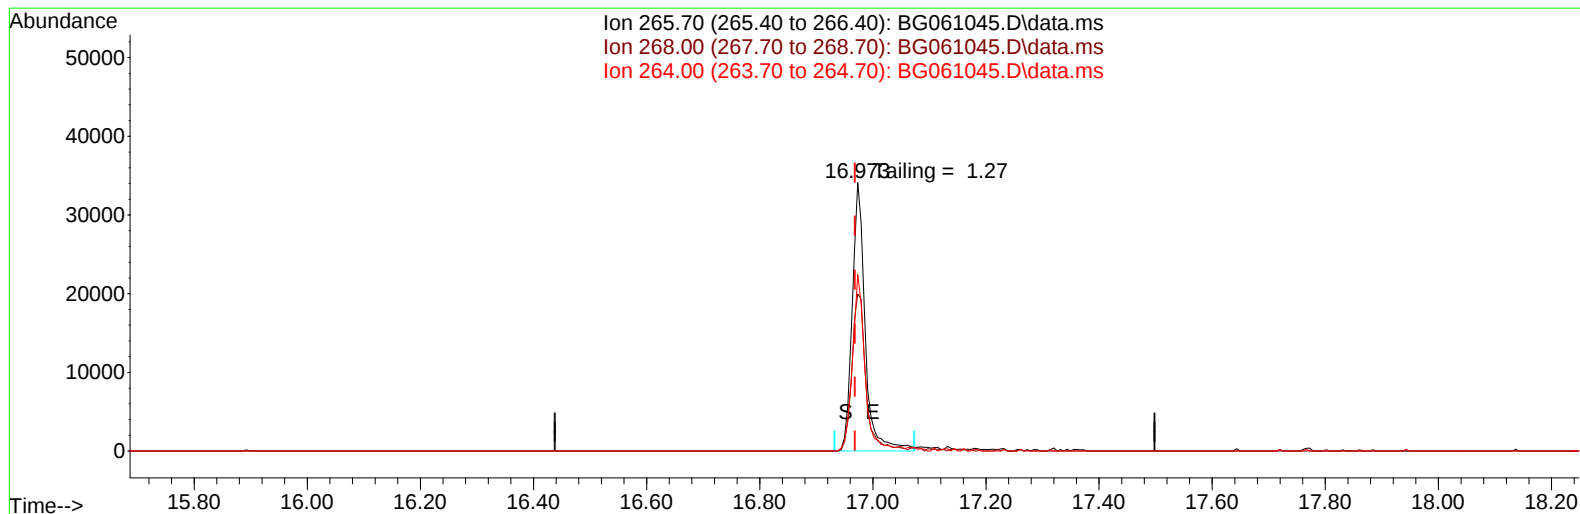

TIC: BG061045.D\data.ms

(70) Pentachlorophenol (C)

16.973min (+ 0.005) 9719.34 ng




response 54722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	58.49
264.00	65.20	65.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042924\
Data File : BG061045.D
Acq On : 29 Apr 2024 9:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 29 09:58:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

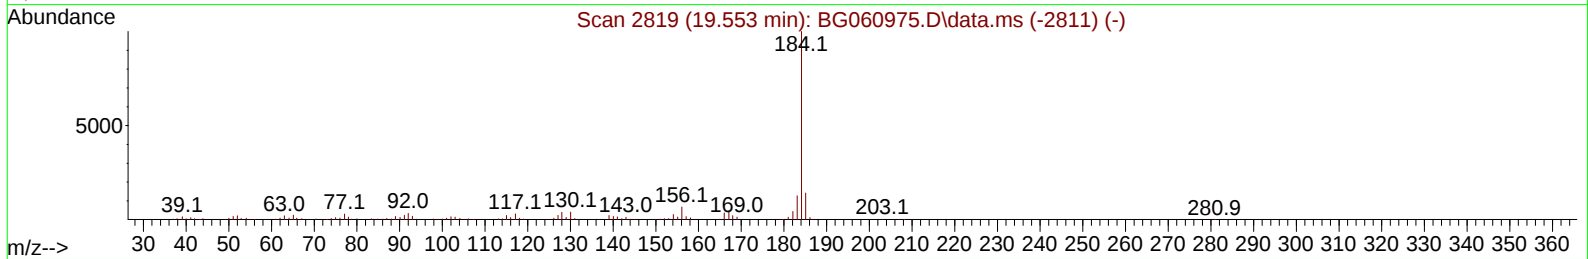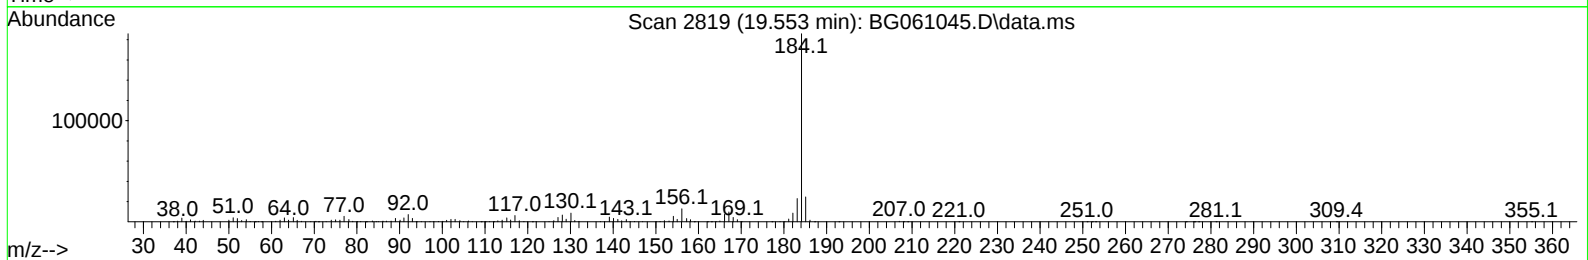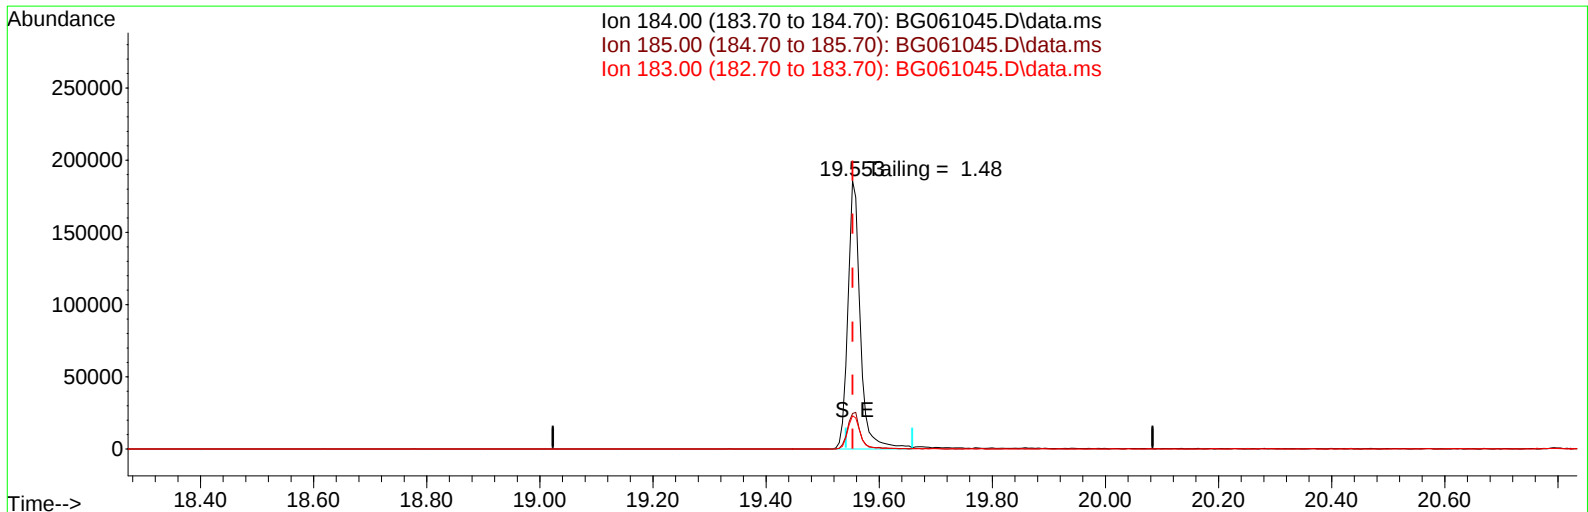

TIC: BG061045.D\data.ms

(77) Benzidine

19.553min (-0.000) 84721.61 ng

response 248028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.26
183.00	12.70	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2024	BNA_G	<u>BG061045.D</u>
Compound Name	Response	Retention Time
DDT	165409	20.792
DDD	14681	20.352
DDE	1228	19.852
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15909	181318	8.77

Instrument :
BNA_G
ClientSampleId :
DFTPP