

Data File : BG026776.D
Acq On : 30 Apr 2017 17:04
Operator : SJ/MA
Sample : I2863-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHTG1

Quant Time: May 01 04:19:16 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 04:18:19 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	164553	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	846872	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	495280	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	959246	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	877146	20.00	ng/ul	0.00
83) Perylene-d12	24.75	264	917286	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	20194	5.53	ng/uL	0.00
5) Phenol-d5	7.19	99	139010	9.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	253648	29.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	311486	24.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	246251	20.20	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	202607	28.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	224702	29.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	339903	27.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	38772	2.37	ng/ul	0.01
43) Dimethylphthalate-d6	14.02	166	1168010	29.30	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1502174	30.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.86	143	48278	6.72	ng/ul	0.02
57) Fluorene-d10	15.60	176	1001758	28.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	159781	27.43	ng/ul	0.00
70) Anthracene-d10	17.45	188	1457019	31.30	ng/ul	0.00
76) Pyrene-d10	19.73	212	1410629	30.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1352348	31.18	ng/ul	0.00

Target Compounds					Qvalue
81) Bis(2-ethylhexyl)phthalate	21.47	149	41745	1.07 ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026776.D

Acq On : 30 Apr 2017 17:04

Operator : SJ/MA

Sample : I2863-10

Misc :

ALS Vial : 13 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

JHTG1


Quant Time: May 01 04:19:16 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon May 01 04:18:19 2017

Response via : Initial Calibration

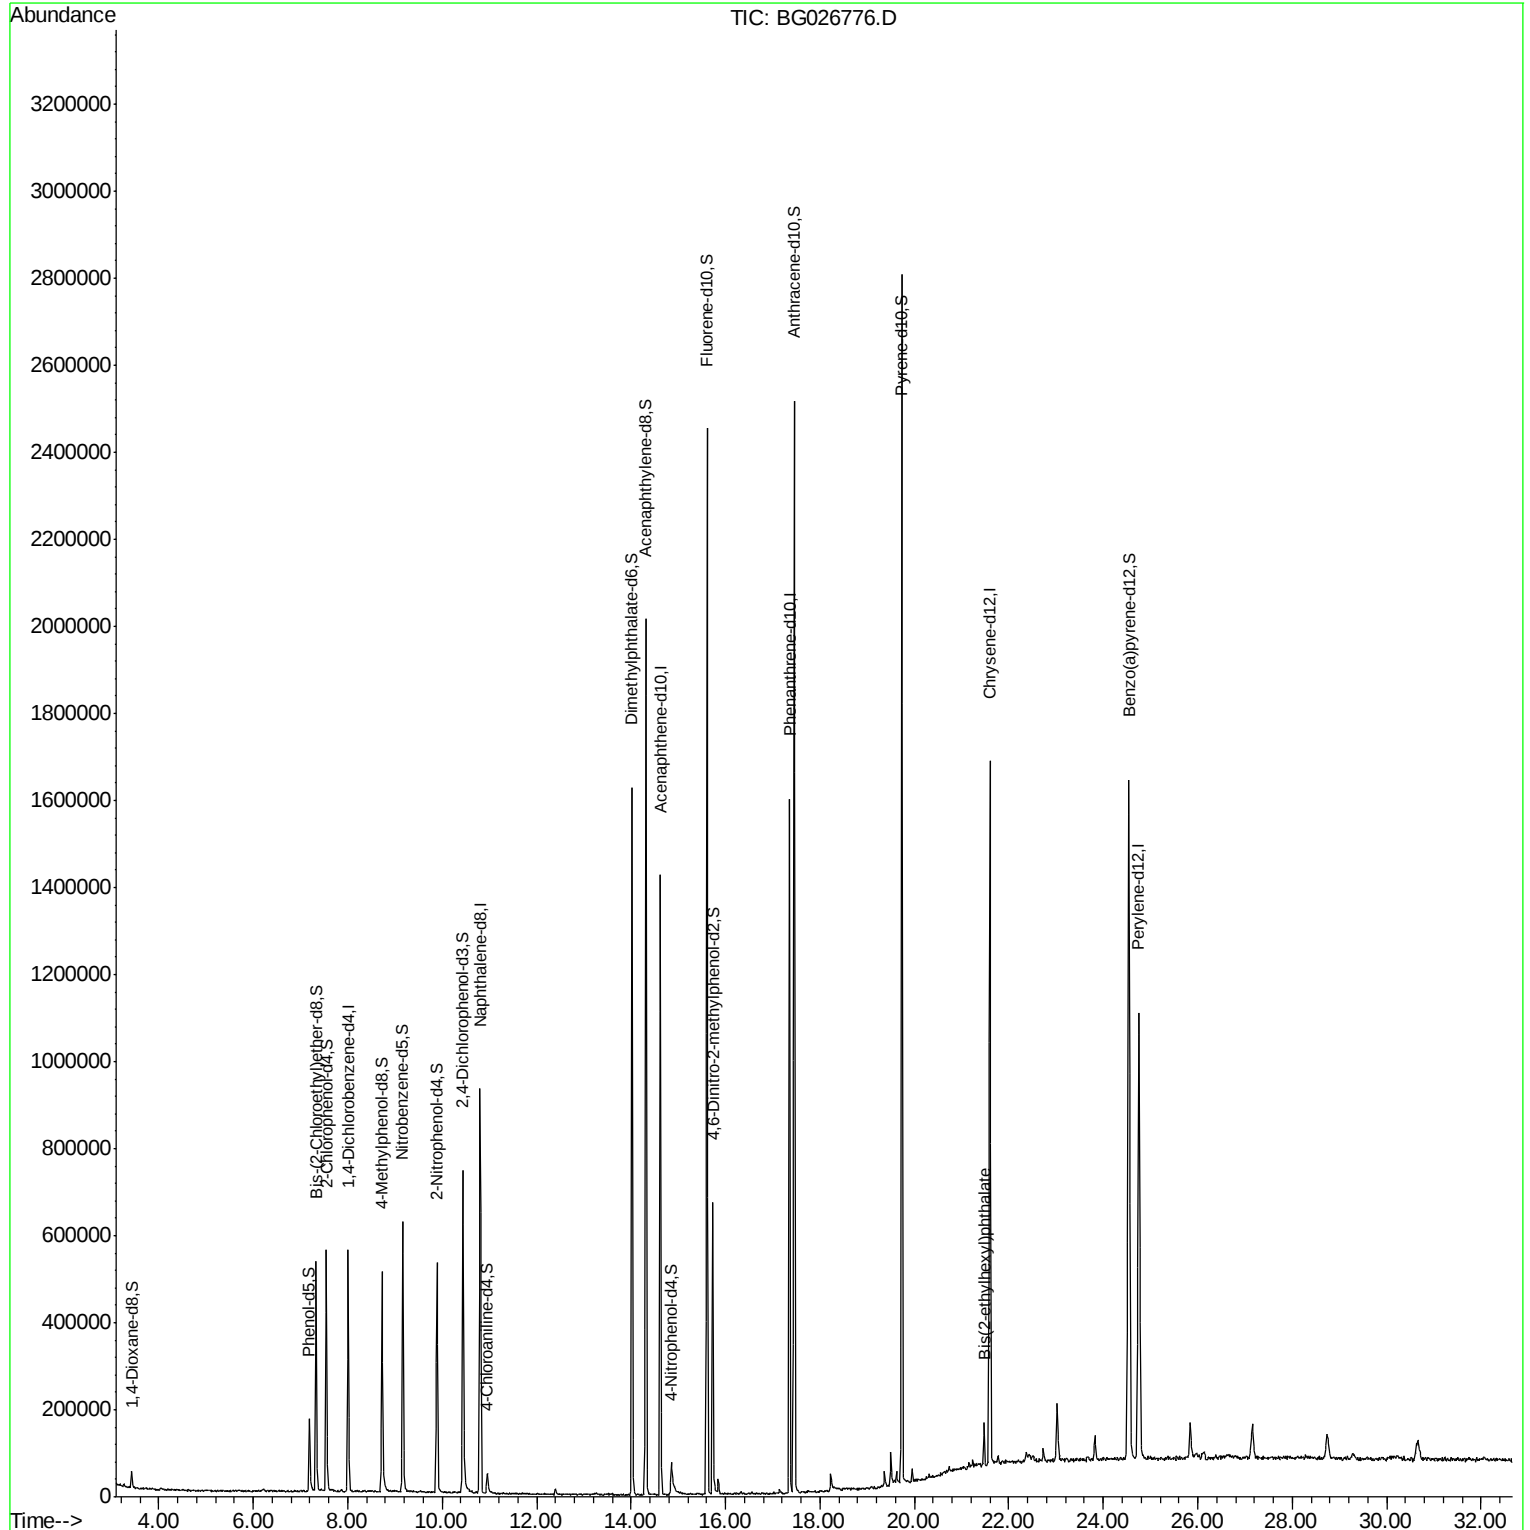

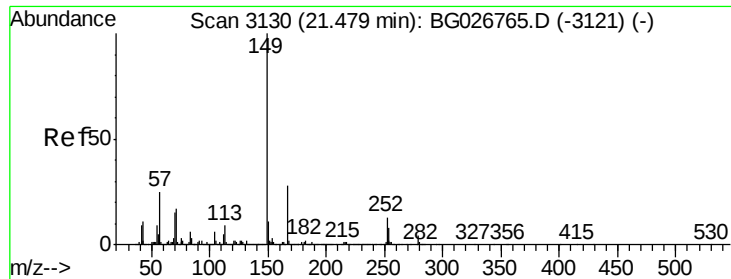

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.07 ng/ul

RT: 21.47 min Scan# 3129

Delta R.T. -0.00 min

Lab File: BG026776.D

Acq: 30 Apr 2017 17:04

Instrument :

BNA_G

ClientSampleId :

JHTG1


Tgt Ion:149 Resp: 41745

Ion Ratio Lower Upper

149 100

167 25.6 21.8 32.8

279 3.7 4.5 6.7#

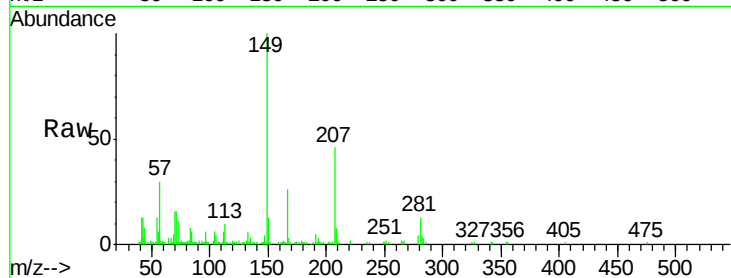

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

