

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026773.D
 Acq On : 30 Apr 2017 15:07
 Operator : SJ/MA
 Sample : I2863-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHTD1

Manual Integrations
 APPROVED

mohammad
 5/1/2017 6:51:28 PM

Quant Time: May 01 04:48:26 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 04:18:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	150674	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	766095	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	449032	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	873469	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	794710	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	823508	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	14677	4.39	ng/uL	0.00
5) Phenol-d5	7.20	99	43150	3.21	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.33	67	142115	17.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	158039	13.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	94606	8.48	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	115902	18.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	129455	18.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	196905	17.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.96	131	17349	1.17	ng/ul	0.02
43) Dimethylphthalate-d6	14.02	166	690044	19.09	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	828977	18.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.87	143	12106m	1.86	ng/ul	0.03
57) Fluorene-d10	15.61	176	551310	17.48	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	78204	14.74	ng/ul	0.00
70) Anthracene-d10	17.45	188	714953	16.87	ng/ul	0.00
76) Pyrene-d10	19.73	212	677695	16.16	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.53	264	619018	15.90	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.06	163	54341	1.54	ng/ul# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026773.D
Acq On : 30 Apr 2017 15:07
Operator : SJ/MA
Sample : I2863-07
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHTD1

Manual Integrations
APPROVED

mohammad
5/1/2017 6:51:28 PM

Quant Time: May 01 04:48:26 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 04:18:19 2017
Response via : Initial Calibration

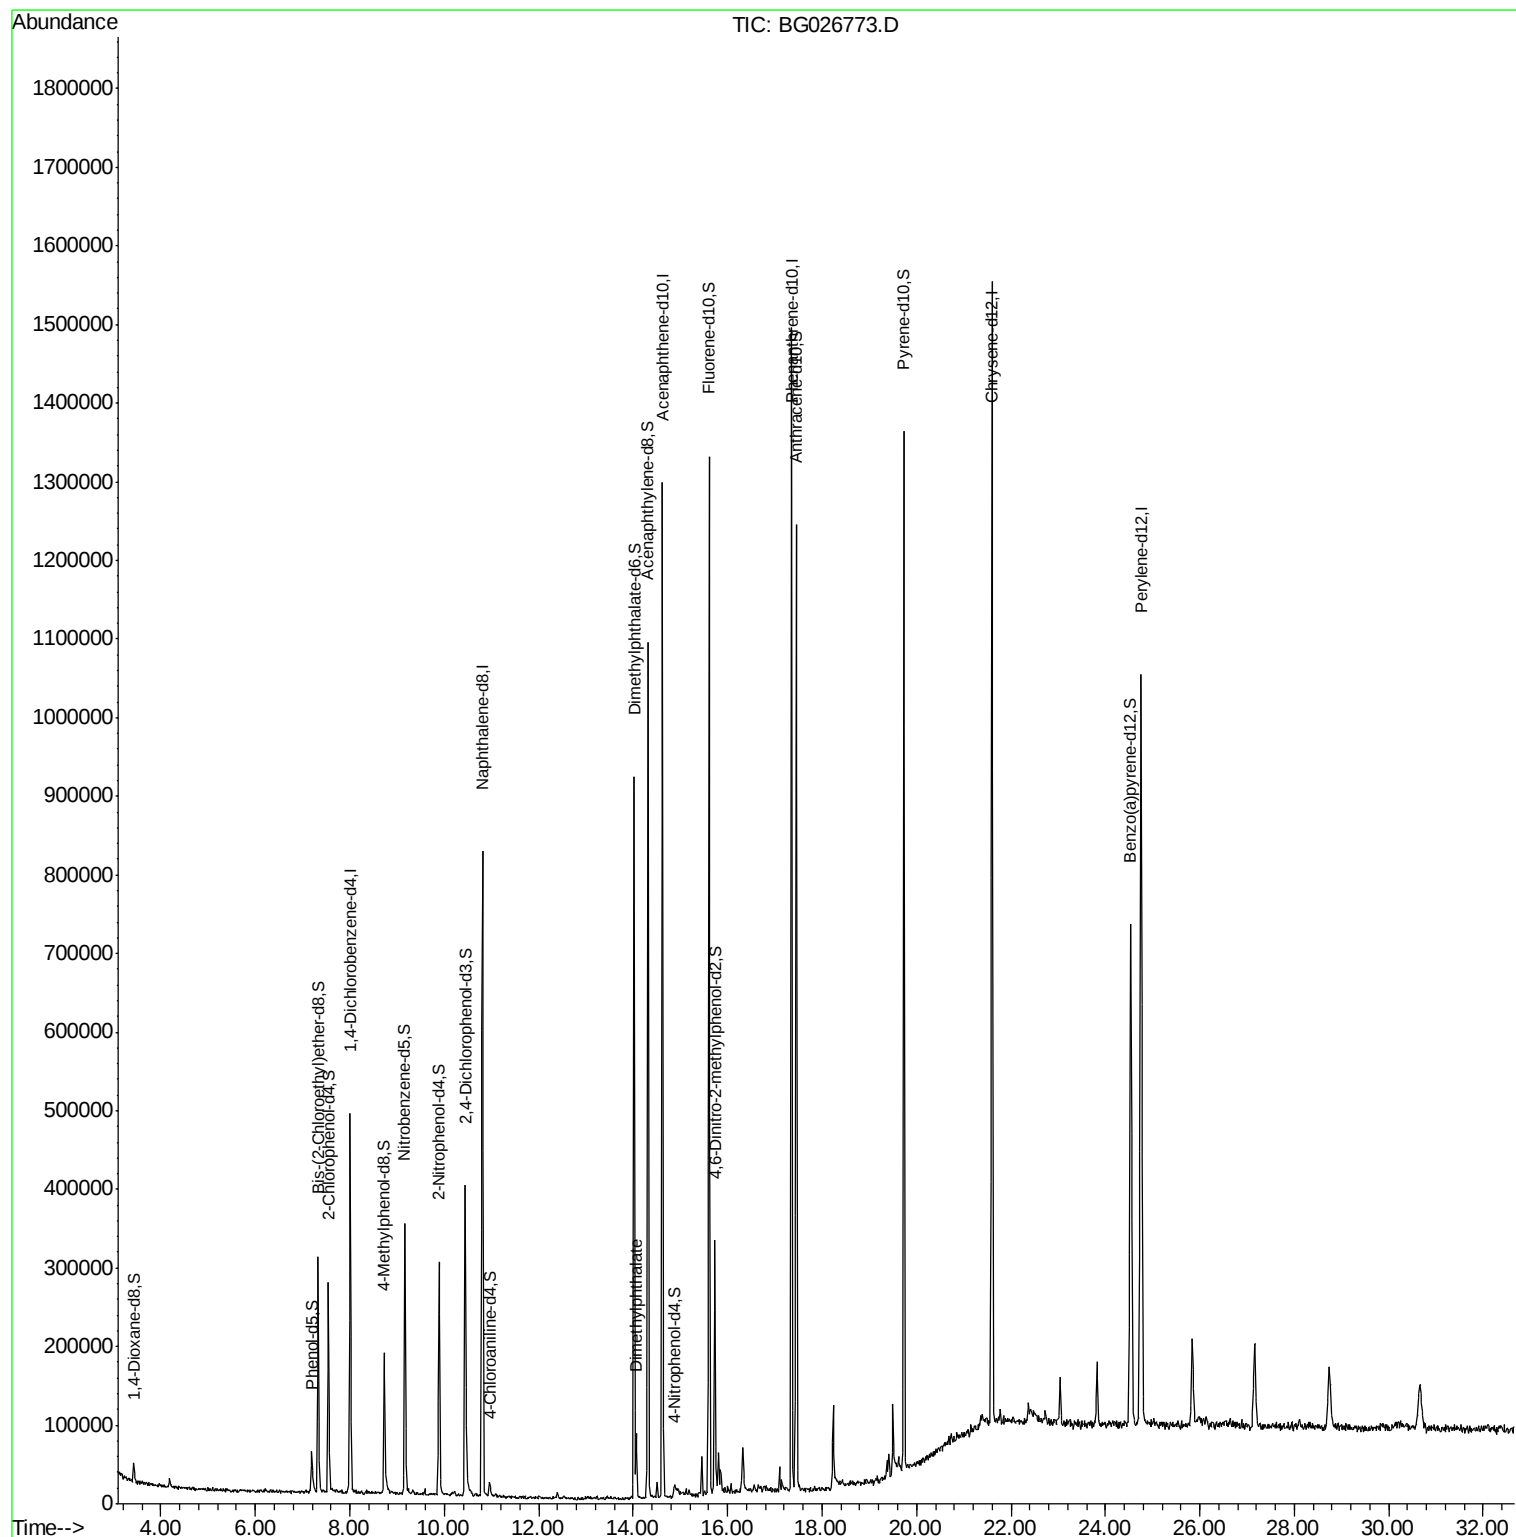

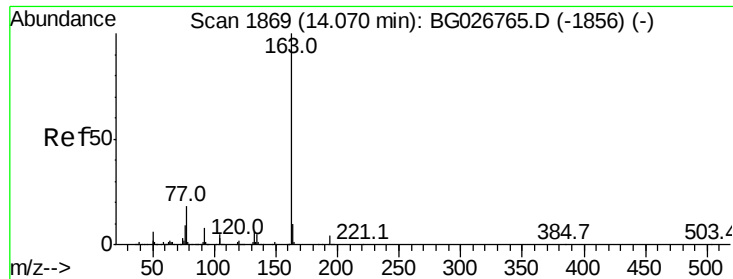

#44
 Dimethylphthalate
 Concen: 1.54 ng/ul
 RT: 14.06 min Scan# 1868
 Delta R.T. -0.01 min
 Lab File: BG026773.D
 Acq: 30 Apr 2017 15:07

Instrument :
 BNA_G
 ClientSampleId :
 JHTD1

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	3.3	3.4	5.0#
164	8.6	9.0	13.4#

Manual Integrations
 APPROVED

mohammad
 5/1/2017 6:51:28 PM

