

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026779.D
 Acq On : 30 Apr 2017 19:01
 Operator : SJ/MA
 Sample : I2846-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT08

Quant Time: May 01 04:19:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 04:18:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	190462	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	960442	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	552987	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	1057462	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	980003	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	1029151	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	24960	5.90	ng/uL	0.00
5) Phenol-d5	7.18	99	594475	34.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	332478	33.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	475505	32.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	514129	36.44	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	263818	32.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	295237	33.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	457987	33.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	718598	38.69	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1459178	32.78	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1844842	33.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.83	143	241848	30.15	ng/ul	0.00
57) Fluorene-d10	15.61	176	1250596	32.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	199513	31.07	ng/ul	0.00
70) Anthracene-d10	17.45	188	1717078	33.46	ng/ul	0.00
76) Pyrene-d10	19.73	212	1678240	32.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1672181	34.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.07	163	243870	5.60	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026779.D
Acq On : 30 Apr 2017 19:01
Operator : SJ/MA
Sample : I2846-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT08

Quant Time: May 01 04:19:34 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 04:18:19 2017
Response via : Initial Calibration

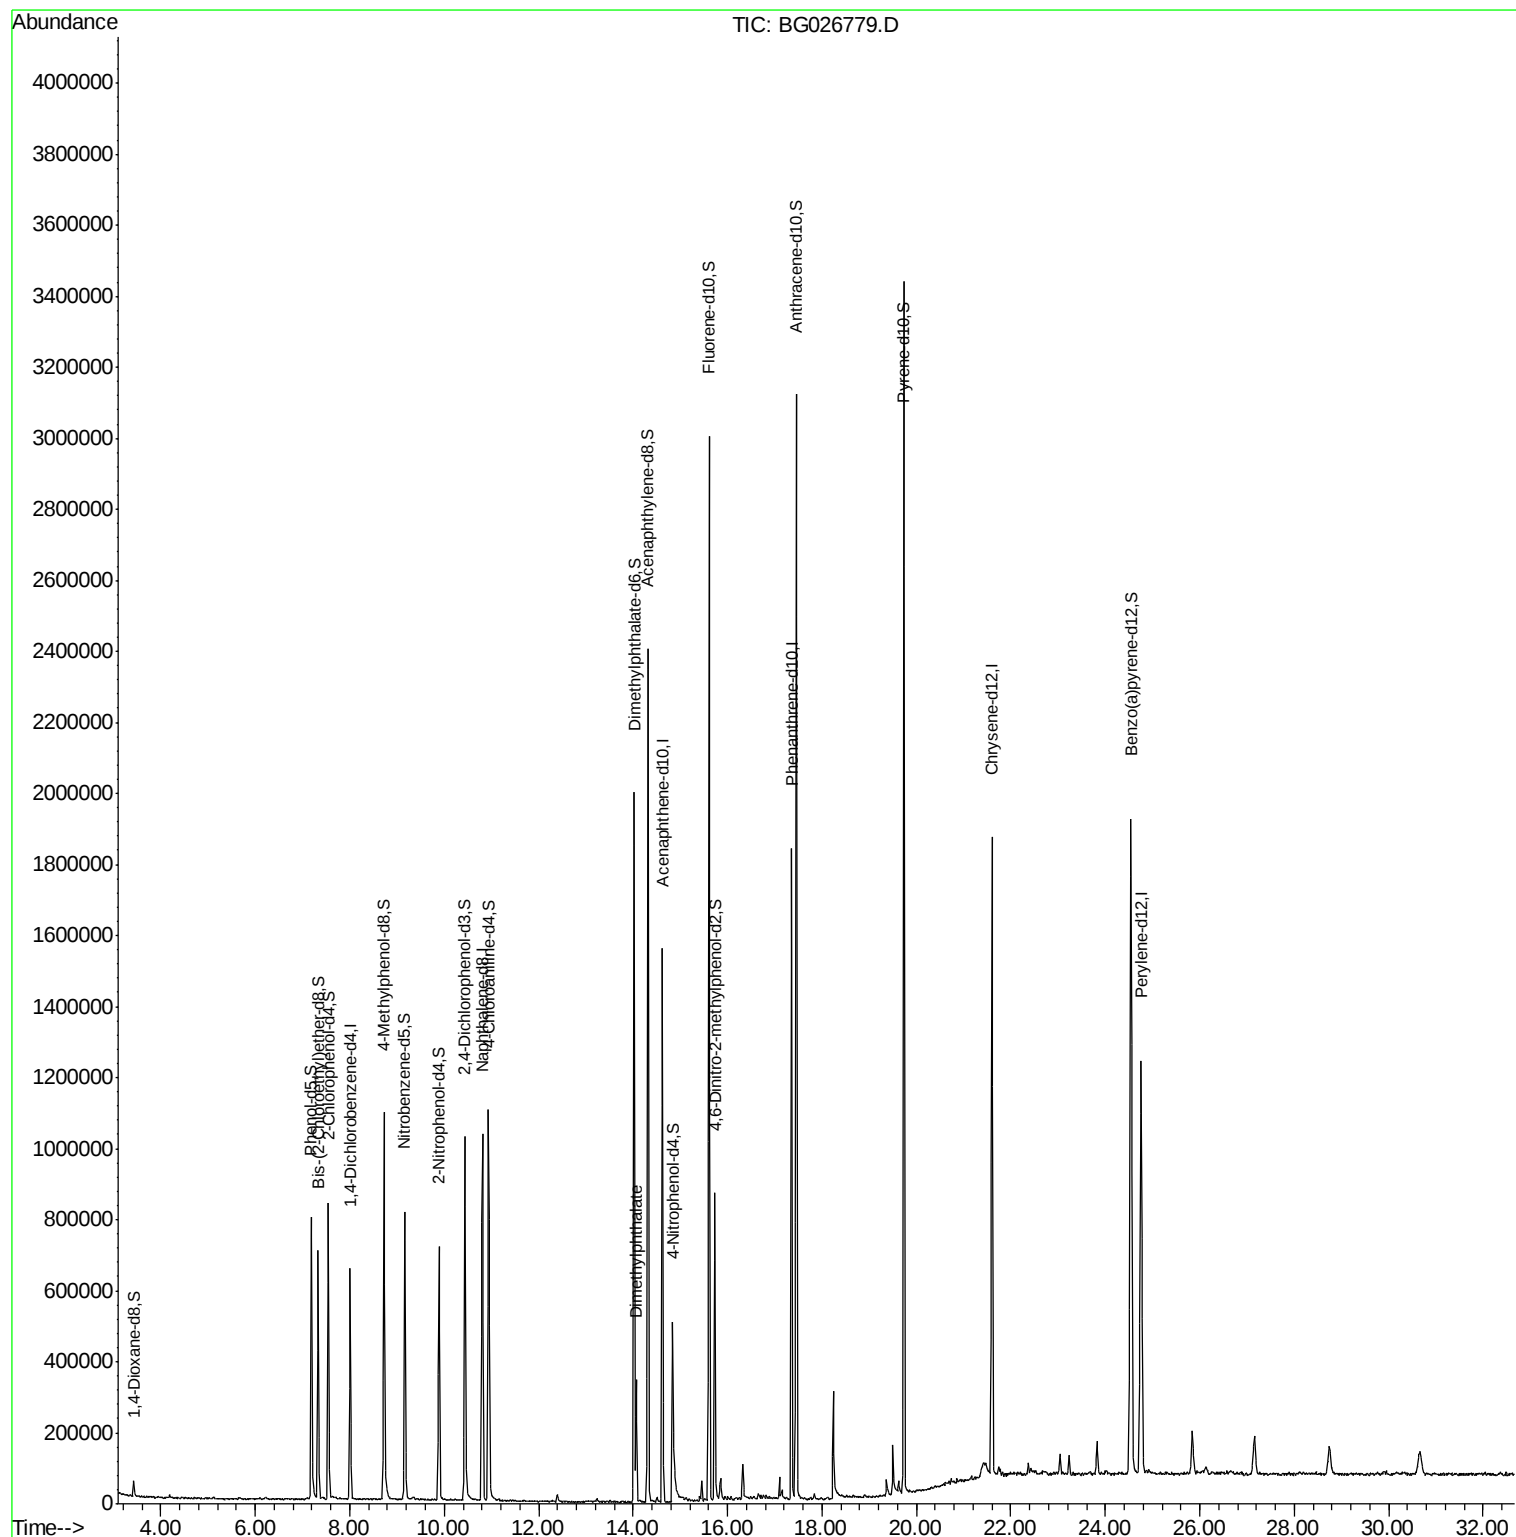

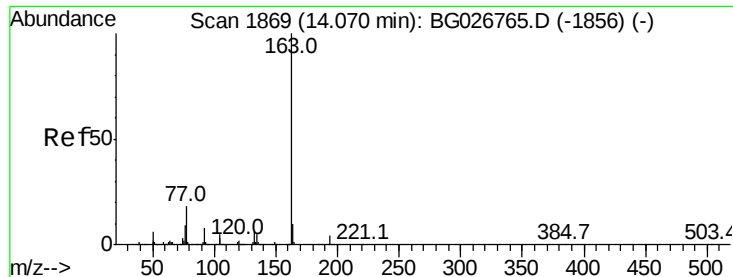

#44

Dimethylphthalate

Concen: 5.60 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. 0.00 min

Lab File: BG026779.D

Acq: 30 Apr 2017 19:01

Instrument :

BNA_G

ClientSampleId :

JHT08


Tot Ion:163 Resp: 243870

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.3 9.0 13.4

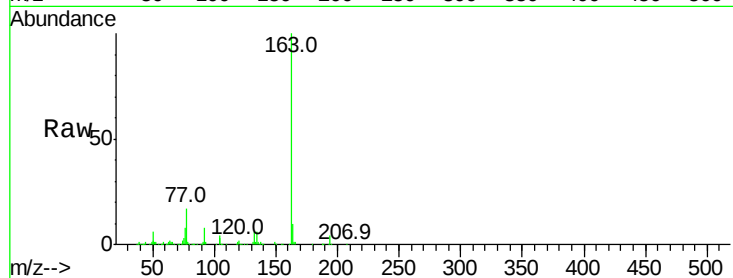

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

