

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026781.D
 Acq On : 30 Apr 2017 20:19
 Operator : SJ/MA
 Sample : I2846-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT47

Quant Time: May 01 05:02:51 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	165415	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	846268	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	491729	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	969032	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	881242	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	911635	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	23752	6.47	ng/uL	0.00
5) Phenol-d5	7.19	99	564307	38.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	324196	37.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	453152	36.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	495873	40.47	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	252509	35.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	284381	36.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	438773	35.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	704257	43.04	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1411123	35.65	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1793717	36.08	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	241882	33.91	ng/ul	0.00
57) Fluorene-d10	15.61	176	1216243	35.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	193541	32.89	ng/ul	0.00
70) Anthracene-d10	17.45	188	1667973	35.47	ng/ul	0.00
76) Pyrene-d10	19.74	212	1602461	34.45	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1585416	36.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.07	163	213914	5.52	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026781.D
Acq On : 30 Apr 2017 20:19
Operator : SJ/MA
Sample : I2846-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT47

Quant Time: May 01 05:02:51 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

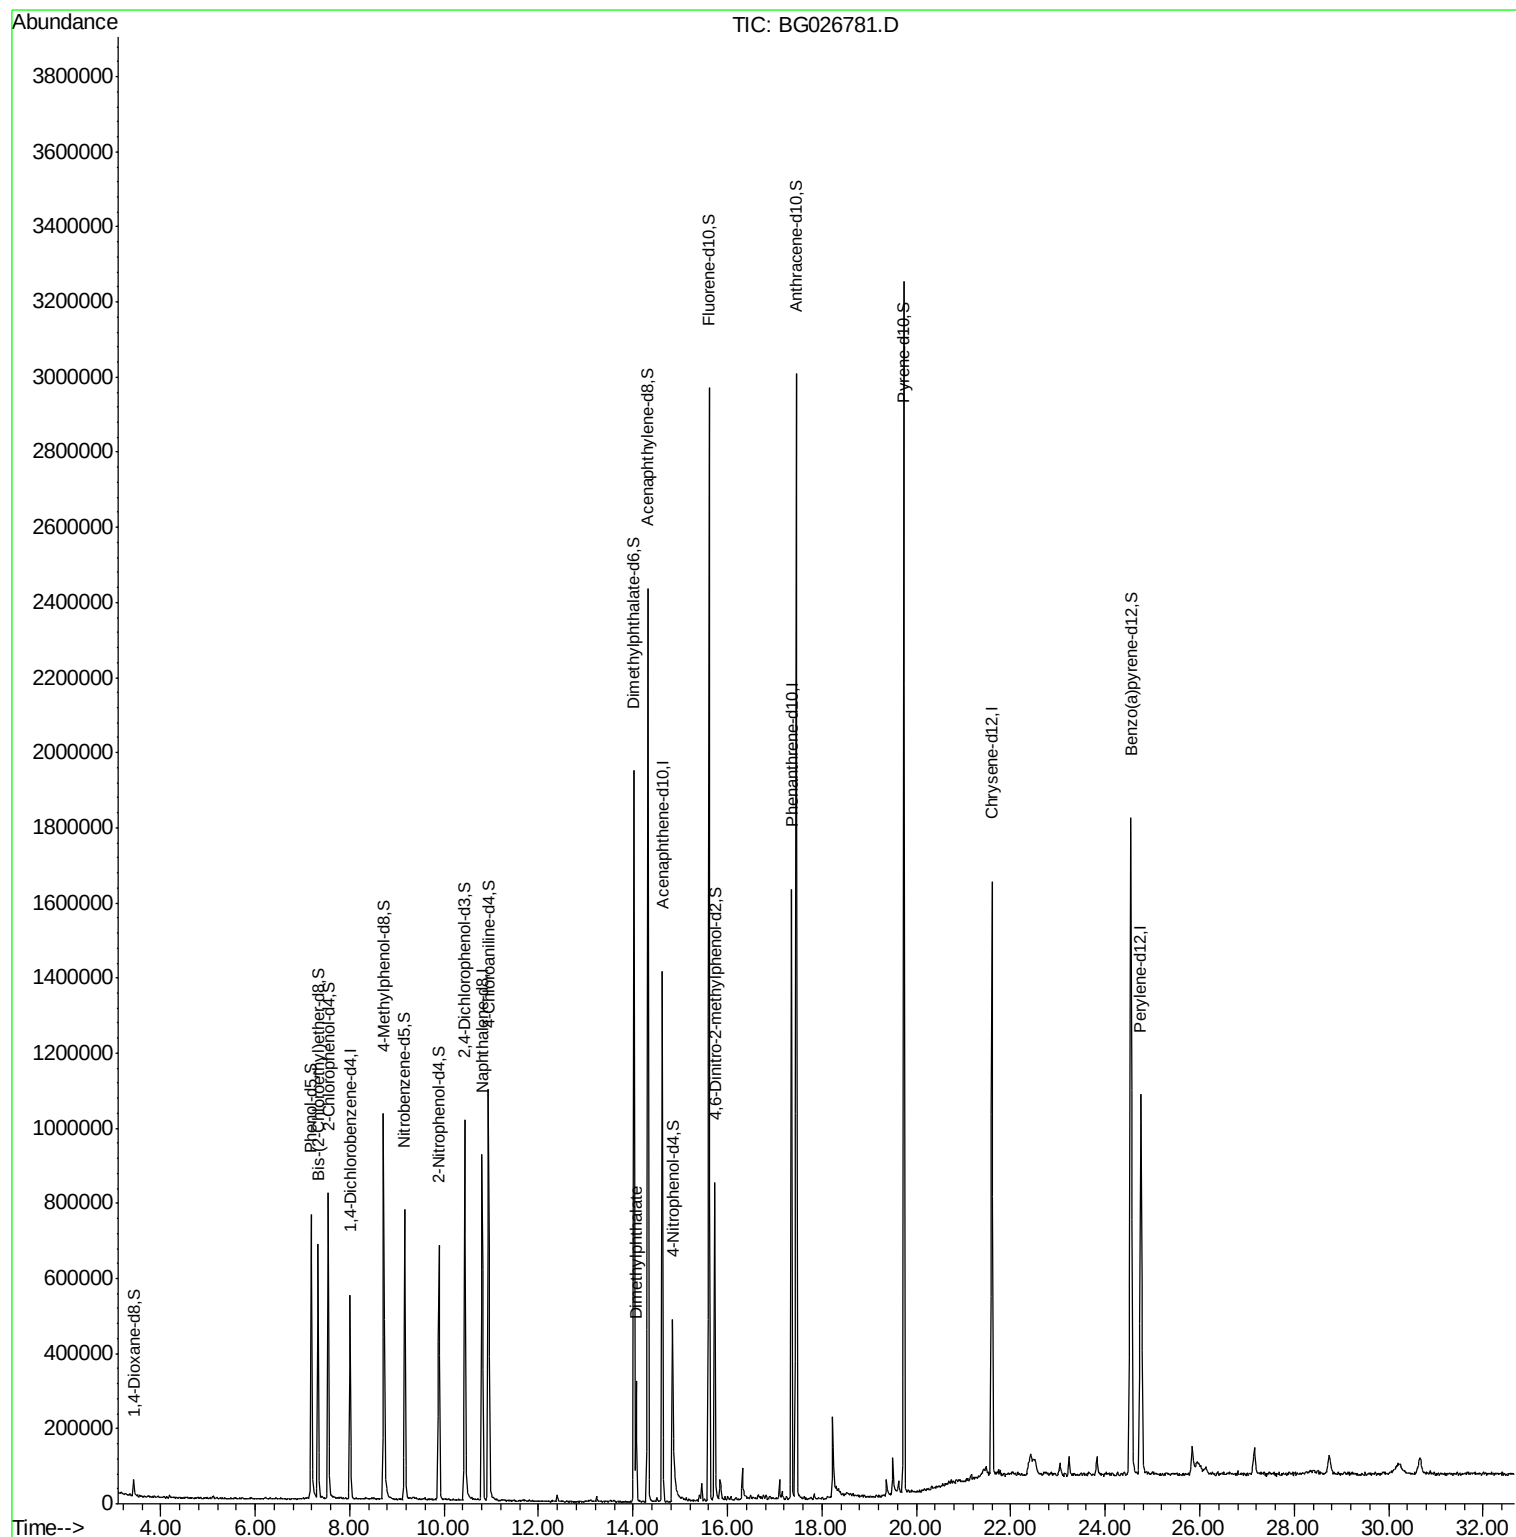

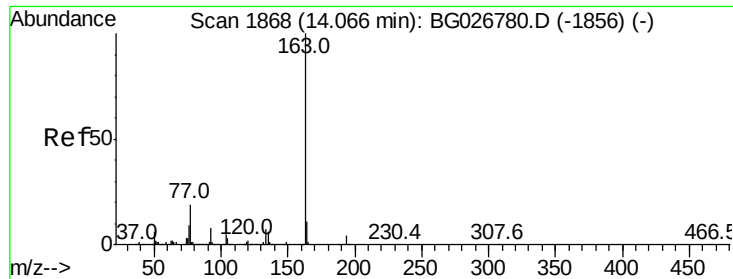

#44

Dimethylphthalate

Concen: 5.52 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. 0.00 min

Lab File: BG026781.D

Acq: 30 Apr 2017 20:19

Instrument :

BNA_G

ClientSampleId :

JHT47

Tot Ion:163 Resp: 213914

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.0 9.0 13.4

