

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026785.D
 Acq On : 30 Apr 2017 22:55
 Operator : SJ/MA
 Sample : I2846-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT60

Quant Time: May 01 05:03:16 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	172688	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	869885	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	495368	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	948135	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	869969	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	905553	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	23185	6.05	ng/uL	0.00
5) Phenol-d5	7.18	99	539639	35.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	308036	33.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	428514	32.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	468388	36.62	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	237783	32.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	269079	34.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	425710	33.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	663265	39.43	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1327429	33.29	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1722615	34.39	ng/ul	0.00
51) 4-Nitrophenol-d4	14.83	143	232810	32.40	ng/ul	0.00
57) Fluorene-d10	15.61	176	1175419	33.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	186088	32.32	ng/ul	0.00
70) Anthracene-d10	17.45	188	1596836	34.70	ng/ul	0.00
76) Pyrene-d10	19.73	212	1541052	33.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1511694	35.31	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.07	163	243631	6.24	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026785.D
Acq On : 30 Apr 2017 22:55
Operator : SJ/MA
Sample : I2846-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT60

Quant Time: May 01 05:03:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

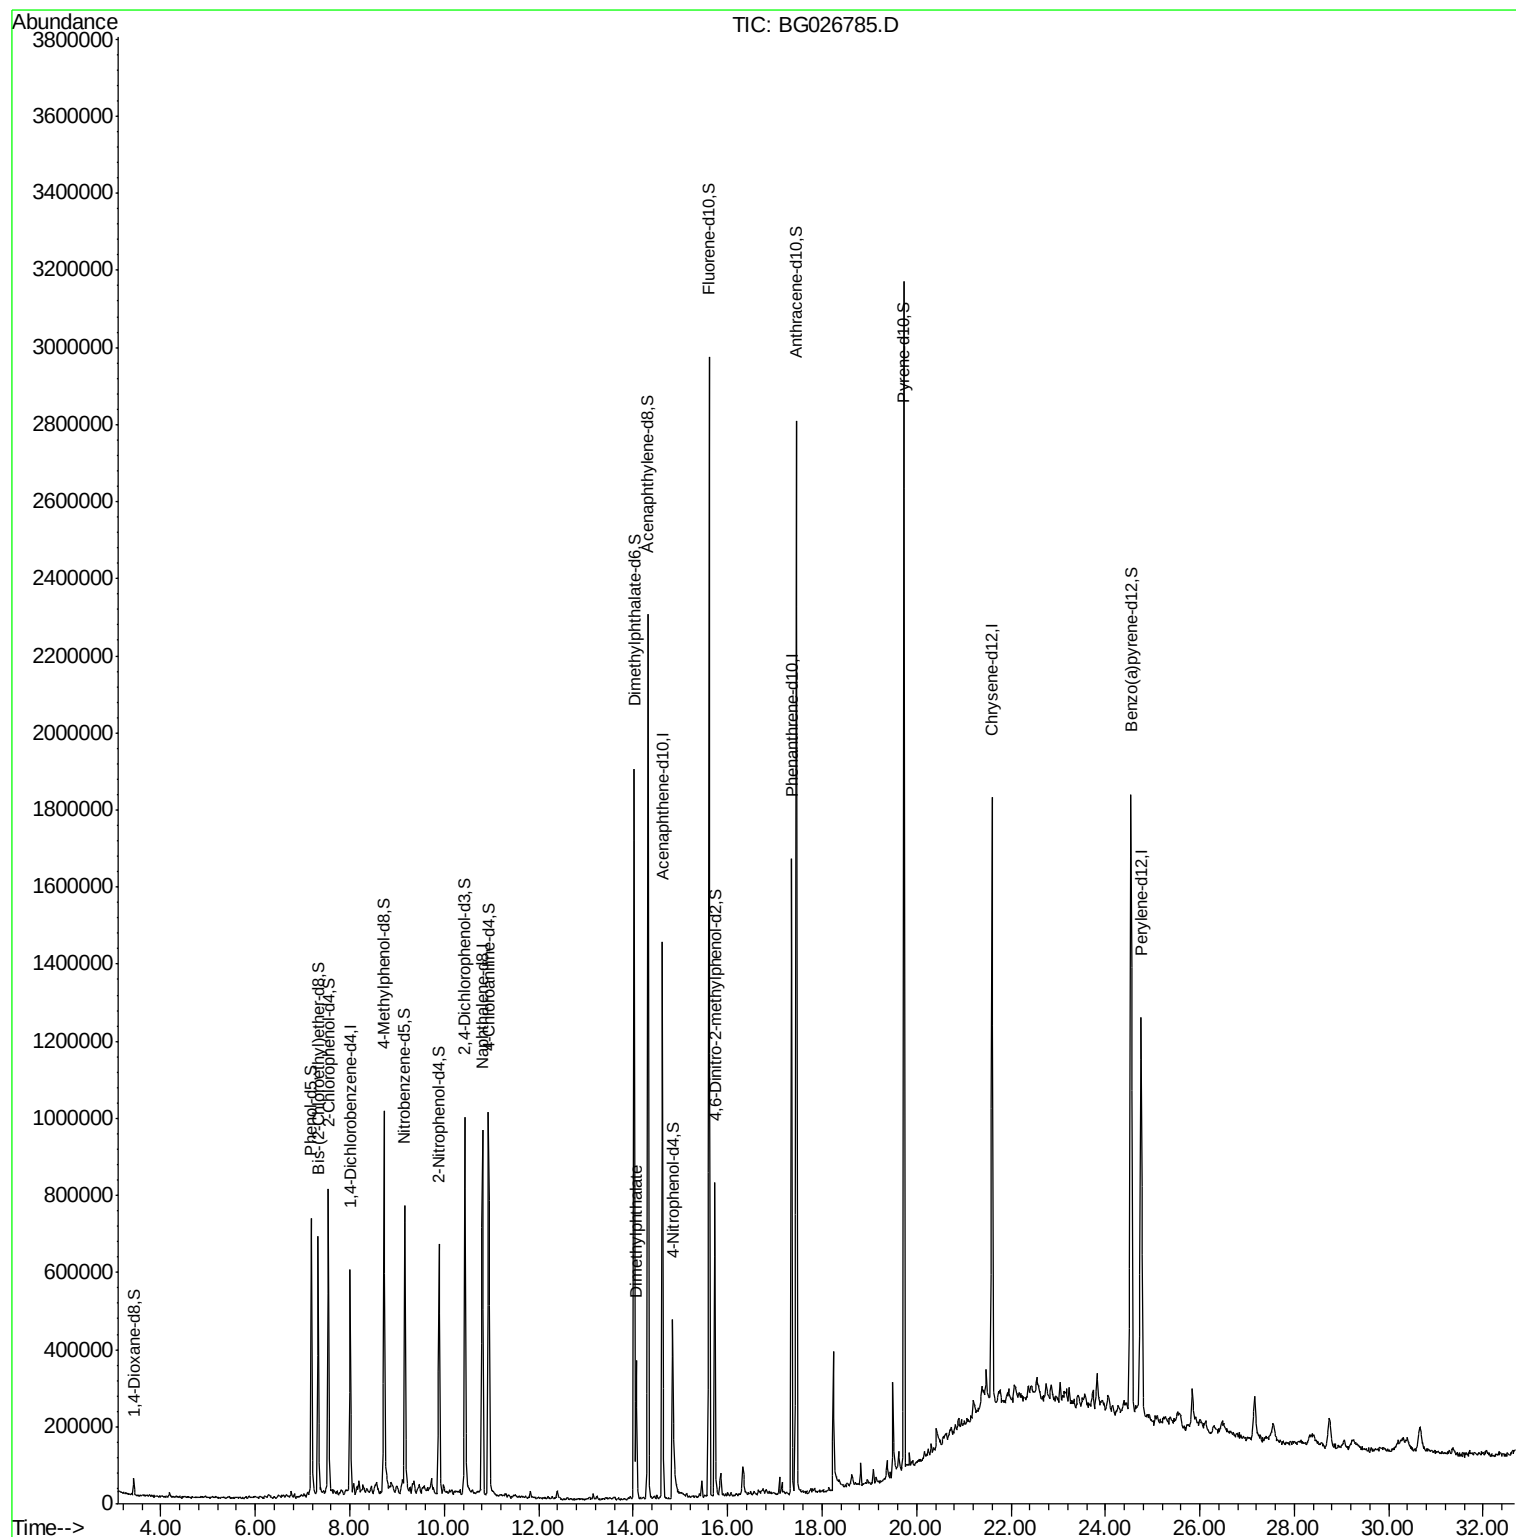

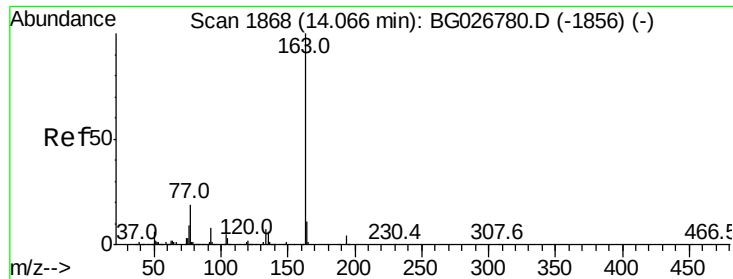

#44

Dimethylphthalate

Concen: 6.24 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. 0.00 min

Lab File: BG026785.D

Acq: 30 Apr 2017 22:55

Instrument :

BNA_G

ClientSampleId :

JHT60


Tot Ion:163 Resp: 243631

Ion Ratio Lower Upper

163 100

194 3.3 3.4 5.0#

164 10.0 9.0 13.4

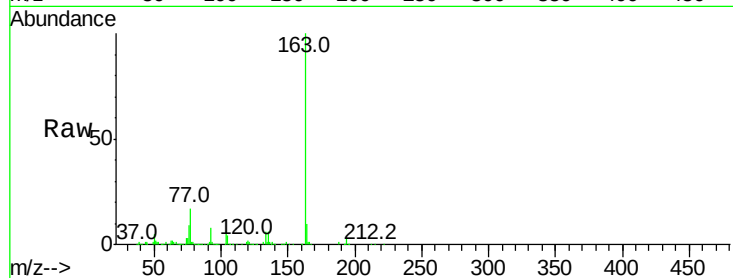

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

