

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026788.D
 Acq On : 1 May 2017 00:52
 Operator : SJ/MA
 Sample : I2846-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT85

Quant Time: May 01 05:03:36 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	162279	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	814268	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	474124	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	934652	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	859052	20.00	ng/ul	0.00
83) Perylene-d12	24.75	264	879332	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.42	96	21184	5.88	ng/uL	0.00
5) Phenol-d5	7.18	99	459043	31.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	273627	32.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	371993	30.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	402425	33.48	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	209244	30.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	235410	31.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	359120	30.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	580433	36.87	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1178527	30.88	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1514877	31.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.83	143	209211	30.42	ng/ul	0.00
57) Fluorene-d10	15.61	176	1023020	30.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	159802	28.16	ng/ul	0.00
70) Anthracene-d10	17.45	188	1423572	31.38	ng/ul	0.00
76) Pyrene-d10	19.73	212	1366260	30.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1328819	31.96	ng/ul	0.00


Target Compounds						Ovalue
6) Phenol	7.21	94	14816	1.01	ng/ul	94
44) Dimethylphthalate	14.06	163	325112	8.70	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026788.D
Acq On : 1 May 2017 00:52
Operator : SJ/MA
Sample : I2846-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHT85

Quant Time: May 01 05:03:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

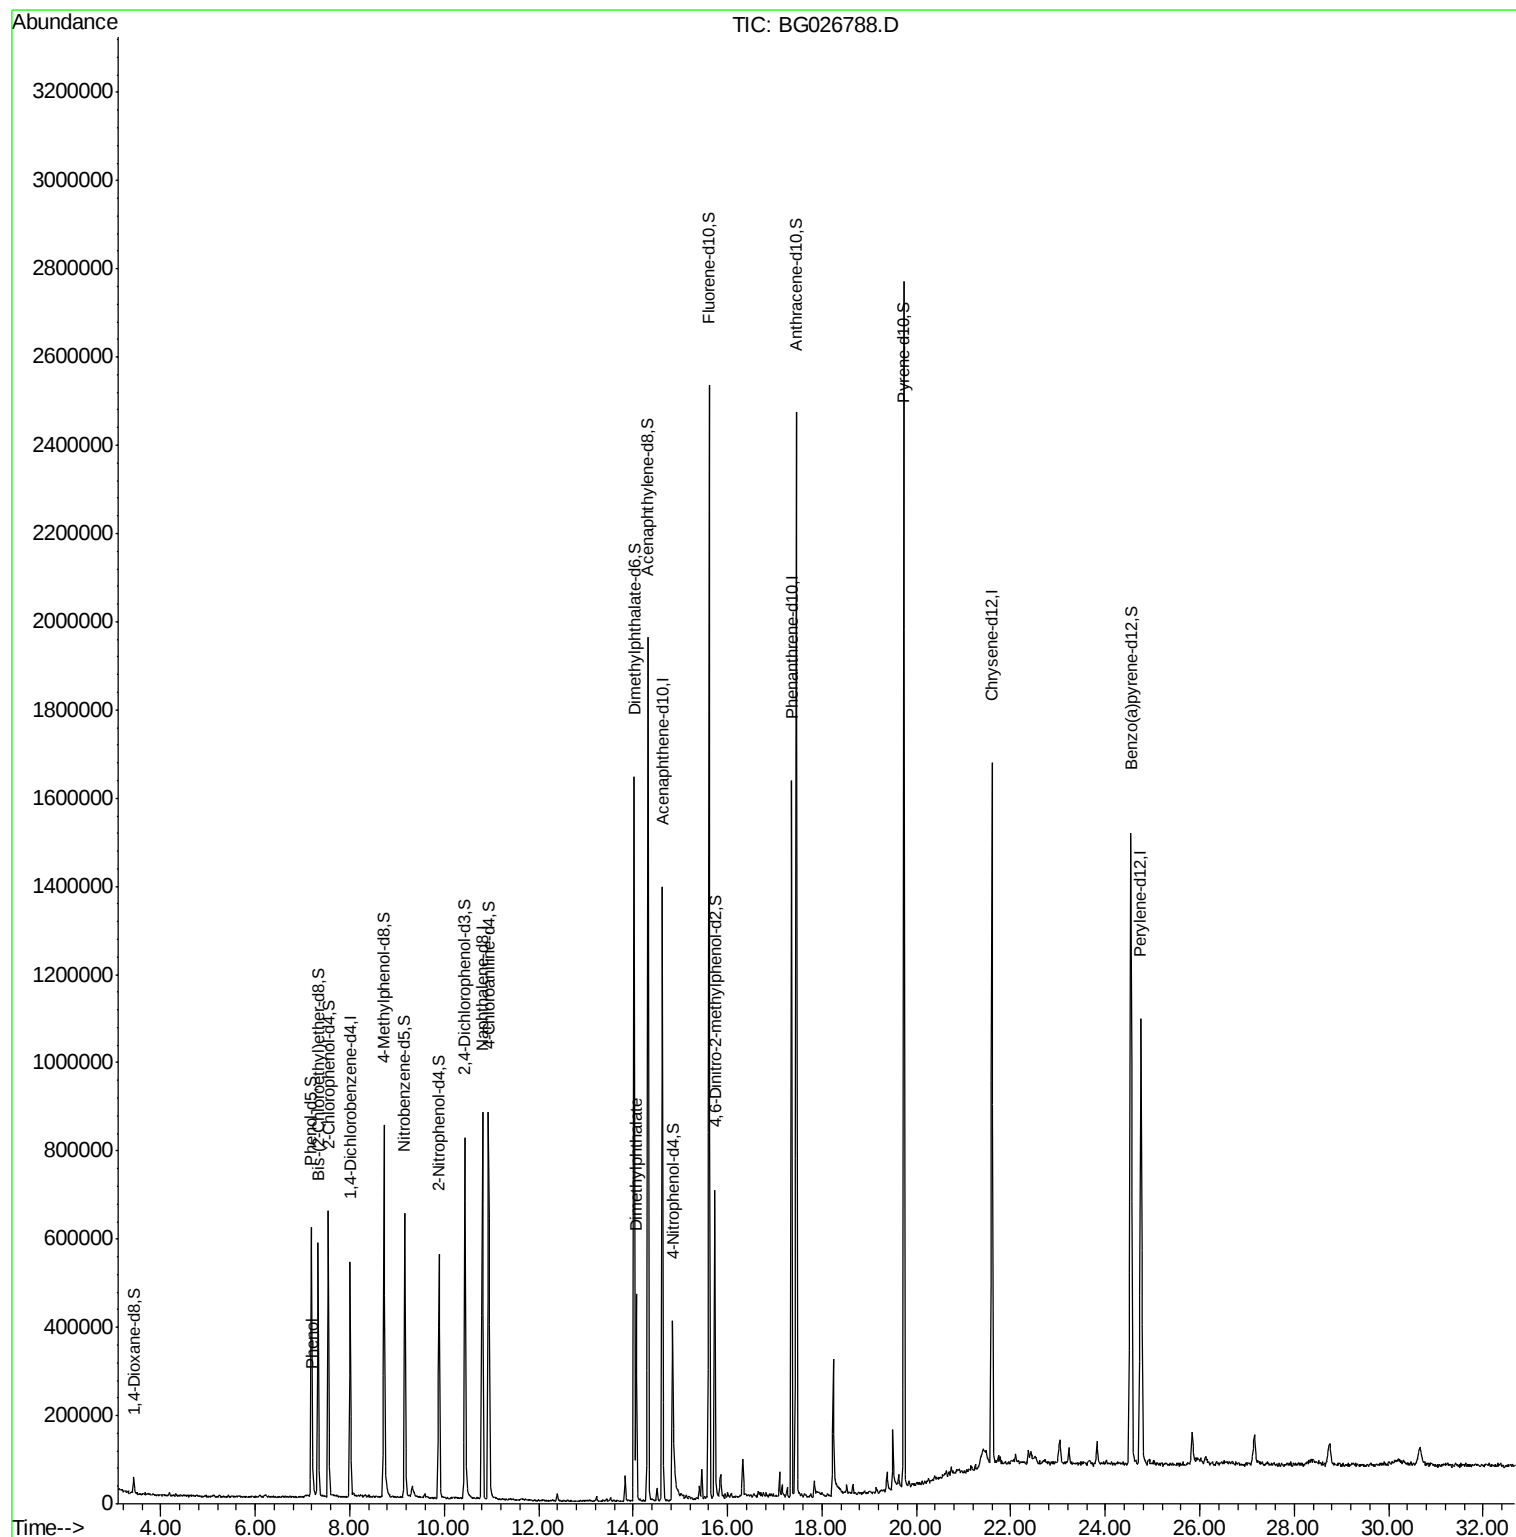

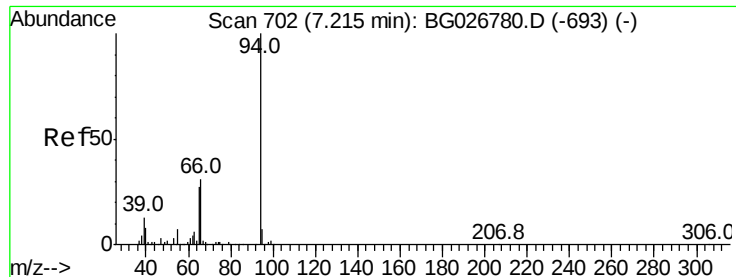

#6

Phenol

Concen: 1.01 ng/ul

RT: 7.21 min Scan# 702

Delta R.T. -0.00 min

Lab File: BG026788.D

Acq: 1 May 2017 00:52

Instrument :

BNA_G

ClientSampleId :

JHT85


Tot Ion: 94 Resp: 14816

Ion Ratio Lower Upper




94 100

65 34.3 26.8 40.2

66 49.5 44.4 66.6

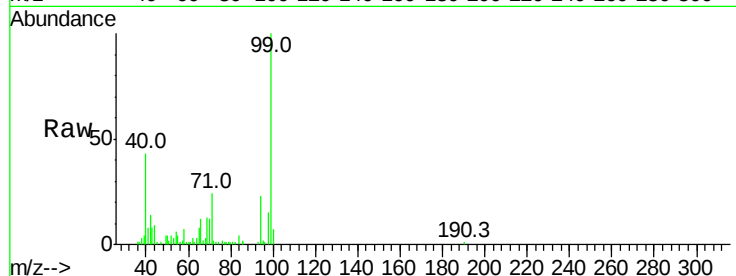

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

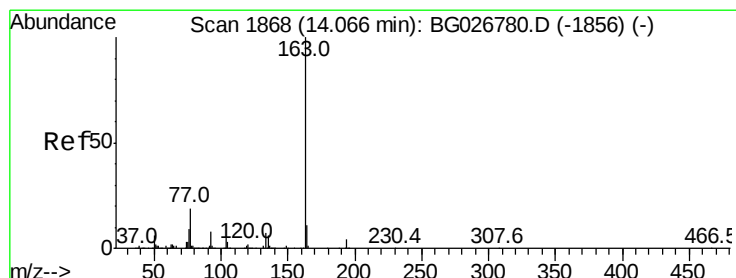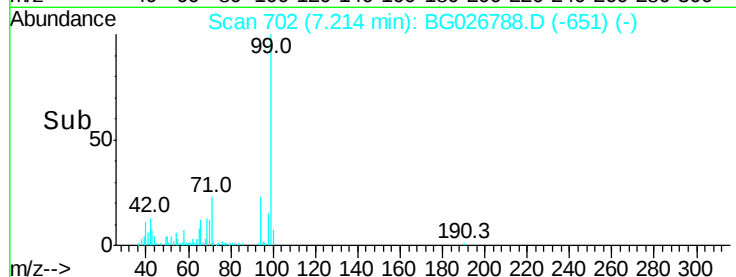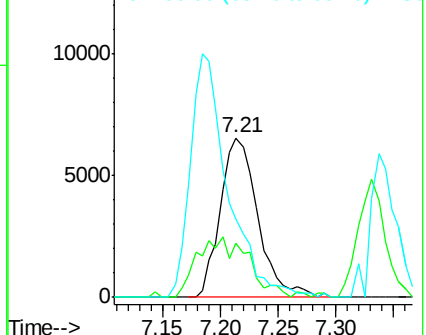

#44

Dimethylphthalate

Concen: 8.70 ng/ul

RT: 14.06 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BG026788.D

Acq: 1 May 2017 00:52


Tgt Ion:163 Resp: 325112

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.5 9.0 13.4

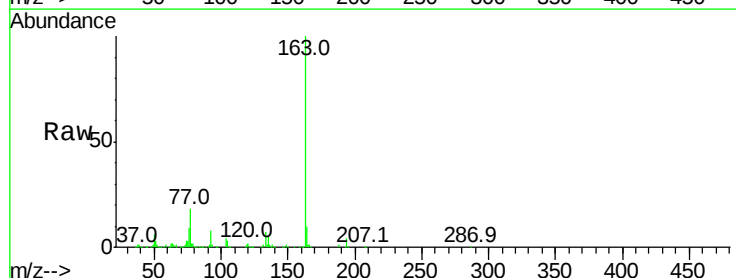

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

