

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026791.D
 Acq On : 1 May 2017 2:49
 Operator : SJ/MA
 Sample : I2846-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHSR7

Quant Time: May 01 05:03:58 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	187667	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	940970	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	536343	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	1048394	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	948791	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	976927	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	24947	5.99	ng/uL	0.00
5) Phenol-d5	7.18	99	594166	35.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	349927	35.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	481735	33.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	513424	36.93	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	268310	34.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	301308	35.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	460142	33.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	704690	38.73	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1451248	33.62	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1857826	34.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.83	143	267635	34.40	ng/ul	0.00
57) Fluorene-d10	15.61	176	1260518	33.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	210751	33.10	ng/ul	0.00
70) Anthracene-d10	17.45	188	1726928	33.94	ng/ul	0.00
76) Pyrene-d10	19.73	212	1669393	33.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1627257	35.23	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.06	163	355433	8.41 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026791.D
Acq On : 1 May 2017 2:49
Operator : SJ/MA
Sample : I2846-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHSR7

Quant Time: May 01 05:03:58 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

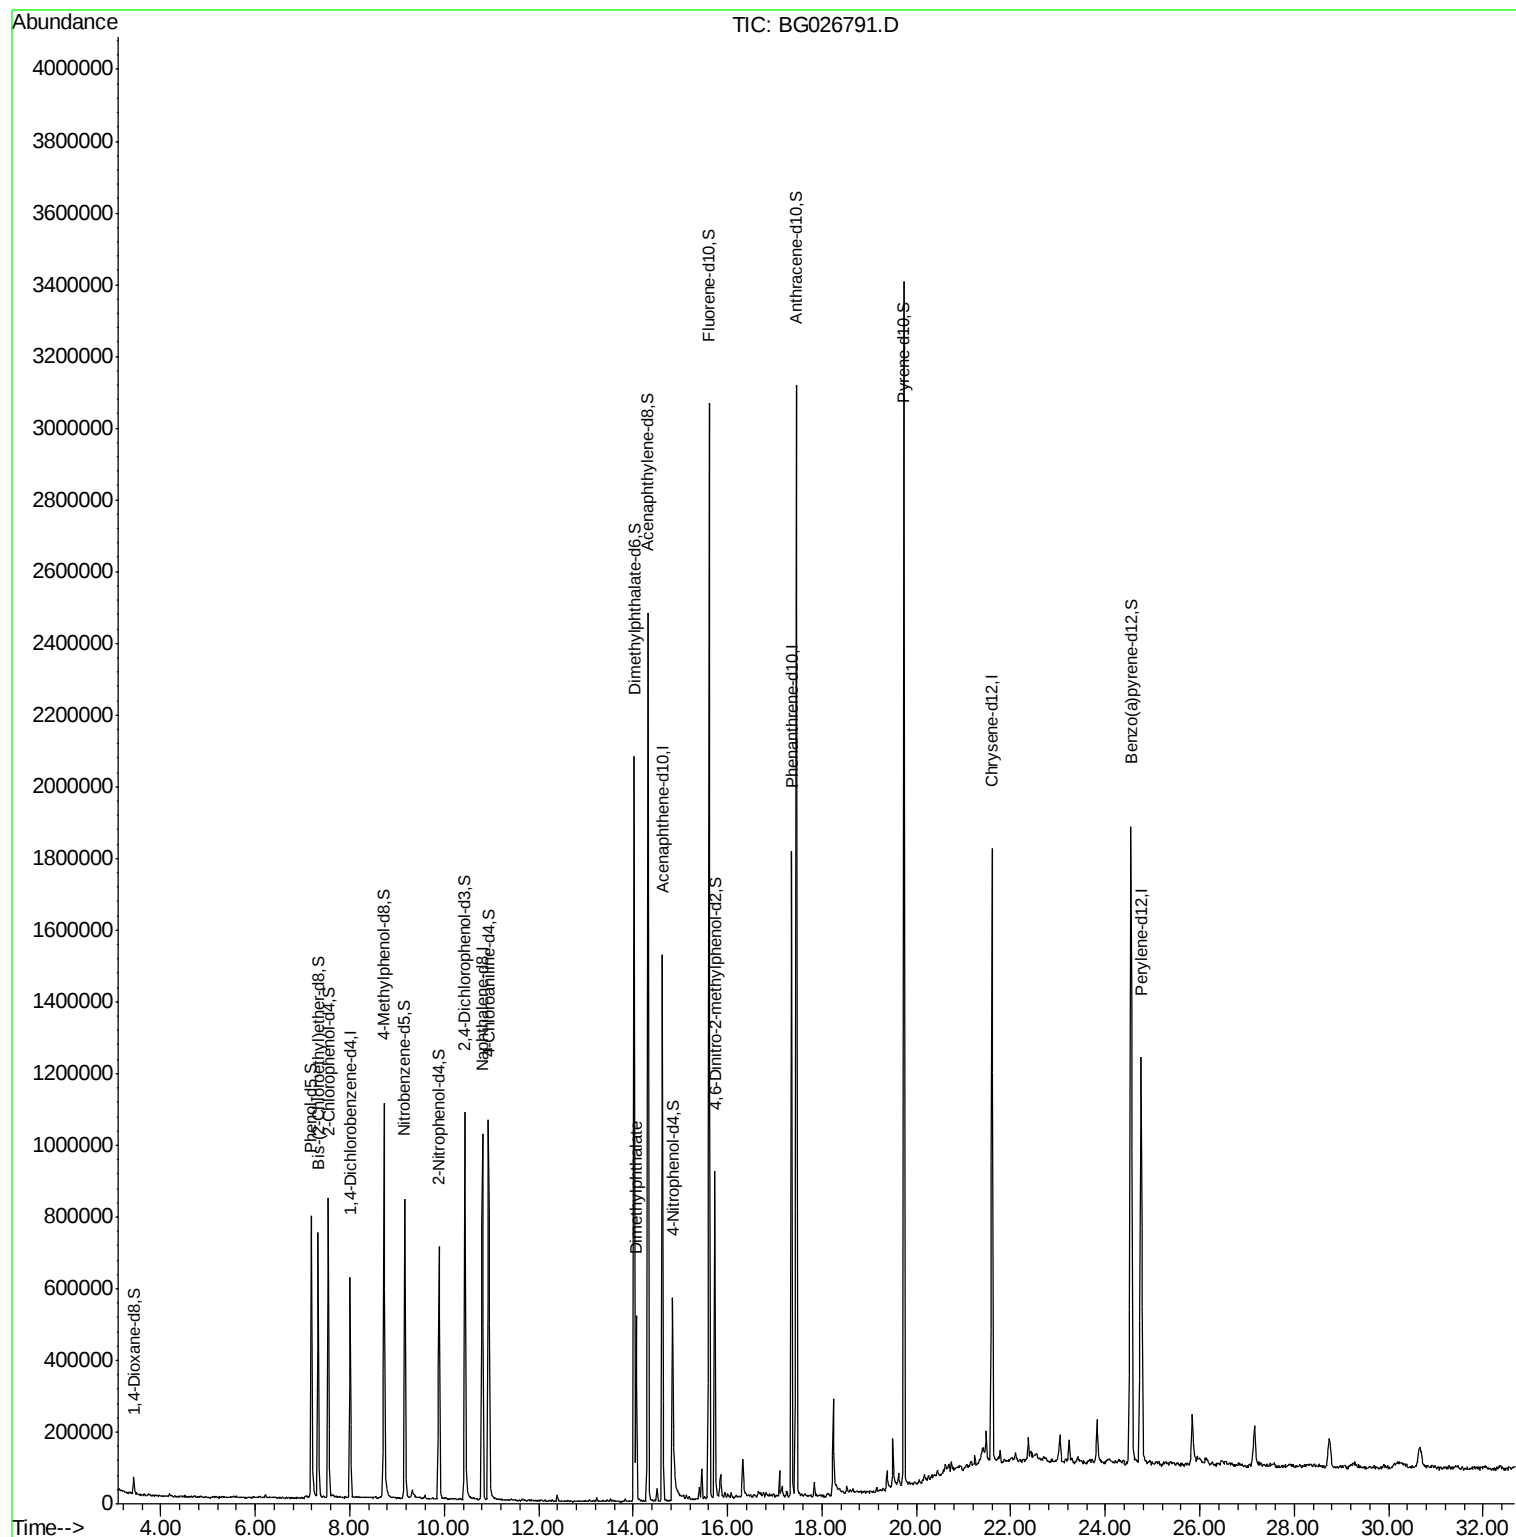

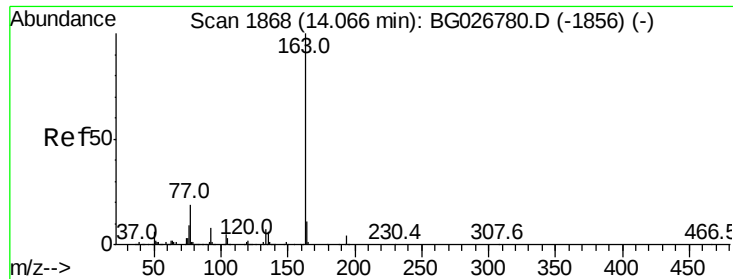

#44

Dimethylphthalate

Concen: 8.41 ng/ul

RT: 14.06 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BG026791.D

Acq: 1 May 2017 2:49

Instrument :

BNA_G

ClientSampleId :

JHSR7


Tot Ion:163 Resp: 355433

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.5 9.0 13.4

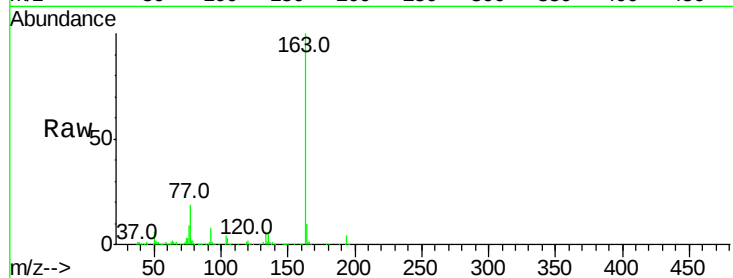

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

