

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026793.D
 Acq On : 1 May 2017 4:07
 Operator : SJ/MA
 Sample : I2846-16
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHSZ8

Quant Time: May 01 05:04:10 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	172146	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	869679	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	503957	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	970691	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	884377	20.00	ng/ul	0.00
83) Perylene-d12	24.75	264	918594	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	23740	6.21	ng/uL	0.00
5) Phenol-d5	7.19	99	540068	35.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	316358	35.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	435075	33.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	468974	36.78	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	245058	33.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	274772	34.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	420230	33.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	676364	40.22	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1334167	32.89	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1714951	33.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	228097	31.20	ng/ul	0.00
57) Fluorene-d10	15.61	176	1160607	32.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	182217	30.91	ng/ul	0.00
70) Anthracene-d10	17.45	188	1600922	33.98	ng/ul	0.00
76) Pyrene-d10	19.73	212	1538430	32.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1491663	34.35	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.07	163	331195	8.34	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026793.D
Acq On : 1 May 2017 4:07
Operator : SJ/MA
Sample : I2846-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHSZ8

Quant Time: May 01 05:04:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

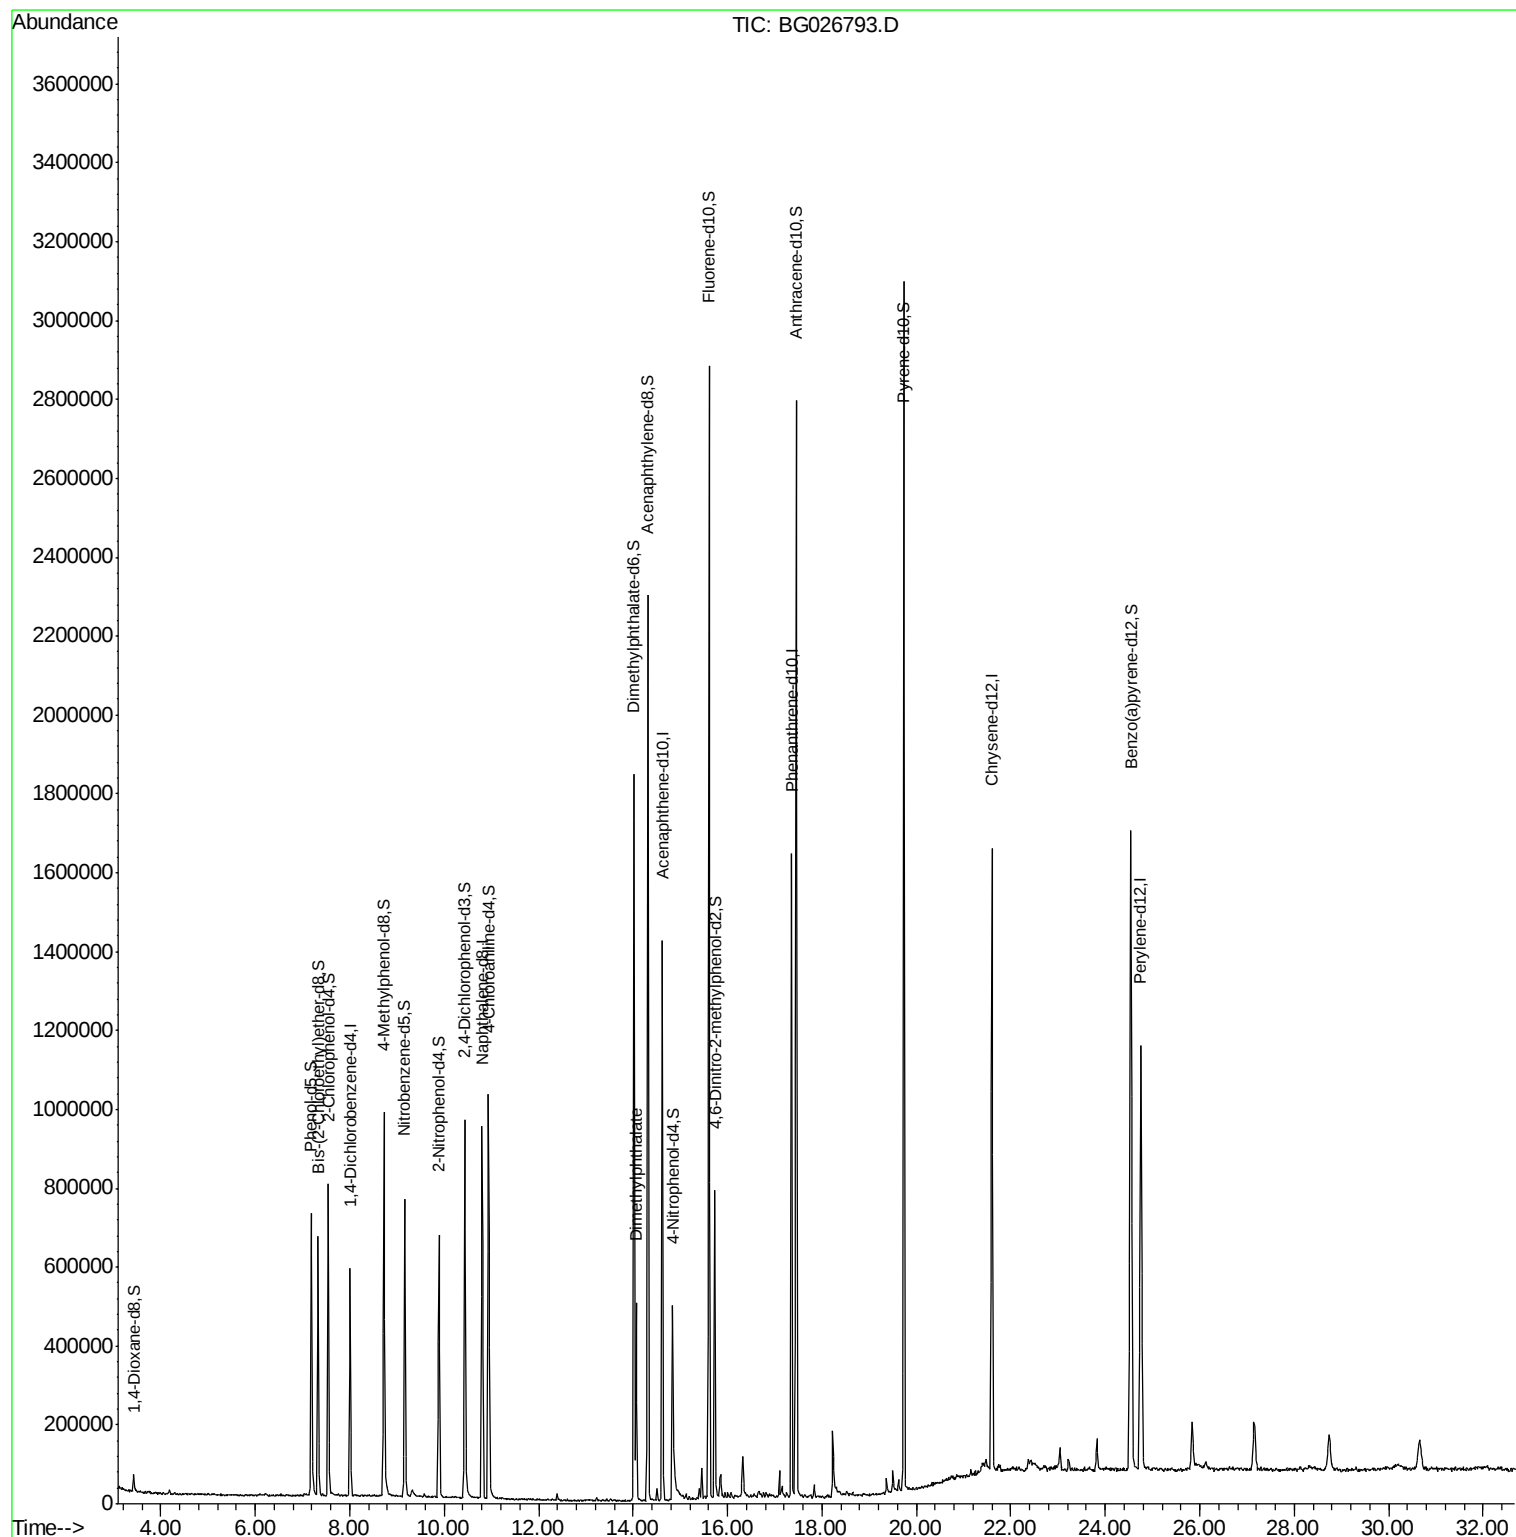

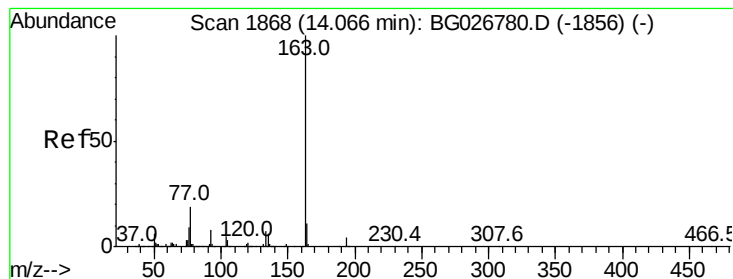

#44

Dimethylphthalate

Concen: 8.34 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. 0.00 min

Lab File: BG026793.D

Acq: 1 May 2017 4:07

Instrument :

BNA_G

ClientSampleId :

JHSZ8


Tot Ion:163 Resp: 331195

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.2 9.0 13.4

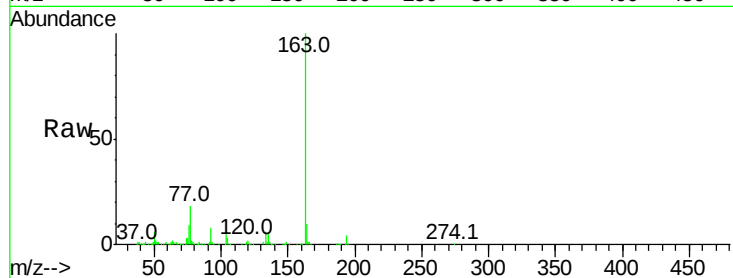

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

