

Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
 Data File : BG026794.D
 Acq On : 1 May 2017 4:47
 Operator : SJ/MA
 Sample : I2846-18
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHT00

Manual Integrations
 APPROVED

mohammad
 5/1/2017 6:52:39 PM

Quant Time: May 01 07:04:22 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 05:02:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	182751	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	941509	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	540982	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	1038337	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	950716	20.00	ng/ul	0.00
83) Perylene-d12	24.75	264	977063	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	25261	6.23	ng/uL	0.00
5) Phenol-d5	7.19	99	581638	35.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	331543m	34.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	461414	33.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	499051	36.87	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	255833	32.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	289192	33.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	450366	33.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	722787	39.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1428354	32.80	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1837528	33.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	264416	33.69	ng/ul	0.00
57) Fluorene-d10	15.61	176	1242850	32.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	197406	31.31	ng/ul	0.00
70) Anthracene-d10	17.45	188	1711992	33.97	ng/ul	0.00
76) Pyrene-d10	19.73	212	1623246	32.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1607605	34.80	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.07	163	469416	11.01 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG043017\
Data File : BG026794.D
Acq On : 1 May 2017 4:47
Operator : SJ/MA
Sample : I2846-18
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHT00

Quant Time: May 01 07:04:22 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/1/2017 6:52:39 PM

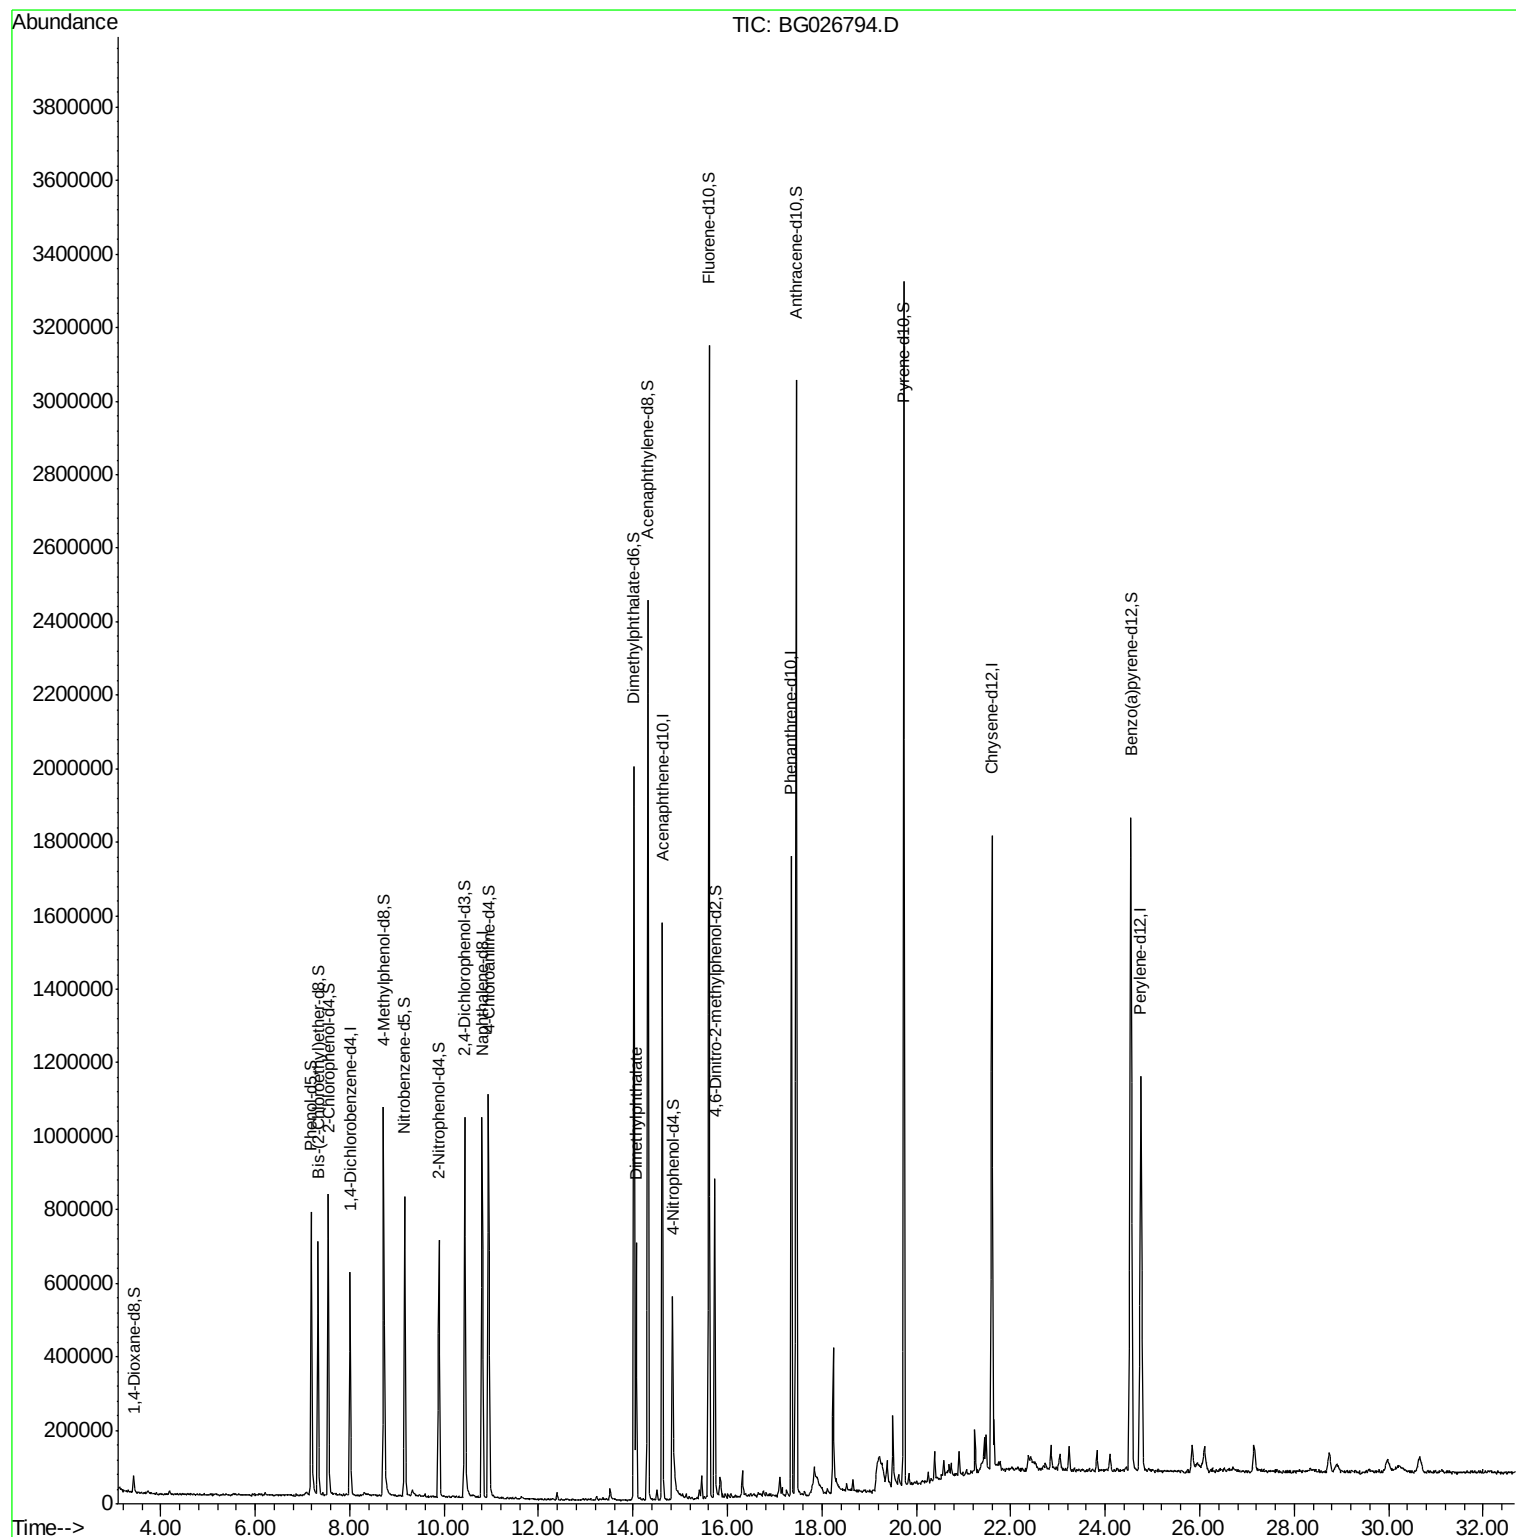

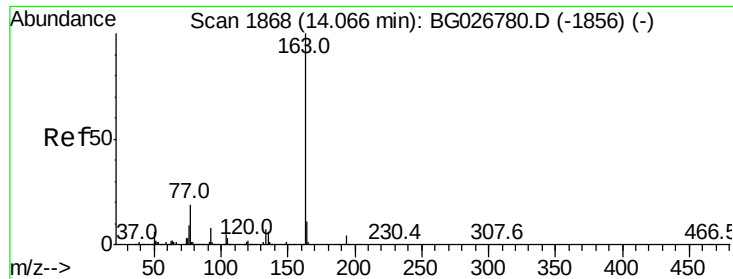

#44

Dimethylphthalate

Concen: 11.01 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. 0.00 min

Lab File: BG026794.D

Acq: 1 May 2017 4:47

Instrument :

BNA_G

ClientSampleId :

JHT00

Tot Ion:	163	Resp:	469416
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.4	5.0
164	10.1	9.0	13.4

Manual Integrations
APPROVED

mohammad
5/1/2017 6:52:39 PM

