


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG043019\
 Data File : BG040671.D
 Acq On : 30 Apr 2019 14:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

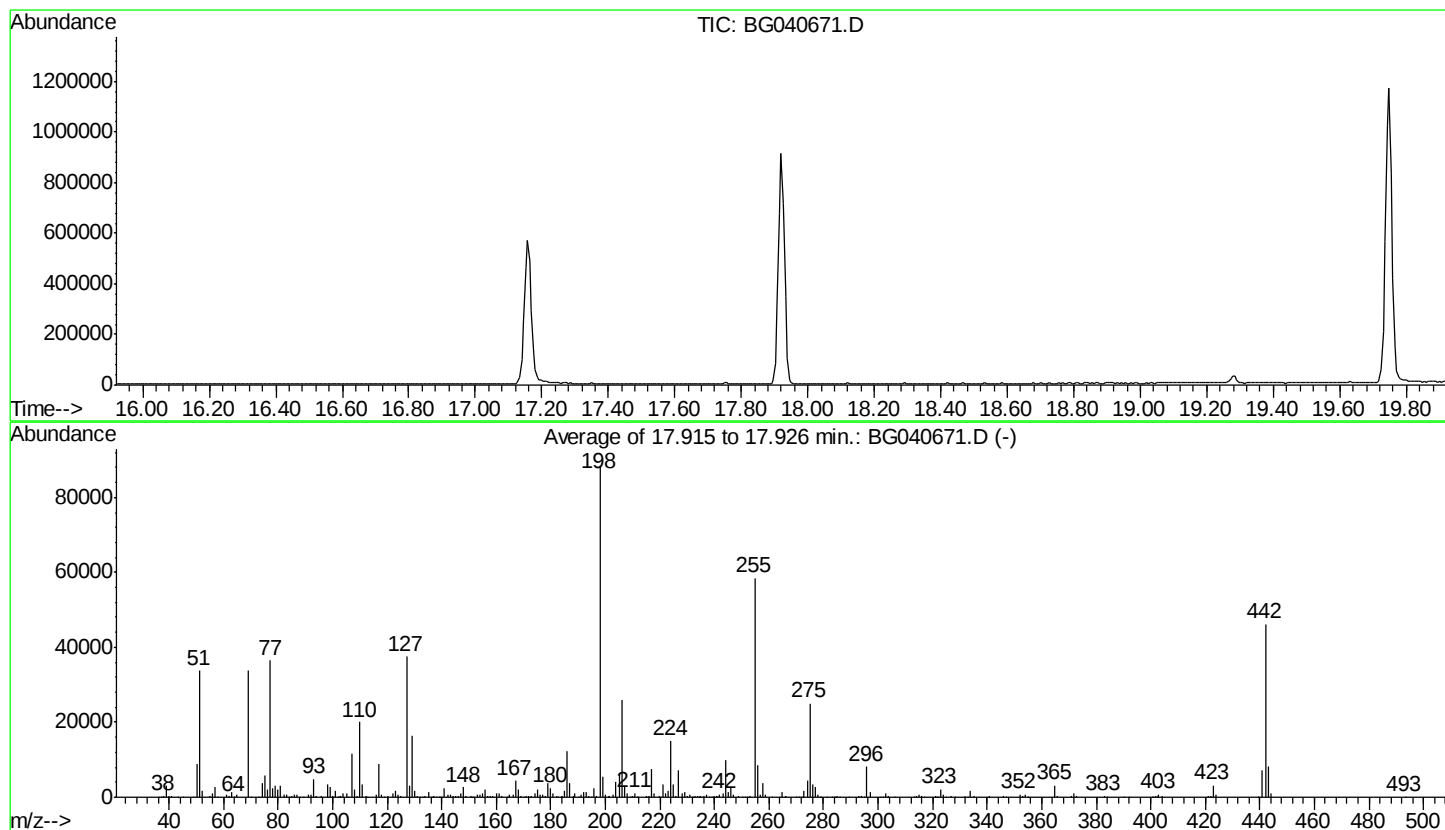

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	33701	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	33680	PASS
70	69	0.00	2	0.4	133	PASS
127	198	10	80	42.3	37426	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88477	PASS
199	198	5	9	6.3	5555	PASS
275	198	10	60	28.4	25098	PASS
365	198	1	100	3.6	3197	PASS
441	198	0.01	100	8.3	7309	PASS
442	198	50	100	52.2	46160	PASS
443	442	15	24	17.8	8206	PASS