


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG043024\
Data File : BG061057.D
Acq On : 30 Apr 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

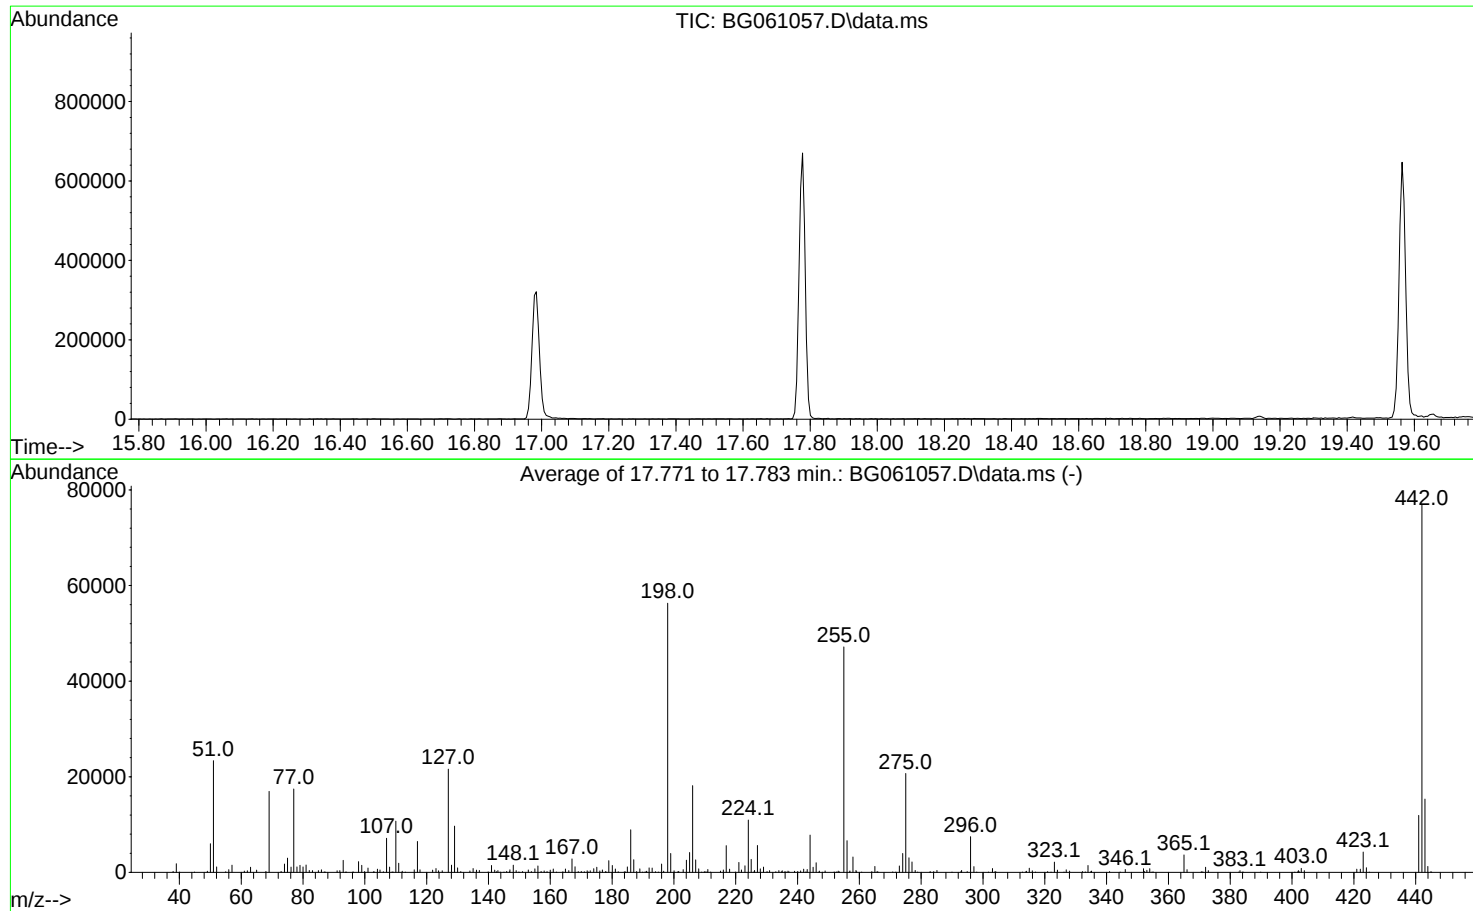




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	23349	PASS
68	69	0.00	2	1.2	198	PASS
69	198	0.00	100	30.1	16925	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.3	21591	PASS
197	198	0.00	2	0.4	228	PASS
198	198	100	100	100.0	56315	PASS
199	198	5	9	7.0	3945	PASS
275	198	10	60	36.7	20691	PASS
365	198	1	100	6.5	3653	PASS
441	198	0.01	100	21.2	11919	PASS
442	442	50	100	100.0	76955	PASS
443	442	15	24	19.9	15323	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG043024\
Data File : BG061057.D
Acq On : 30 Apr 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 03 13:27:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

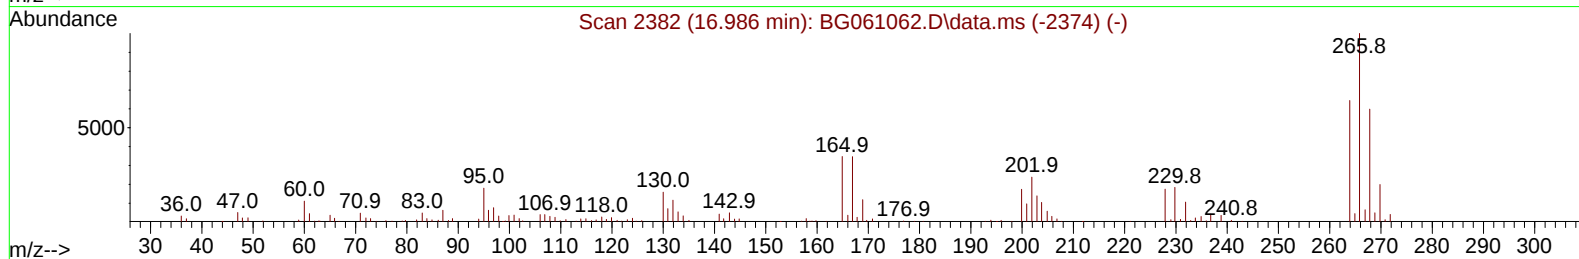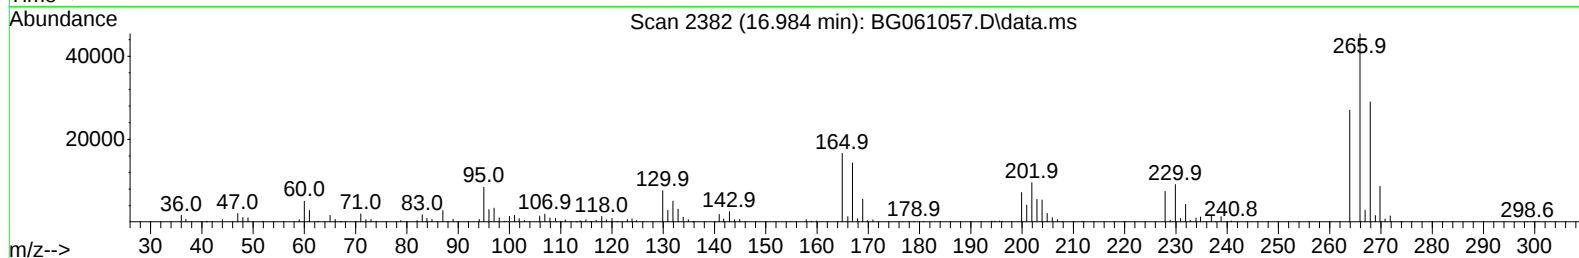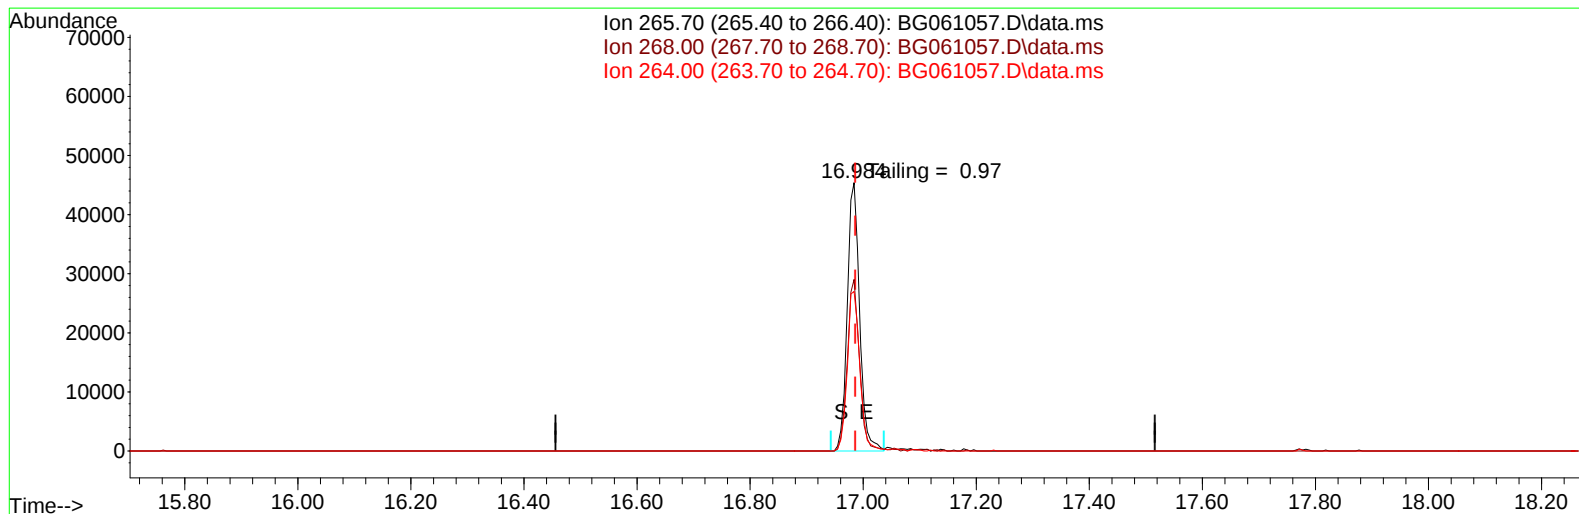

TIC: BG061057.D\data.ms

(70) Pentachlorophenol (C)

16.984min (-0.002) 44271.60 ng




response 68990

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	63.91
264.00	64.40	59.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG043024\
Data File : BG061057.D
Acq On : 30 Apr 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 03 13:27:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

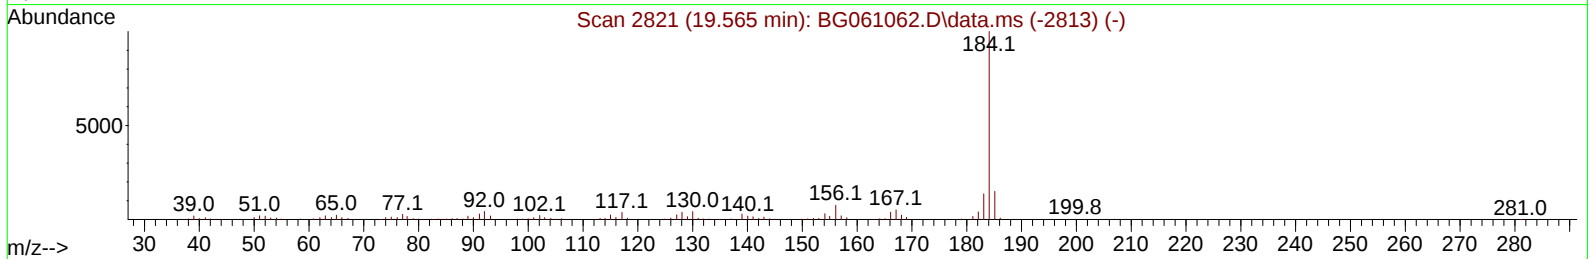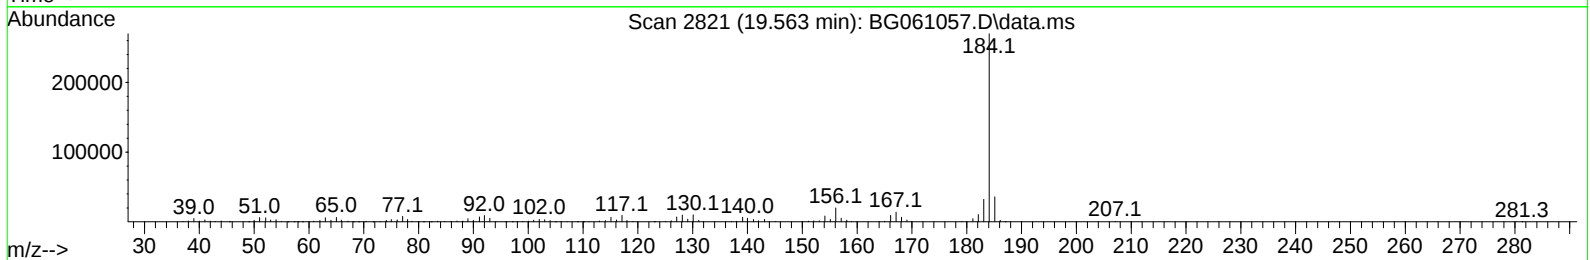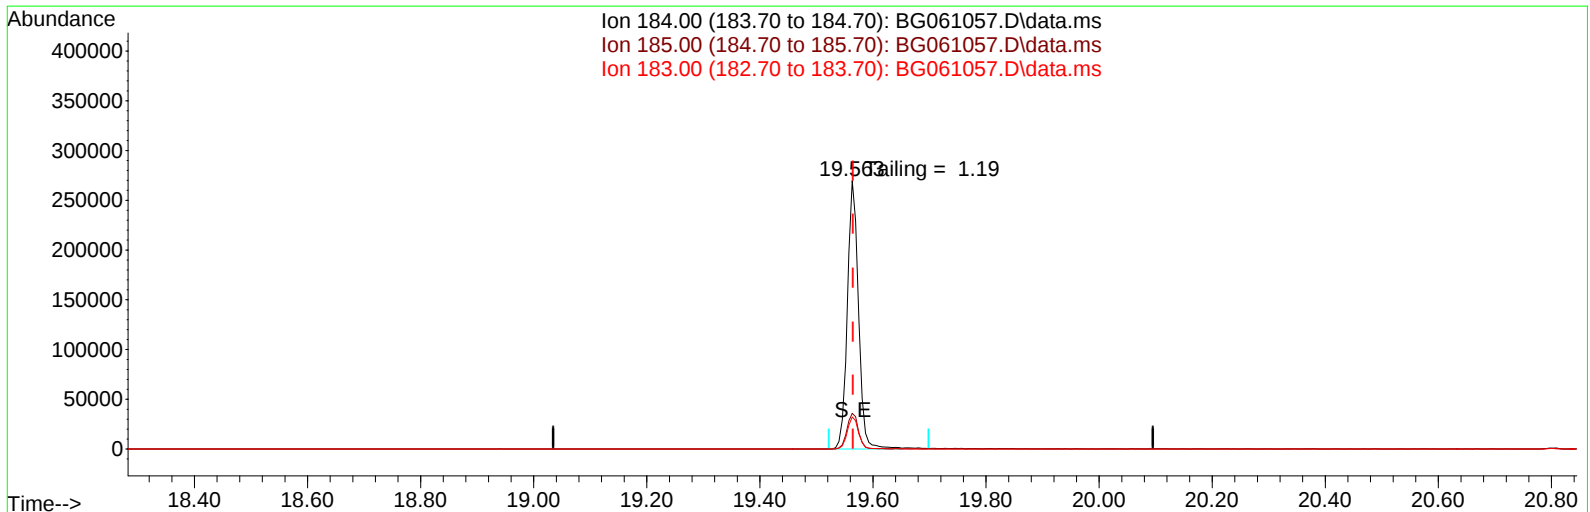

TIC: BG061057.D\data.ms

(77) Benzidine

19.563min (-0.002) 285195.57 ng m

response 368805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.32
183.00	13.60	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2024	BNA_G	<u>BG061057.D</u>
Compound Name	Response	Retention Time
DDT	255420	20.803
DDD	2843	20.409
DDE	0	19.852
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2843	258263	1.10

Instrument :
BNA_G
ClientSampleId :
DFTPP